

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0102320\
 Data File : P0072732.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 23 Oct 2020 19:03
 Operator : DD\AJ
 Sample : L4486-07
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 1836

Manual Integrations
 APPROVED

mohammad
 10/26/2020 5:06:42 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 24 05:49:02 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101420.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 14 17:47:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.317	3.500	1310499	694097	15.451m	16.478
2) SA Decachlor...	9.918	8.665	938463	452720	8.508	8.758

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102320\
Data File : PO072732.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Oct 2020 19:03
Operator : DD\AJ
Sample : L4486-07
Misc :
ALS Vial : 29 Sample Multiplier: 1


Instrument :
ECD_O
ClientSampleId :
1836


Manual Integrations
APPROVED

mohammad
10/26/2020 5:06:42 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 24 05:49:02 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101420.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 14 17:47:24 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

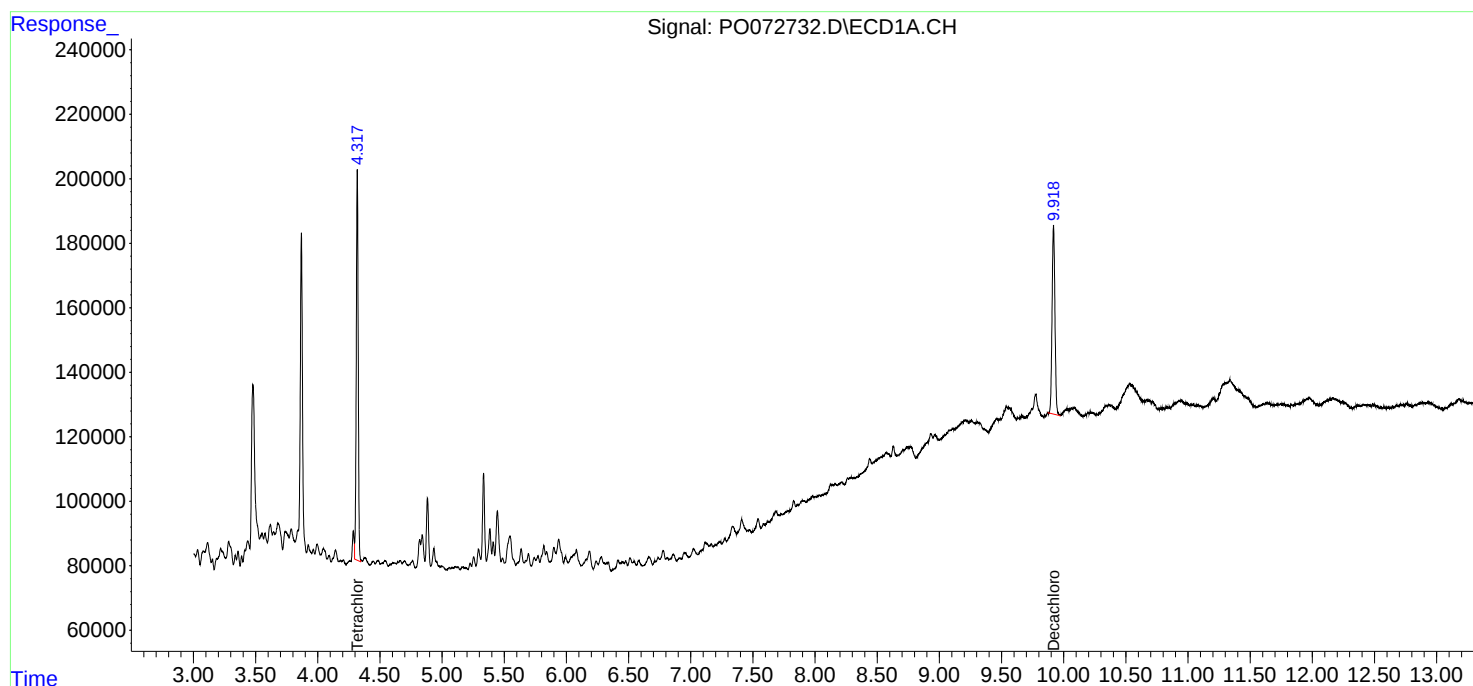

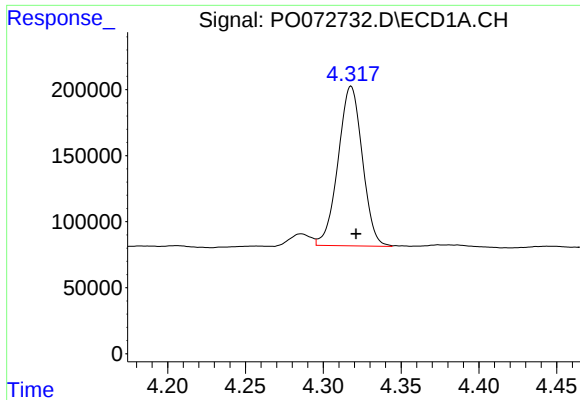


#1 Tetrachloro-m-xylene

R.T.: 4.317 min
Delta R.T.: -0.003 min
Response: 1310499
Conc: 15.45 ng/ml m

Instrument :
ECD_O
ClientSampleId :
1836


Manual Integrations
APPROVED

mohammad
10/26/2020 5:06:42 PM

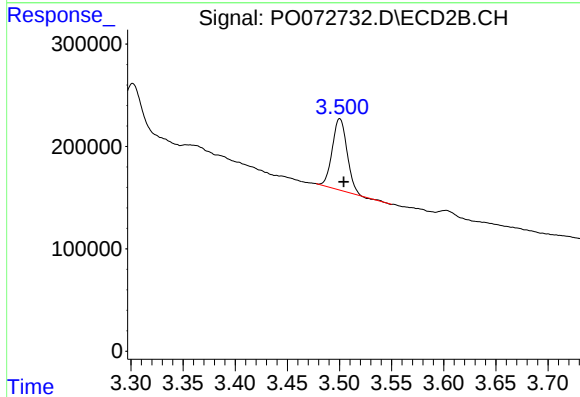


#1 Tetrachloro-m-xylene

R.T.: 3.500 min
Delta R.T.: -0.004 min
Response: 694097
Conc: 16.48 ng/ml

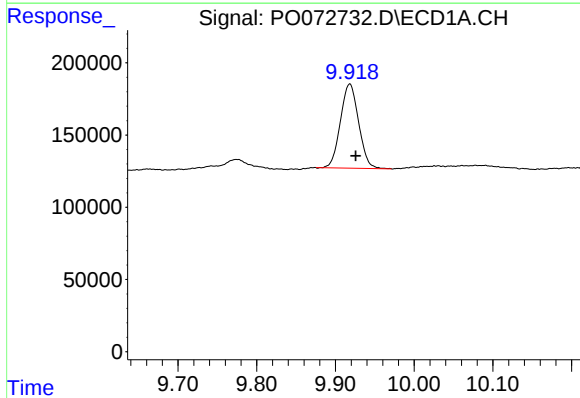

#2 Decachlorobiphenyl

R.T.: 9.918 min
Delta R.T.: -0.008 min
Response: 938463
Conc: 8.51 ng/ml

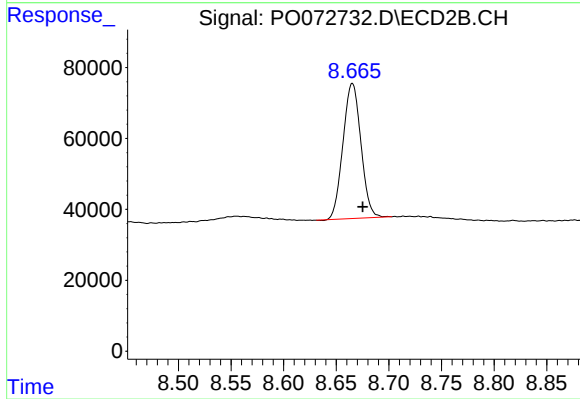

#2 Decachlorobiphenyl

R.T.: 8.665 min
Delta R.T.: -0.010 min
Response: 452720
Conc: 8.76 ng/ml