

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102320\
 Data File : PO072736.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 23 Oct 2020 20:11
 Operator : DD\AJ
 Sample : L4488-06
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 1576

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 24 05:50:32 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101420.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 14 17:47:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.319	3.501	802690	448797	9.464	10.655
2) SA Decachlor...	9.919	8.666	566593	282263	5.137	5.460

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102320\
Data File : PO072736.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Oct 2020 20:11
Operator : DD\AJ
Sample : L4488-06
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
1576

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 24 05:50:32 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101420.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 14 17:47:24 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

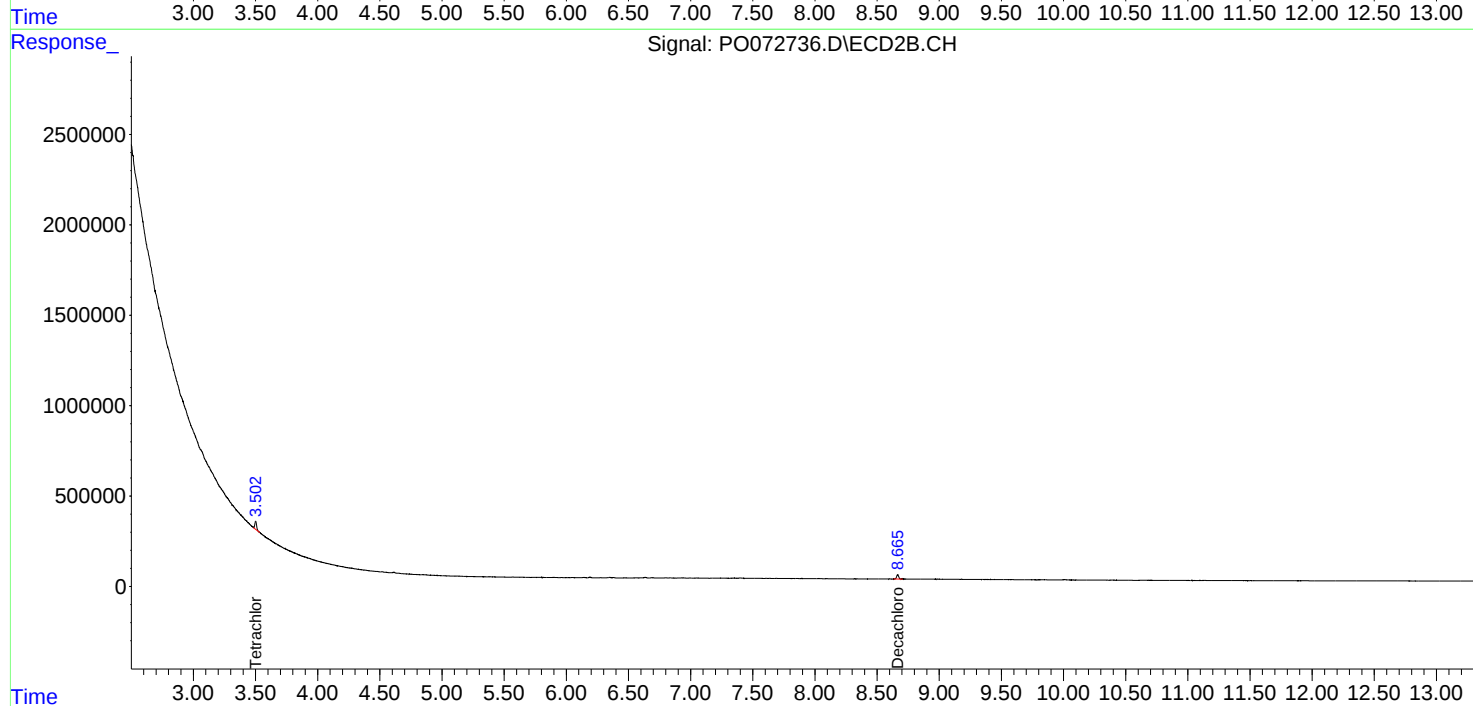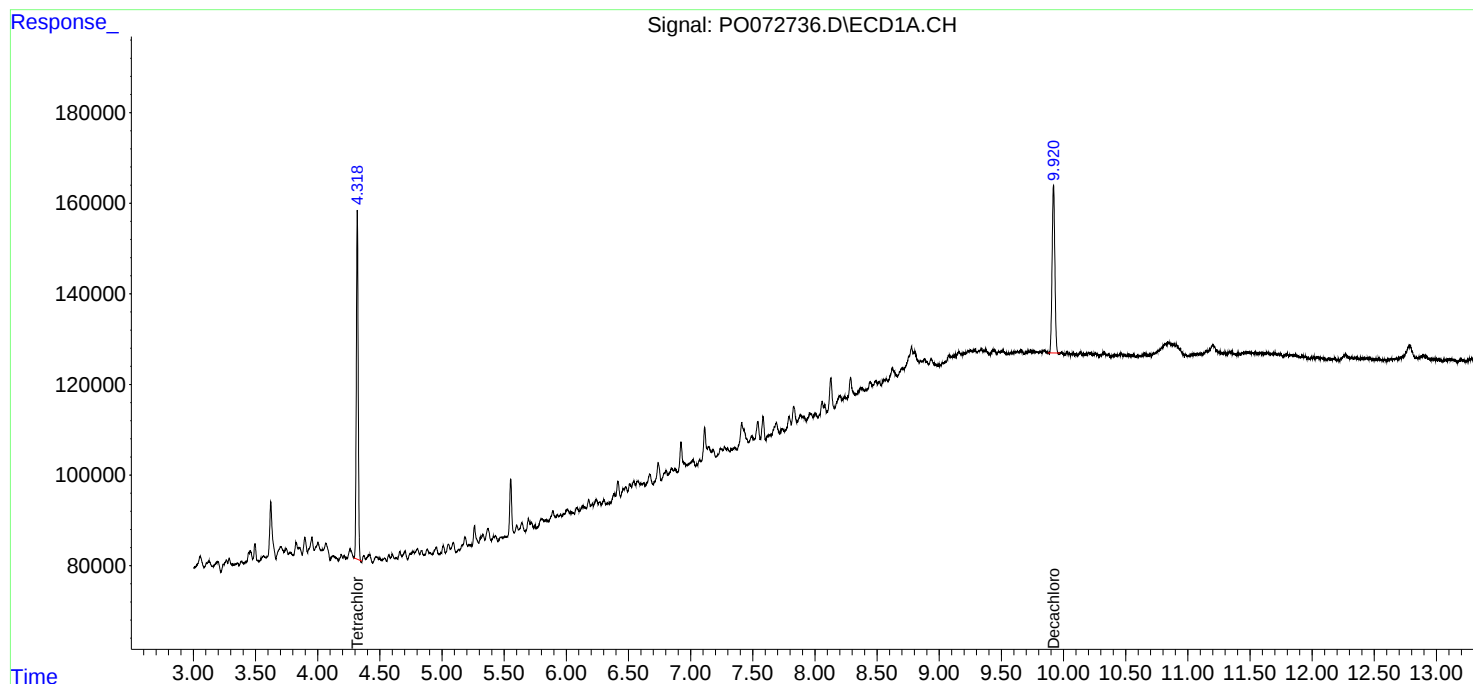


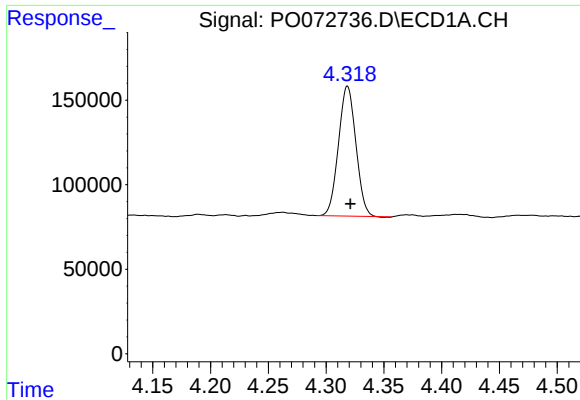

#1 Tetrachloro-m-xylene


R.T.: 4.319 min
Delta R.T.: -0.002 min
Response: 802690
Conc: 9.46 ng/ml

Instrument :
ECD_O
ClientSampleId :
1576

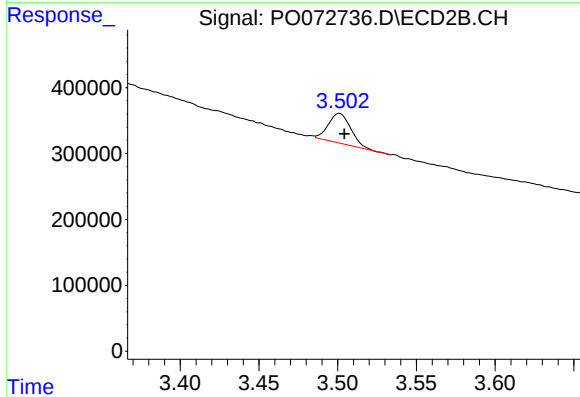


#1 Tetrachloro-m-xylene

R.T.: 3.501 min
Delta R.T.: -0.003 min
Response: 448797
Conc: 10.65 ng/ml

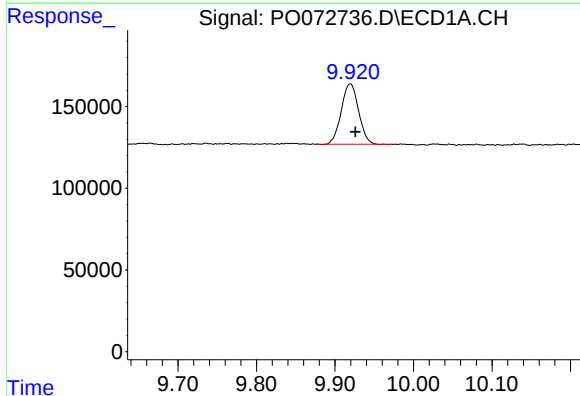

#2 Decachlorobiphenyl

R.T.: 9.919 min
Delta R.T.: -0.006 min
Response: 566593
Conc: 5.14 ng/ml

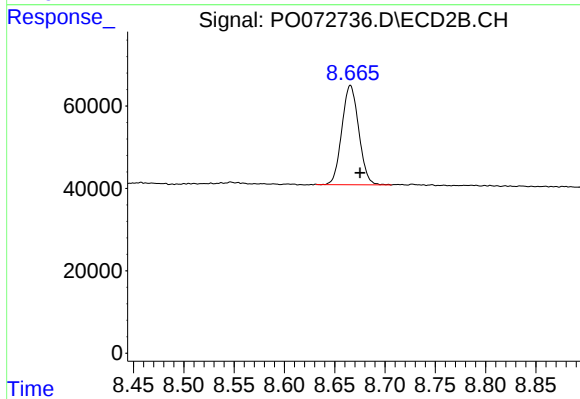

#2 Decachlorobiphenyl

R.T.: 8.666 min
Delta R.T.: -0.010 min
Response: 282263
Conc: 5.46 ng/ml