

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0102320\
 Data File : P0072739.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 23 Oct 2020 21:03
 Operator : DD\AJ
 Sample : L4496-01
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SA-01-102220

Manual Integrations
 APPROVED

mohammad
 10/26/2020 5:06:49 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 24 05:51:50 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101420.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 14 17:47:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.316	3.498	2217812	1013490	26.148m	24.061
2) SA Decachlor...	9.919	8.664	2121380	970241	19.232	18.769

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102320\
Data File : PO072739.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Oct 2020 21:03
Operator : DD\AJ
Sample : L4496-01
Misc :
ALS Vial : 34 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SA-01-102220


Manual Integrations
APPROVED

mohammad
10/26/2020 5:06:49 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 24 05:51:50 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101420.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 14 17:47:24 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

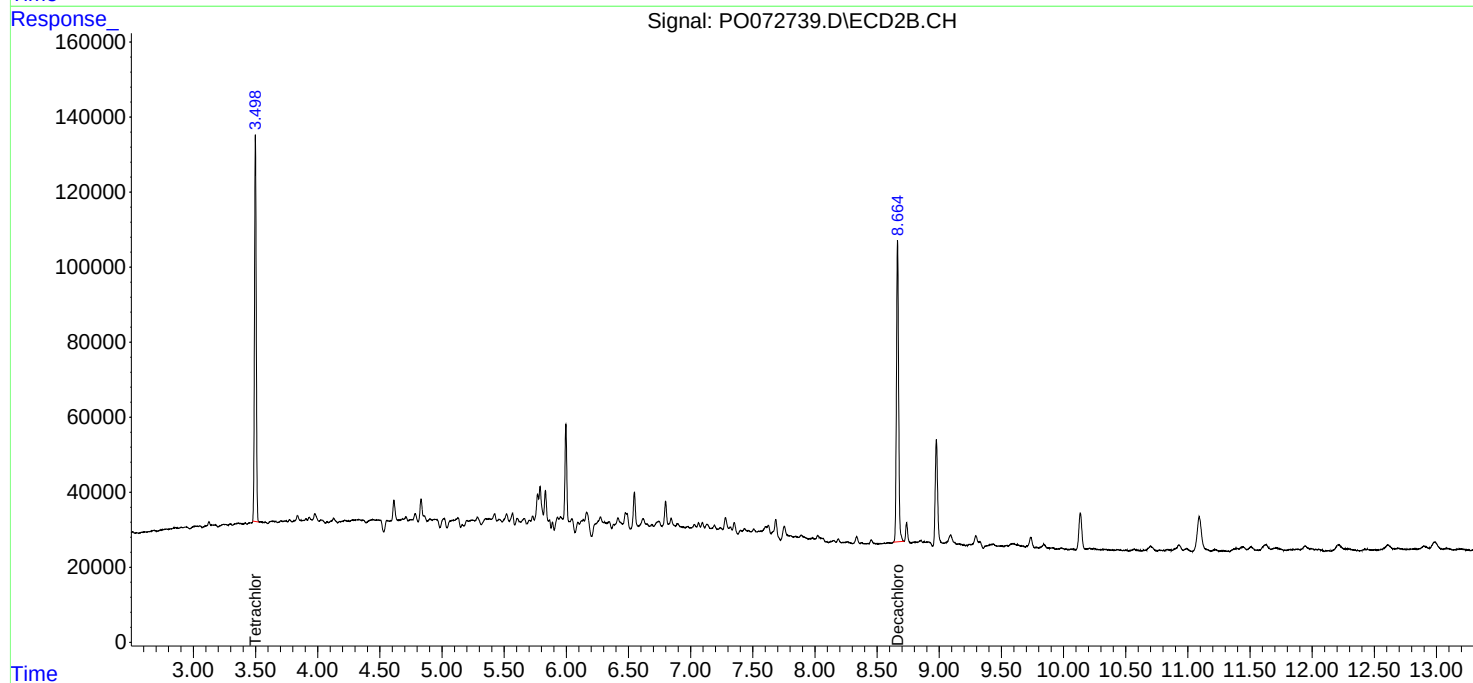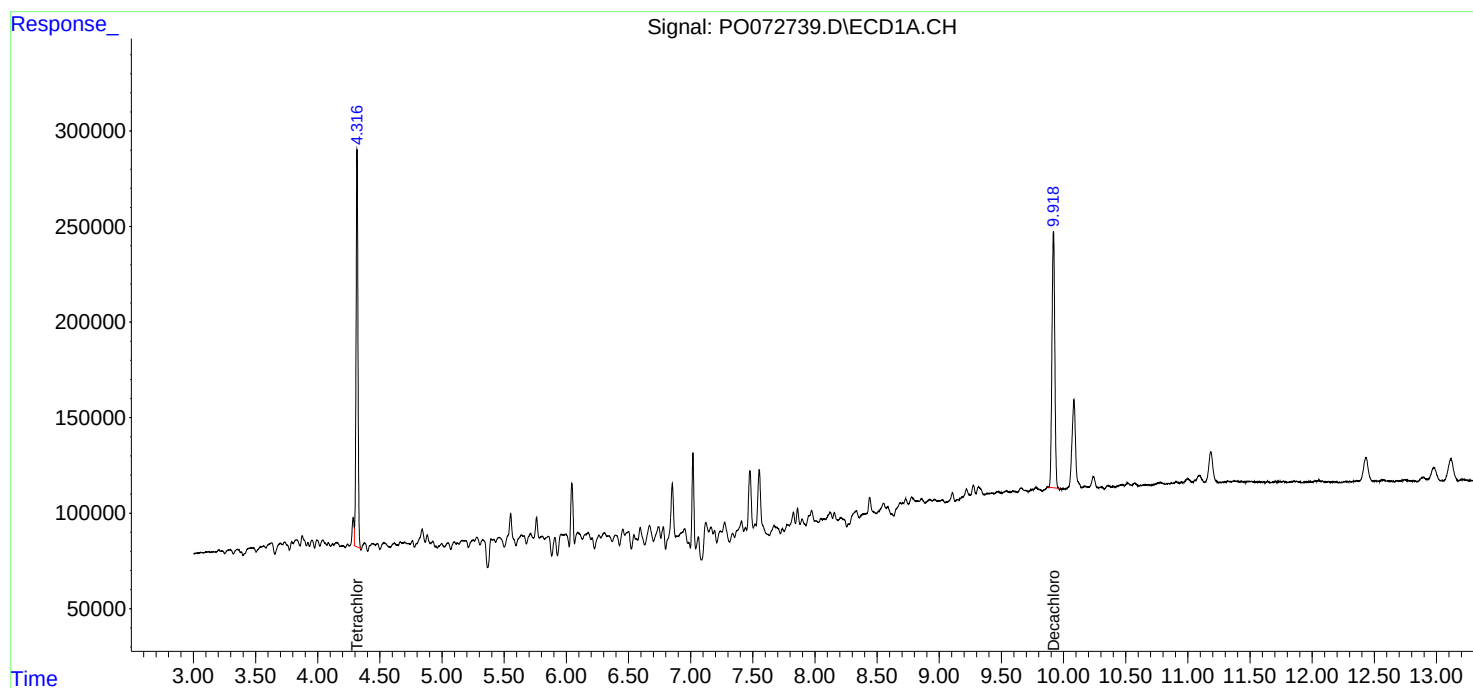

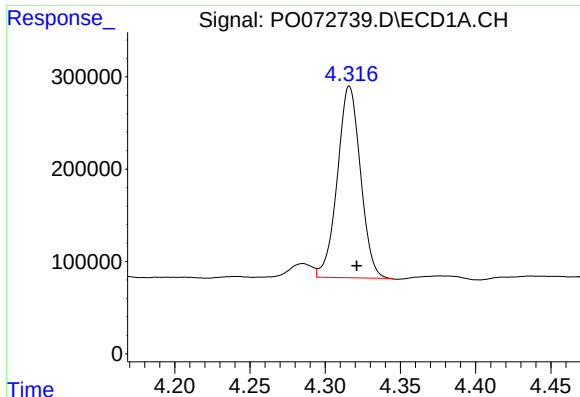


#1 Tetrachloro-m-xylene

R.T.: 4.316 min
Delta R.T.: -0.005 min
Response: 2217812
Conc: 26.15 ng/ml m

Instrument :
ECD_O
ClientSampleId :
SA-01-102220


Manual Integrations
APPROVED

mohammad
10/26/2020 5:06:49 PM

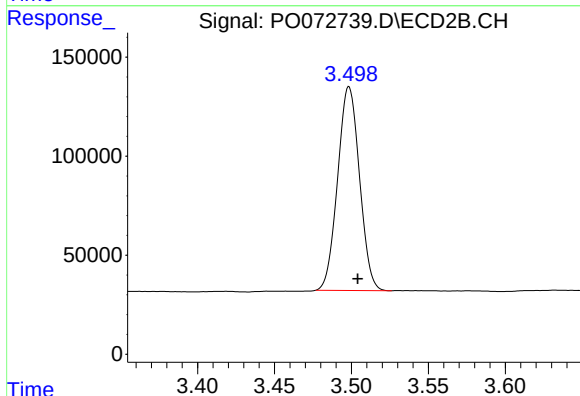


#1 Tetrachloro-m-xylene

R.T.: 3.498 min
Delta R.T.: -0.006 min
Response: 1013490
Conc: 24.06 ng/ml

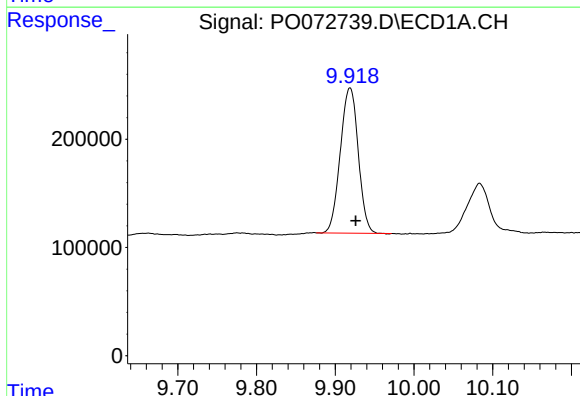

#2 Decachlorobiphenyl

R.T.: 9.919 min
Delta R.T.: -0.007 min
Response: 2121380
Conc: 19.23 ng/ml

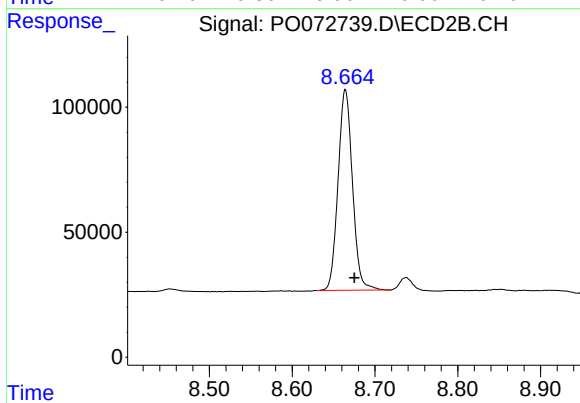

#2 Decachlorobiphenyl

R.T.: 8.664 min
Delta R.T.: -0.011 min
Response: 970241
Conc: 18.77 ng/ml