

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102320\
 Data File : PO072743.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 23 Oct 2020 22:11
 Operator : DD\AJ
 Sample : L4487-03 10X
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 D-89

Manual Integrations
 APPROVED

mohammad
 10/26/2020 5:07:02 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 24 05:53:26 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101420.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 14 17:47:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.316	3.498	165195	83915	1.948m	1.992
2) SA Decachlor...	9.919	8.666	178582	94860	1.619	1.835

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102320\
Data File : PO072743.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Oct 2020 22:11
Operator : DD\AJ
Sample : L4487-03 10X
Misc :
ALS Vial : 38 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
D-89


Manual Integrations
APPROVED

mohammad
10/26/2020 5:07:02 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 24 05:53:26 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101420.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 14 17:47:24 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

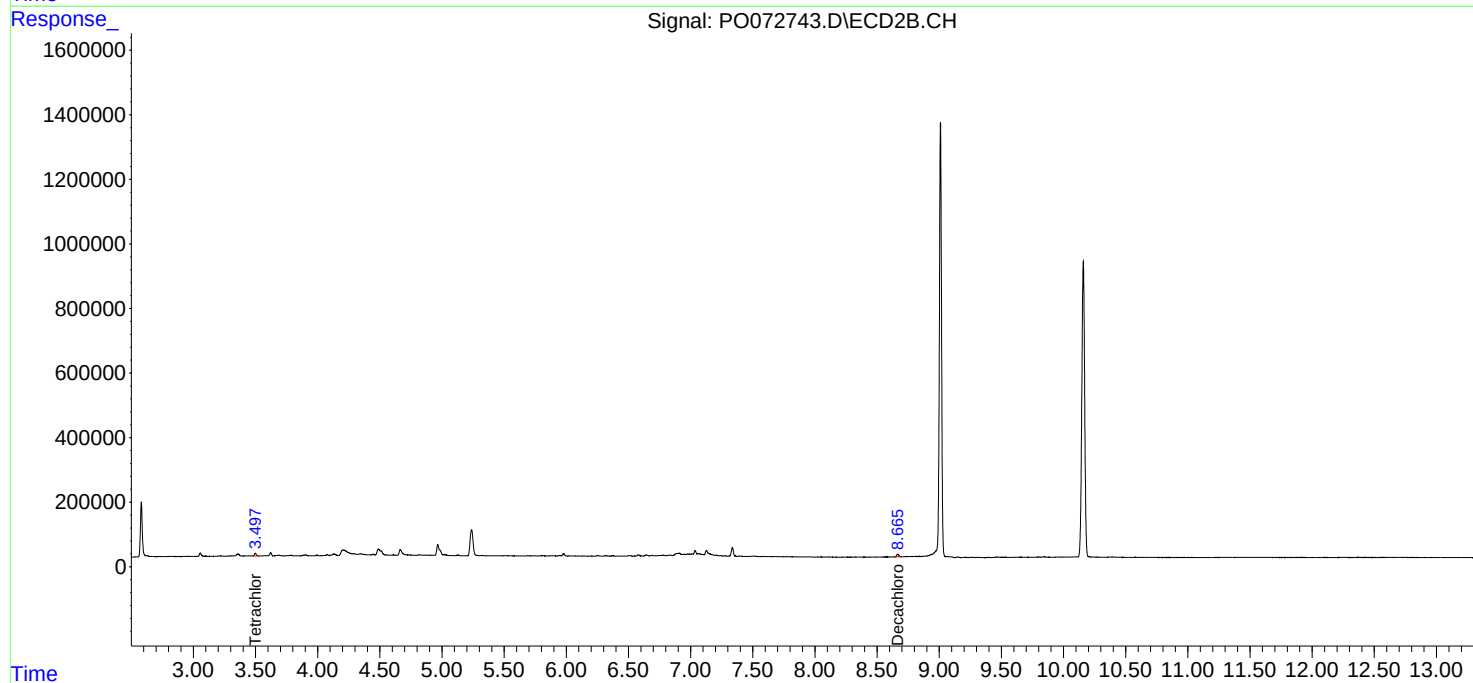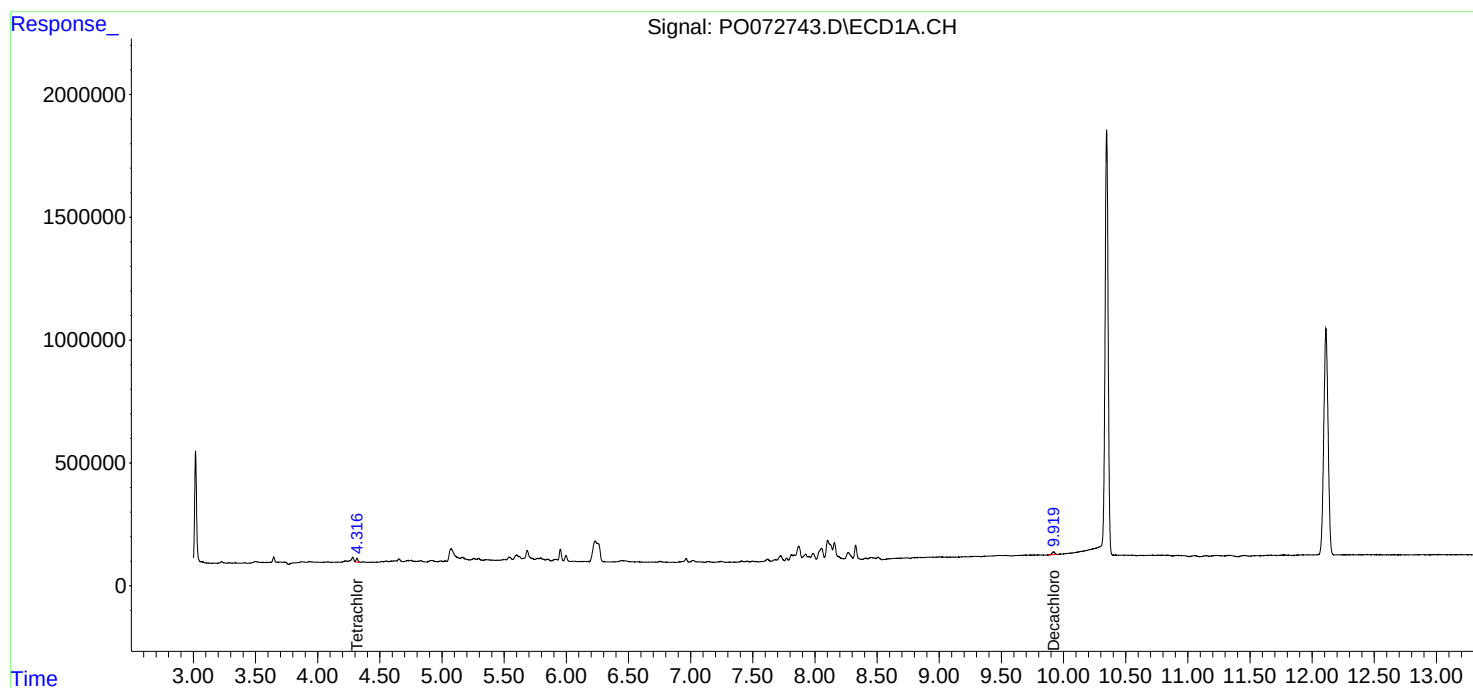

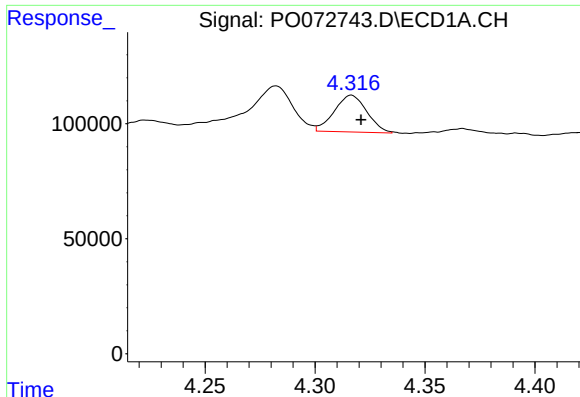


#1 Tetrachloro-m-xylene

R.T.: 4.316 min
Delta R.T.: -0.005 min
Response: 165195
Conc: 1.95 ng/ml m

Instrument :
ECD_O
ClientSampleId :
D-89


Manual Integrations
APPROVED

mohammad
10/26/2020 5:07:02 PM

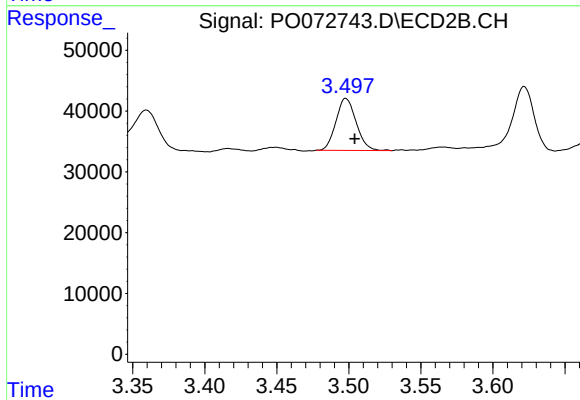


#1 Tetrachloro-m-xylene

R.T.: 3.498 min
Delta R.T.: -0.006 min
Response: 83915
Conc: 1.99 ng/ml

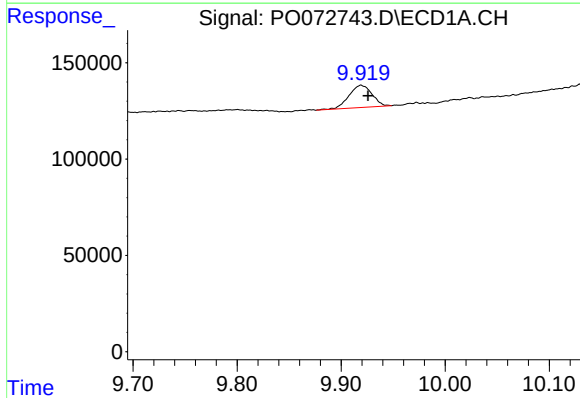

#2 Decachlorobiphenyl

R.T.: 9.919 min
Delta R.T.: -0.007 min
Response: 178582
Conc: 1.62 ng/ml

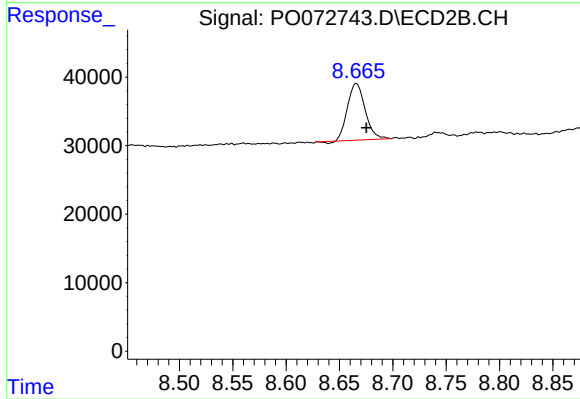

#2 Decachlorobiphenyl

R.T.: 8.666 min
Delta R.T.: -0.009 min
Response: 94860
Conc: 1.84 ng/ml