

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0102325\
 Data File : P0114638.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Oct 2025 16:55
 Operator : YP/AJ
 Sample : Q3405-04
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SW-10-20-25

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/24/2025
 Supervised By :mohammad ahmed 10/25/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 24 06:02:43 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0100925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Oct 21 02:40:25 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.354	3.656	145.3E6	100.9E6	26.761	25.205
2) SA Decachlor...	9.938	8.653	88081798	74080821	24.191	22.225m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\PO102325\
Data File : PO114638.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Oct 2025 16:55
Operator : YP/AJ
Sample : Q3405-04
Misc :
ALS Vial : 17 Sample Multiplier: 1


Instrument :
ECD_O
ClientSampleId :
SW-10-20-25


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/24/2025
Supervised By :mohammad ahmed 10/25/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 24 06:02:43 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\PO100925.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Oct 21 02:40:25 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

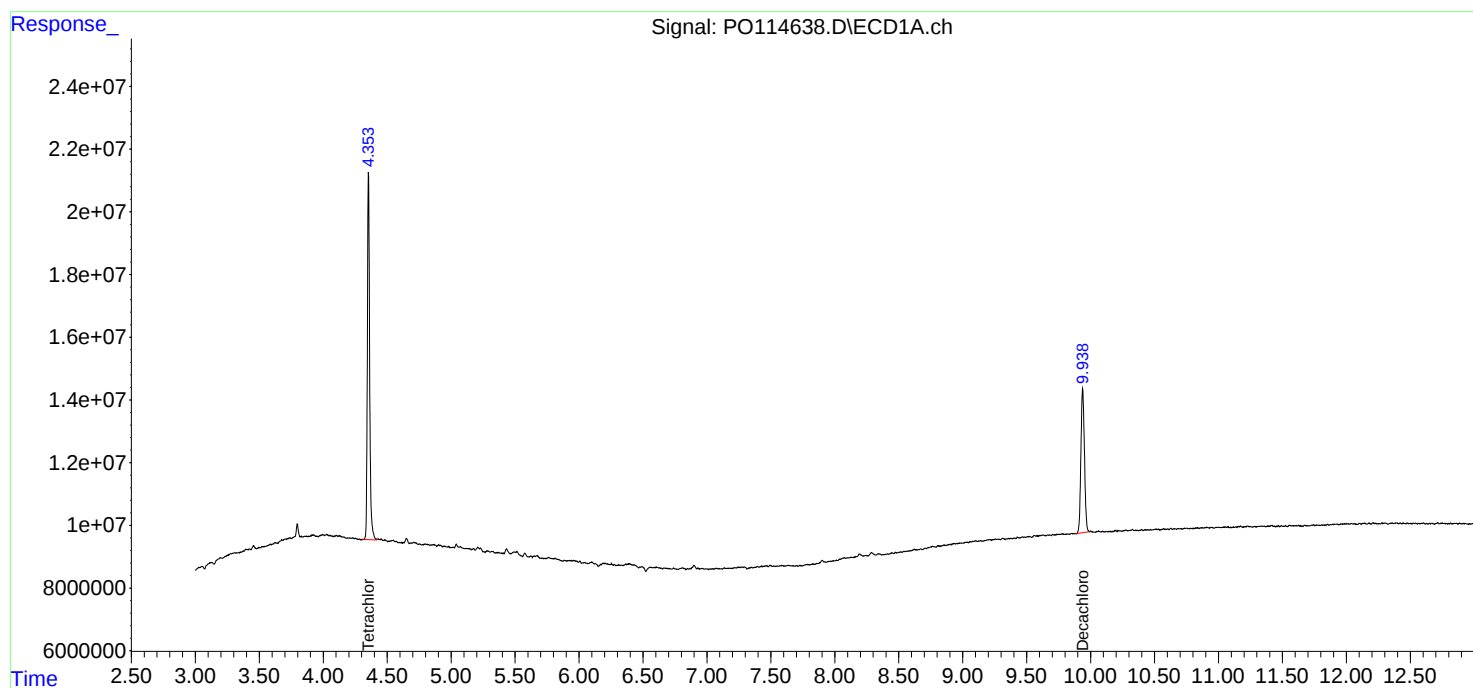

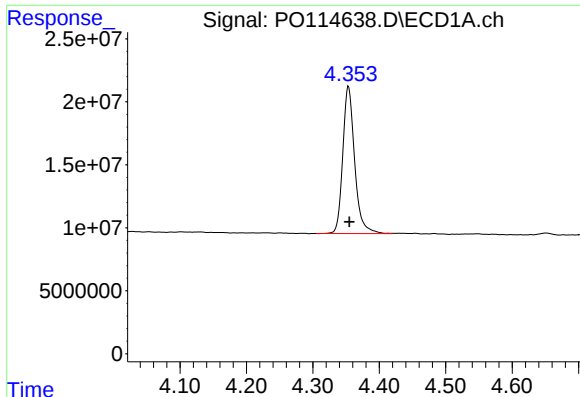


#1 Tetrachloro-m-xylene

R.T.: 4.354 min
Delta R.T.: -0.001 min
Response: 145287433
Conc: 26.76 ng/ml

Instrument :
ECD_O
ClientSampleId :
SW-10-20-25


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/24/2025
Supervised By :mohammad ahmed 10/25/2025

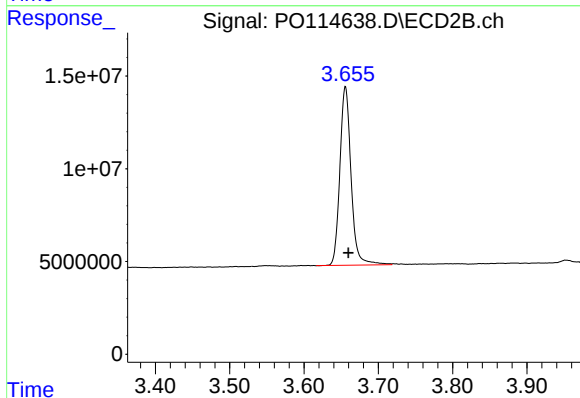


#1 Tetrachloro-m-xylene

R.T.: 3.656 min
Delta R.T.: -0.004 min
Response: 100874916
Conc: 25.20 ng/ml

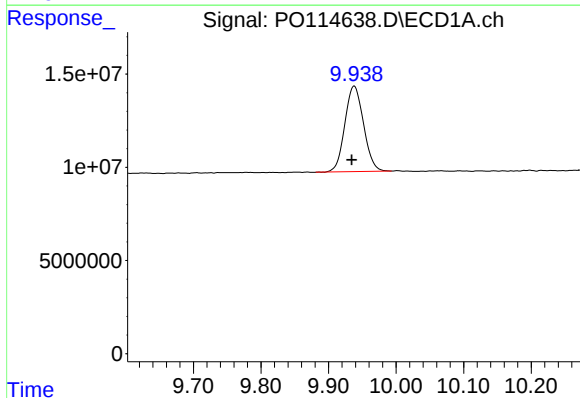

#2 Decachlorobiphenyl

R.T.: 9.938 min
Delta R.T.: 0.004 min
Response: 88081798
Conc: 24.19 ng/ml

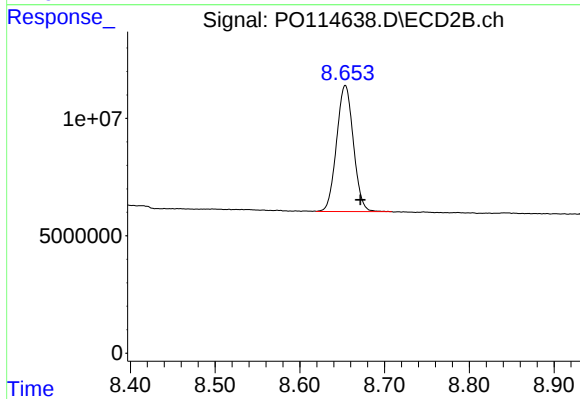

#2 Decachlorobiphenyl

R.T.: 8.653 min
Delta R.T.: -0.018 min
Response: 74080821
Conc: 22.23 ng/ml m