

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102420\
 Data File : PO072758.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Oct 2020 10:28
 Operator : DD\AJ
 Sample : L4488-06RE
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 1576RE

Manual Integrations
 APPROVED

mohammad
 10/26/2020 4:34:54 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 26 02:10:58 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101420.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 14 17:47:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.317	3.499	855659	453701	10.088	10.771m
2) SA Decachlor...	9.920	8.665	578702	256097	5.246	4.954

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102420\
Data File : PO072758.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Oct 2020 10:28
Operator : DD\AJ
Sample : L4488-06RE
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
1576RE


Manual Integrations
APPROVED

mohammad
10/26/2020 4:34:54 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 26 02:10:58 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101420.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 14 17:47:24 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

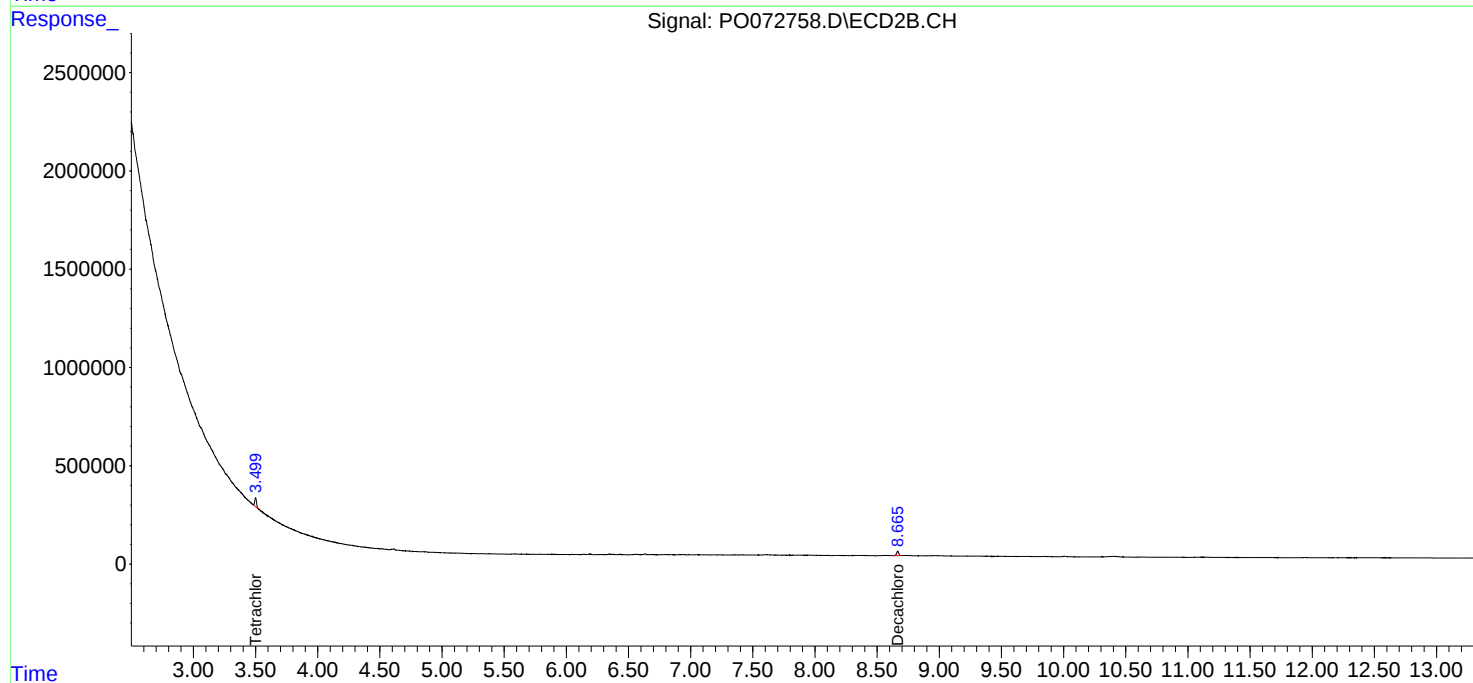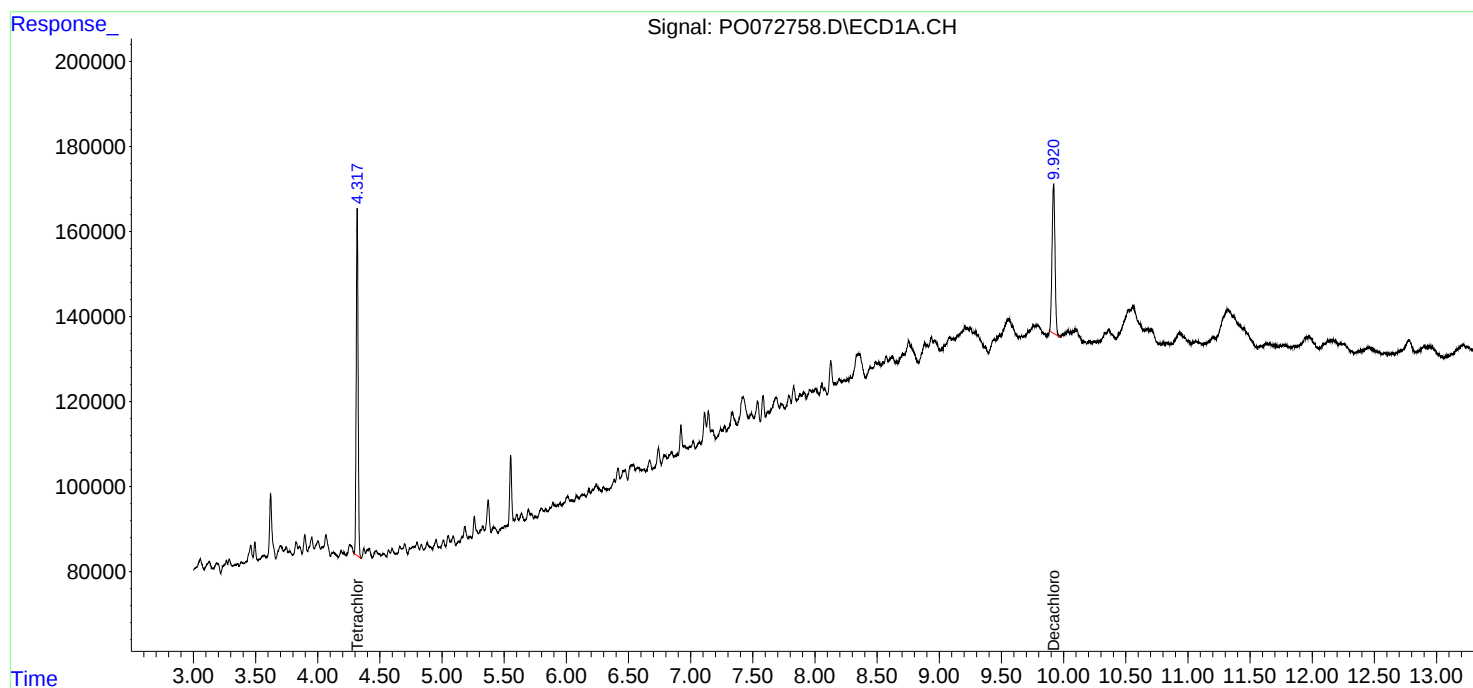

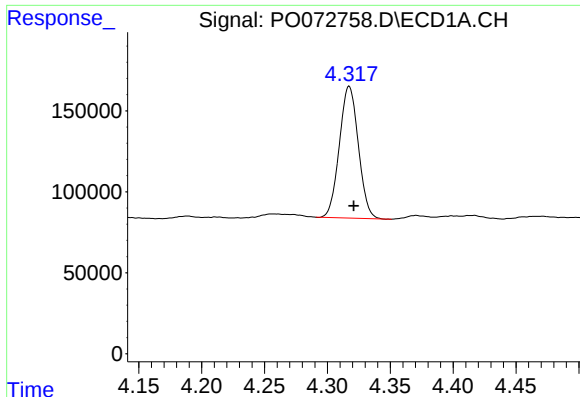


#1 Tetrachloro-m-xylene

R.T.: 4.317 min
Delta R.T.: -0.004 min
Response: 855659
Conc: 10.09 ng/ml

Instrument :
ECD_O
ClientSampleId :
1576RE


Manual Integrations
APPROVED

mohammad
10/26/2020 4:34:54 PM

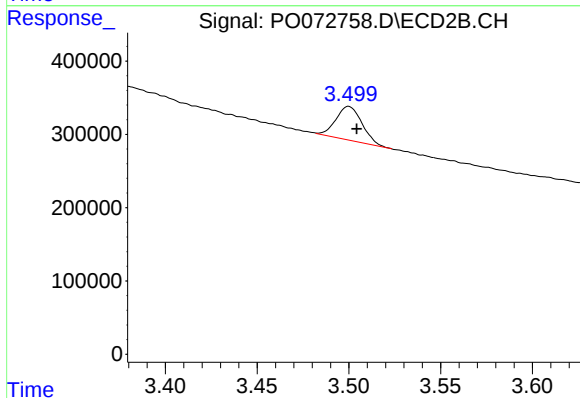


#1 Tetrachloro-m-xylene

R.T.: 3.499 min
Delta R.T.: -0.005 min
Response: 453701
Conc: 10.77 ng/ml m

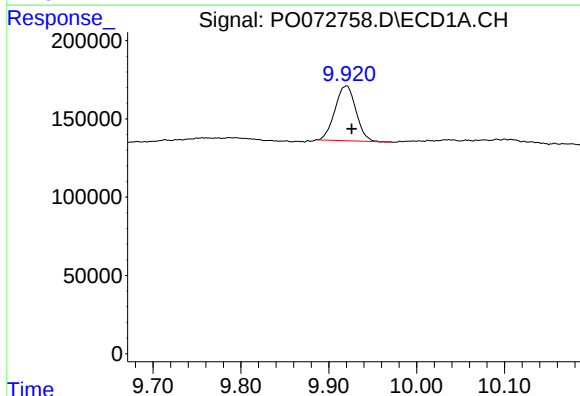

#2 Decachlorobiphenyl

R.T.: 9.920 min
Delta R.T.: -0.006 min
Response: 578702
Conc: 5.25 ng/ml

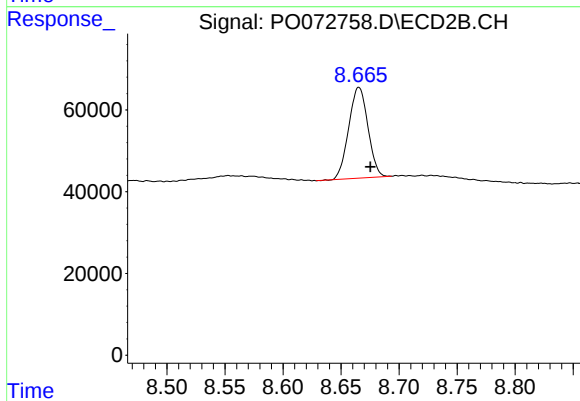

#2 Decachlorobiphenyl

R.T.: 8.665 min
Delta R.T.: -0.010 min
Response: 256097
Conc: 4.95 ng/ml