

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102422\
 Data File : PO089888.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Oct 2022 03:20
 Operator : YP/AJ
 Sample : N4955-07
 Misc : AR1221 LOD 25 PPB
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 LOD-MDL-WATER-01-QT4-2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 25 04:50:22 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102422.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Oct 25 02:35:13 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.306	3.486	69769318	23023992	21.925	23.006
2)	SA Decachlor...	10.051	8.496	57535794	21843636	24.039	24.041
Target Compounds							
8)	L2 AR-1221-1	4.515	3.699	1409434	373181	34.879	27.229
9)	L2 AR-1221-2	4.609	3.786	1543096	539217	51.690	51.999
10)	L2 AR-1221-3	4.679	3.862	2441156	769827	26.774	23.889



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102422\
Data File : PO089888.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Oct 2022 03:20
Operator : YP/AJ
Sample : N4955-07
Misc : AR1221 LOD 25 PPB
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 25 04:50:22 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102422.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Oct 25 02:35:13 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

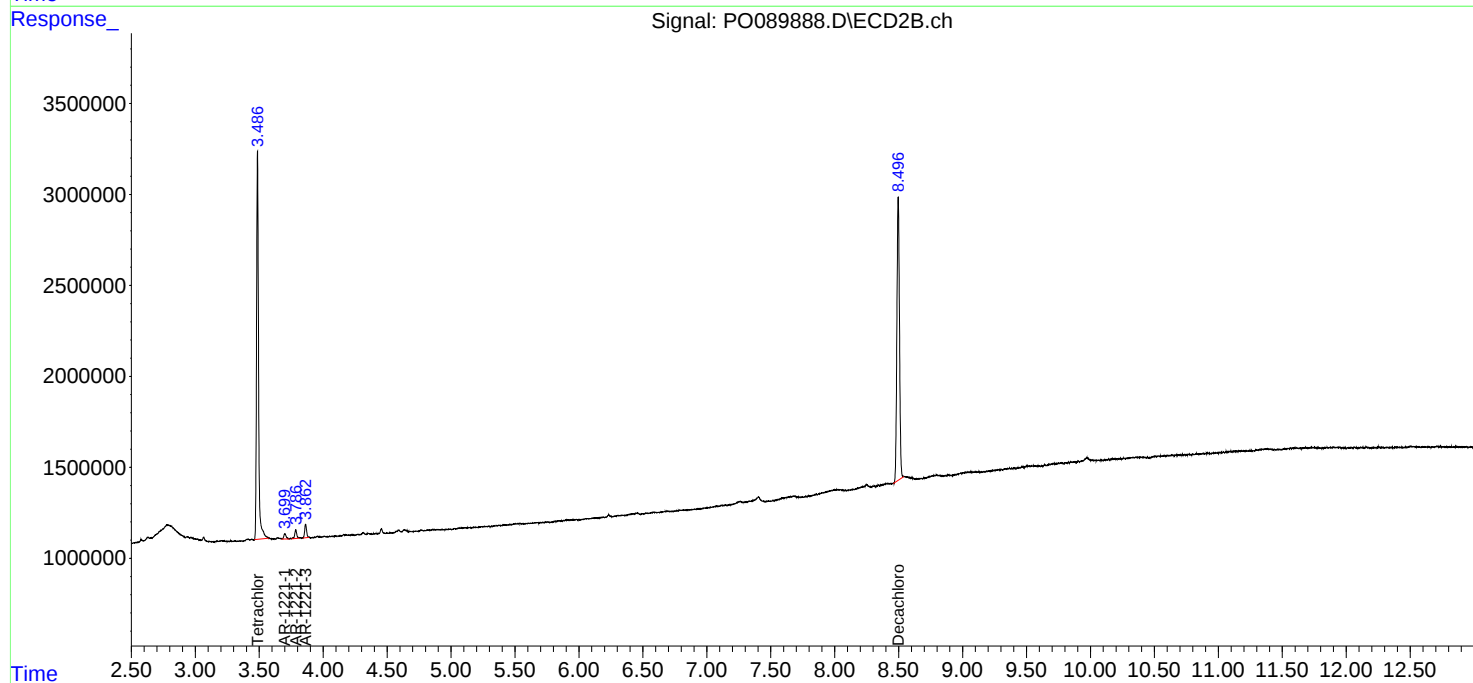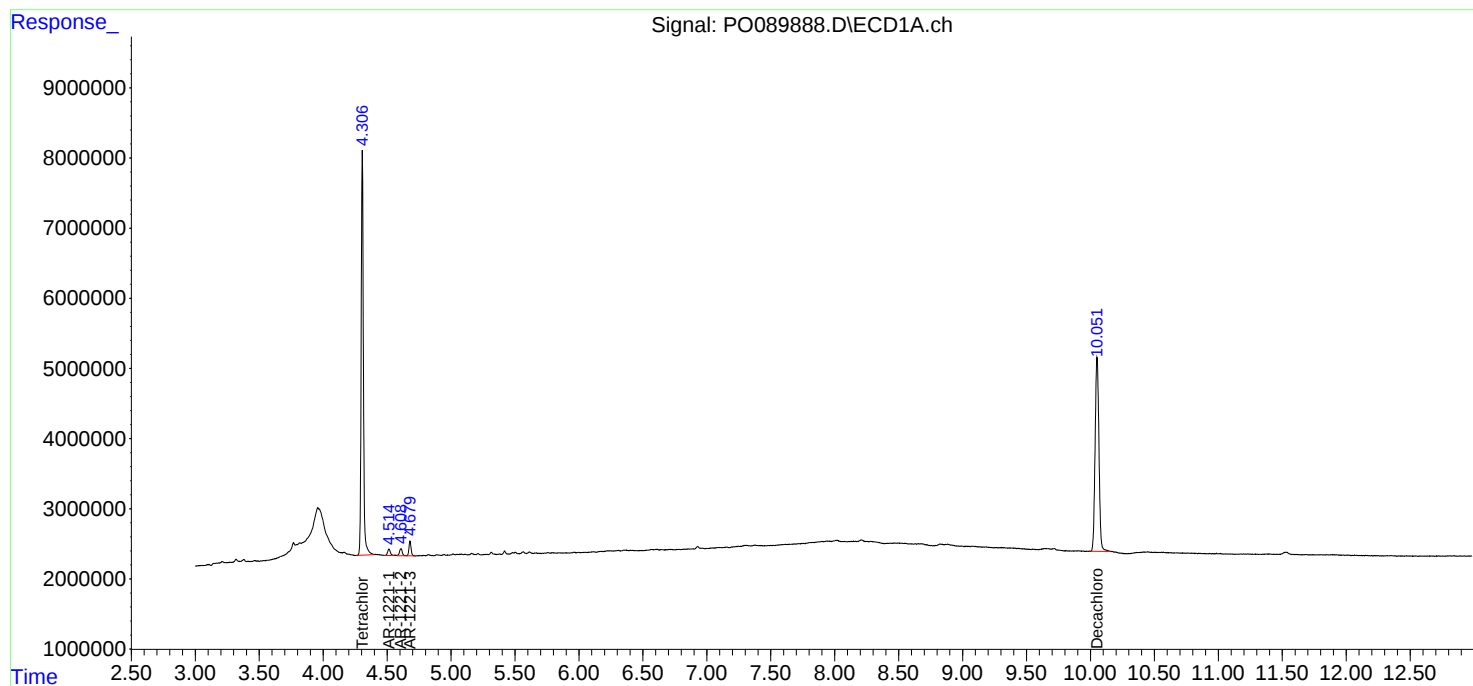


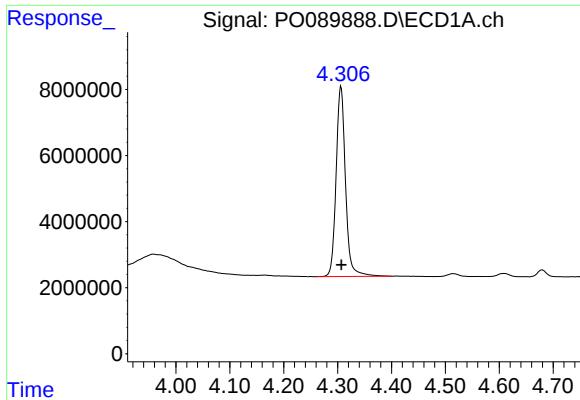

#1 Tetrachloro-m-xylene


R.T.: 4.306 min
Delta R.T.: 0.000 min
Response: 69769318
Conc: 21.92 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2022

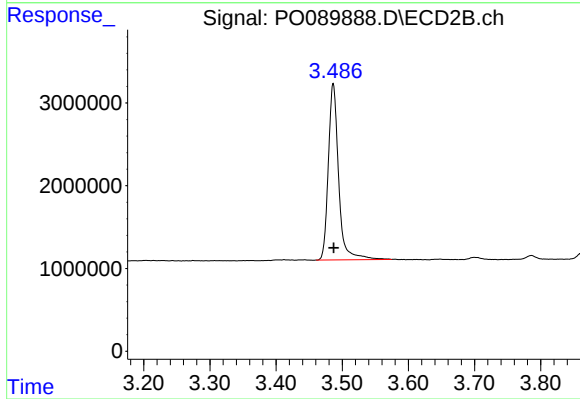


#1 Tetrachloro-m-xylene

R.T.: 3.486 min
Delta R.T.: 0.000 min
Response: 23023992
Conc: 23.01 ng/ml

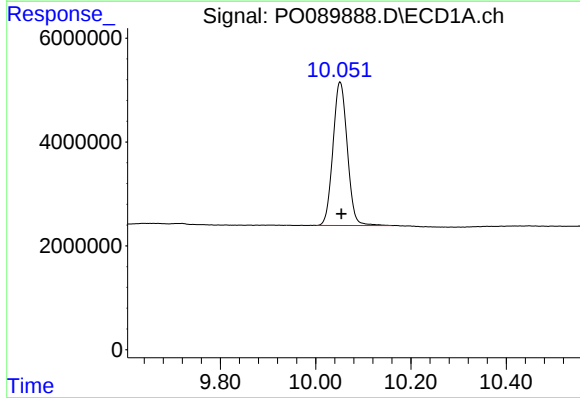


#2 Decachlorobiphenyl

R.T.: 10.051 min
Delta R.T.: -0.003 min
Response: 57535794
Conc: 24.04 ng/ml

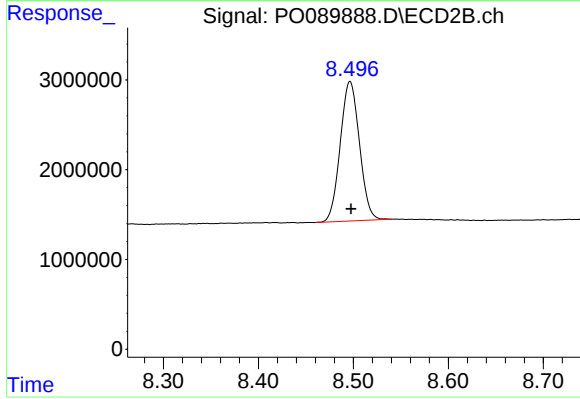

#2 Decachlorobiphenyl


R.T.: 8.496 min
Delta R.T.: -0.001 min
Response: 21843636
Conc: 24.04 ng/ml

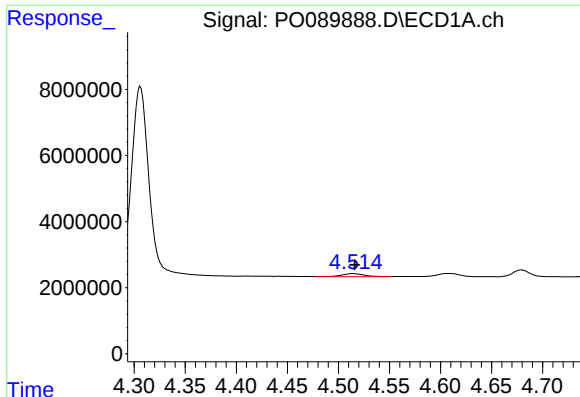

#8 AR-1221-1


R.T.: 4.515 min
Delta R.T.: -0.001 min
Response: 1409434
Conc: 34.88 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2022

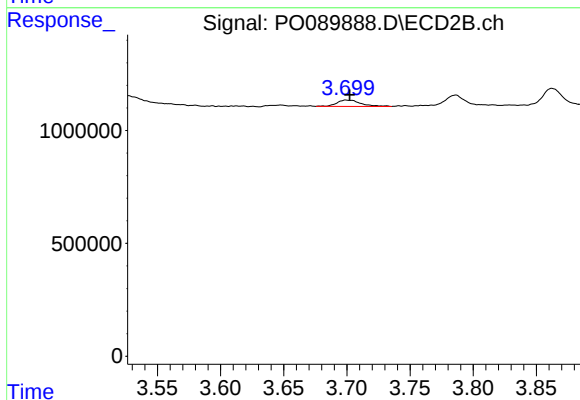


#8 AR-1221-1

R.T.: 3.699 min
Delta R.T.: -0.003 min
Response: 373181
Conc: 27.23 ng/ml

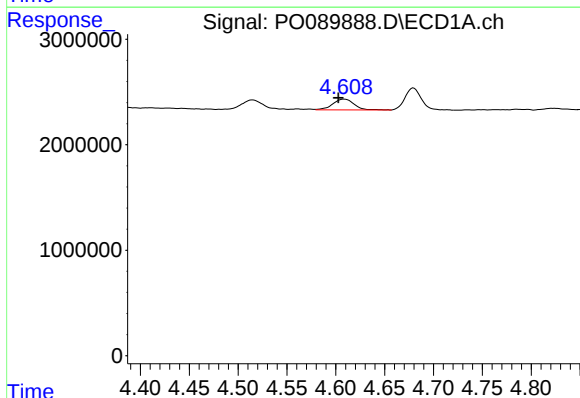


#9 AR-1221-2

R.T.: 4.609 min
Delta R.T.: 0.006 min
Response: 1543096
Conc: 51.69 ng/ml

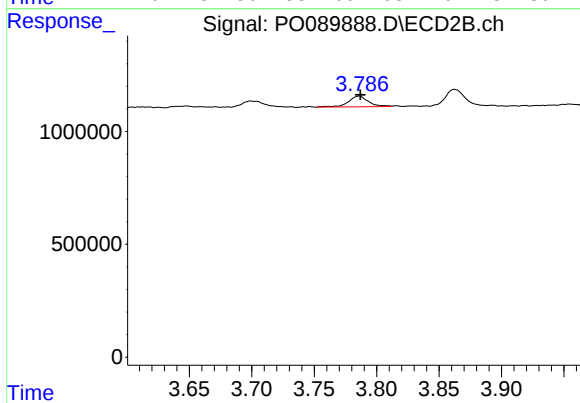

#9 AR-1221-2


R.T.: 3.786 min
Delta R.T.: 0.000 min
Response: 539217
Conc: 52.00 ng/ml

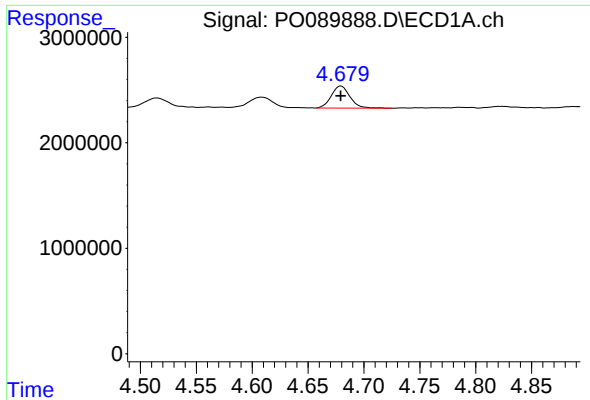

#10 AR-1221-3

R.T.: 4.679 min
Delta R.T.: 0.000 min
Response: 2441156
Conc: 26.77 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2022

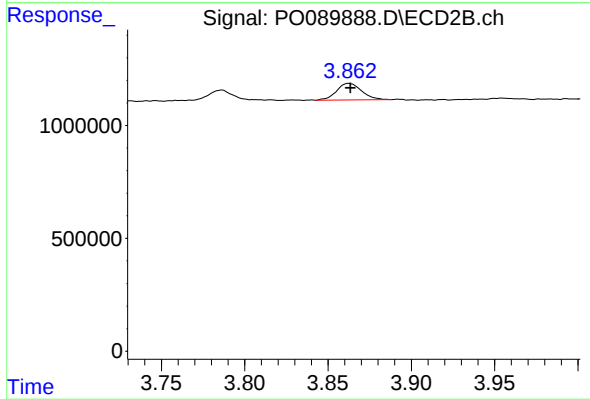

#10 AR-1221-3

R.T.: 3.862 min
Delta R.T.: -0.001 min
Response: 769827
Conc: 23.89 ng/ml