

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102422\
 Data File : PO089892.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Oct 2022 04:28
 Operator : YP/AJ
 Sample : N4955-07
 Misc : AR1254 LOD 25 PPB
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 LOD-MDL-WATER-01-QT4-2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 25 05:36:08 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102422.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Oct 25 02:35:13 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.306	3.487	82763051	26794136	26.008	26.773
2) SA Decachlor...	10.052	8.497	68133467	25824927	28.467	28.422
Target Compounds						
26) L6 AR-1254-1	6.341	5.379	3165153	1368900	27.552	23.918
27) L6 AR-1254-2	6.562	5.527	4677435	1404953	27.153	27.472
28) L6 AR-1254-3	6.929	5.932	4523334	1823307	26.114	23.122
29) L6 AR-1254-4	7.217	6.162	3581577	1154627	28.254	24.232
30) L6 AR-1254-5	7.637	6.581	3154384	1550488	22.653	21.942



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102422\
Data File : PO089892.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Oct 2022 04:28
Operator : YP/AJ
Sample : N4955-07
Misc : AR1254 LOD 25 PPB
ALS Vial : 31 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 25 05:36:08 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102422.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Oct 25 02:35:13 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

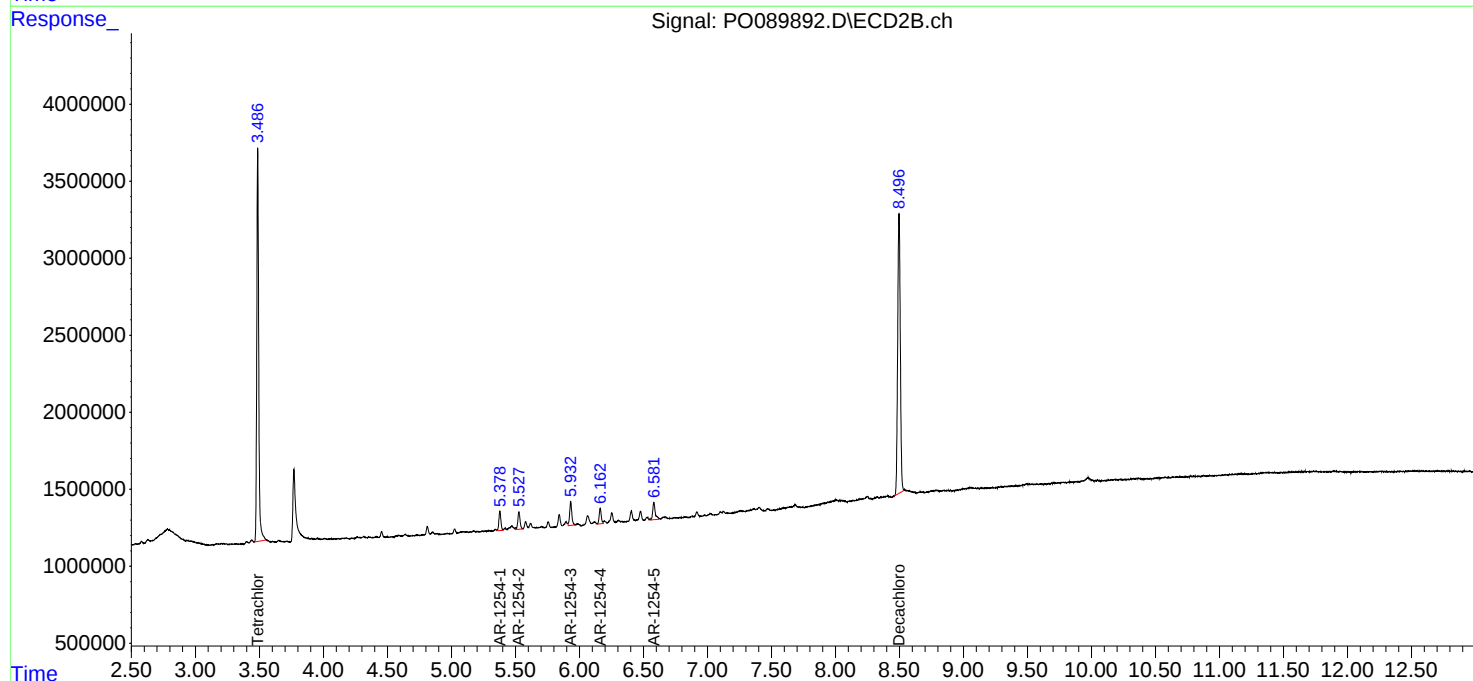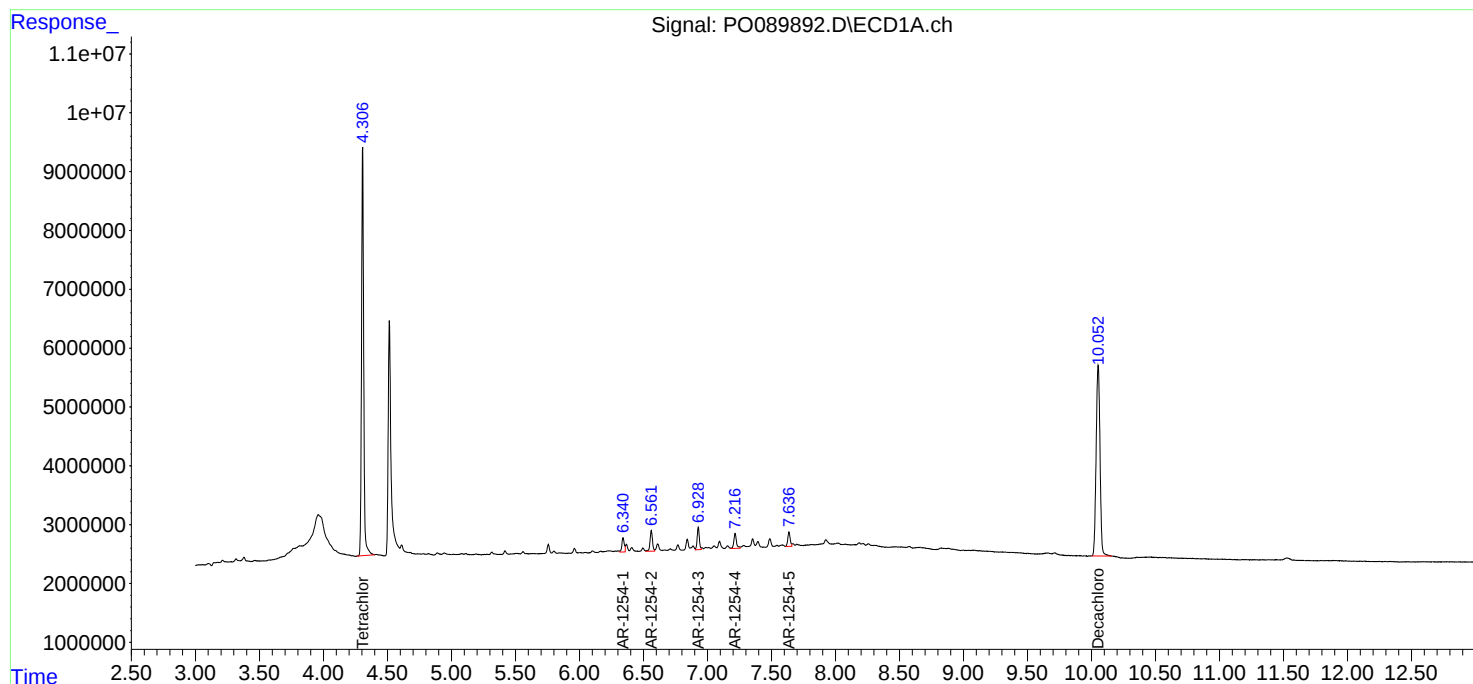


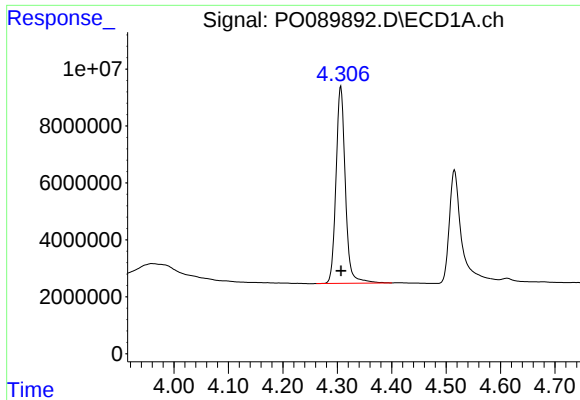

#1 Tetrachloro-m-xylene


R.T.: 4.306 min
Delta R.T.: 0.000 min
Response: 82763051
Conc: 26.01 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2022

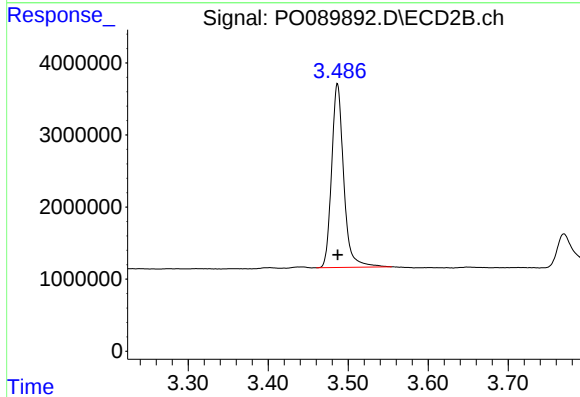


#1 Tetrachloro-m-xylene

R.T.: 3.487 min
Delta R.T.: 0.000 min
Response: 26794136
Conc: 26.77 ng/ml

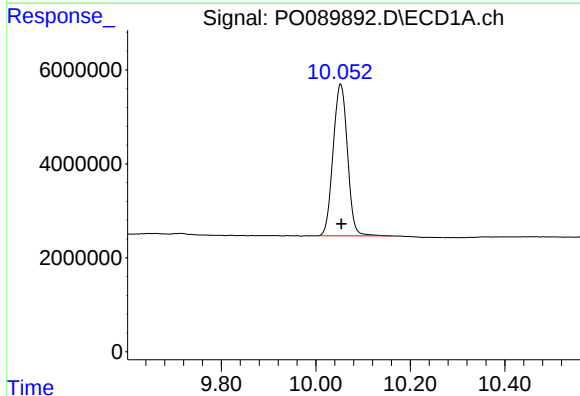


#2 Decachlorobiphenyl

R.T.: 10.052 min
Delta R.T.: -0.002 min
Response: 68133467
Conc: 28.47 ng/ml

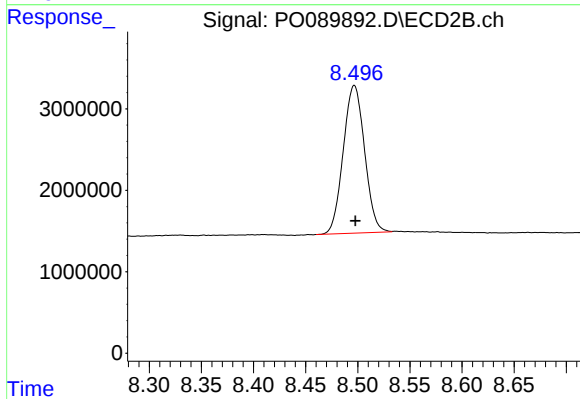

#2 Decachlorobiphenyl


R.T.: 8.497 min
Delta R.T.: 0.000 min
Response: 25824927
Conc: 28.42 ng/ml

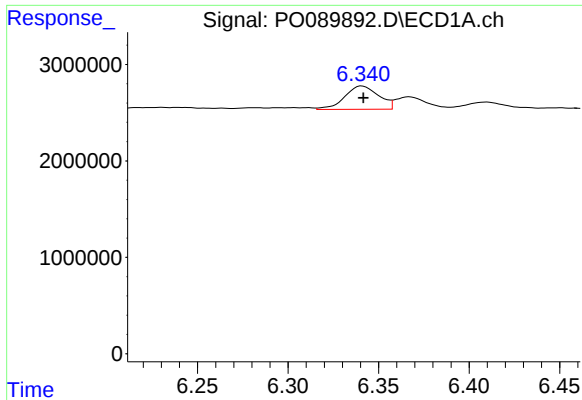

#26 AR-1254-1


R.T.: 6.341 min
Delta R.T.: 0.000 min
Response: 3165153
Conc: 27.55 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2022

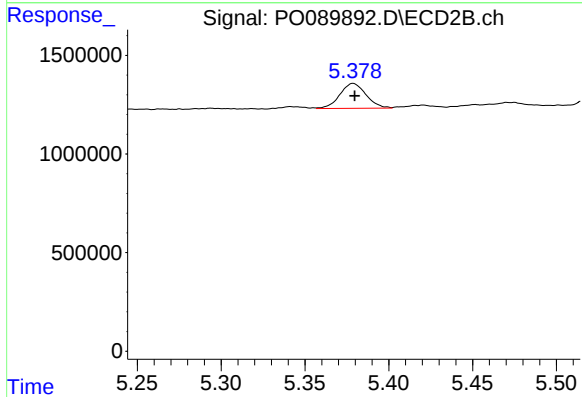


#26 AR-1254-1

R.T.: 5.379 min
Delta R.T.: 0.000 min
Response: 1368900
Conc: 23.92 ng/ml

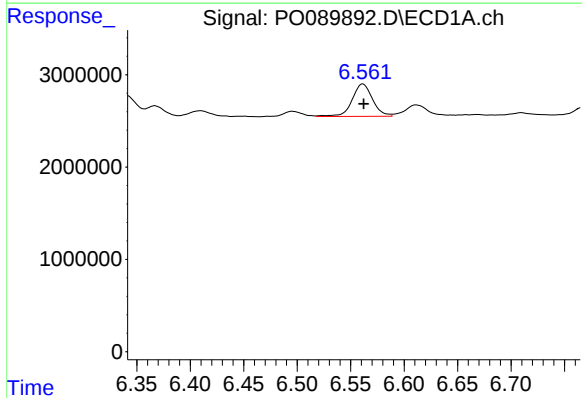


#27 AR-1254-2

R.T.: 6.562 min
Delta R.T.: 0.000 min
Response: 4677435
Conc: 27.15 ng/ml

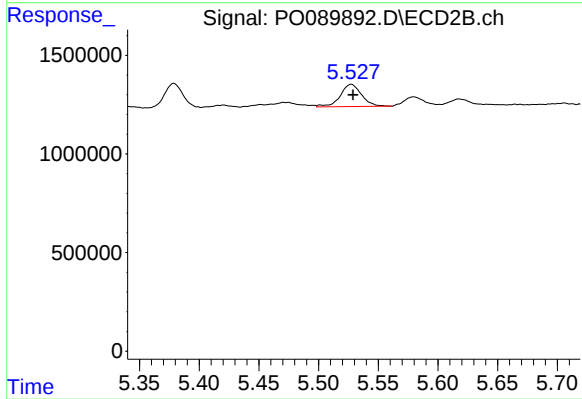

#27 AR-1254-2


R.T.: 5.527 min
Delta R.T.: -0.001 min
Response: 1404953
Conc: 27.47 ng/ml

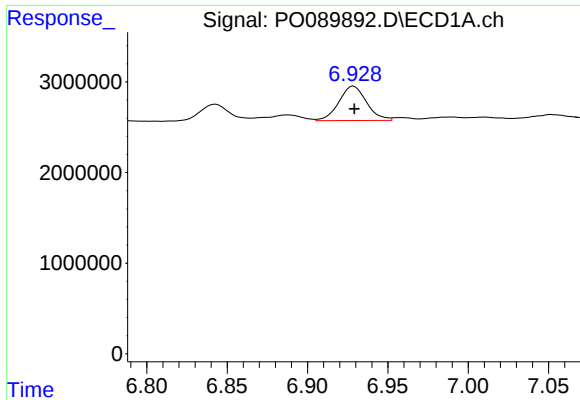

#28 AR-1254-3


R.T.: 6.929 min
Delta R.T.: 0.000 min
Response: 4523334
Conc: 26.11 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2022

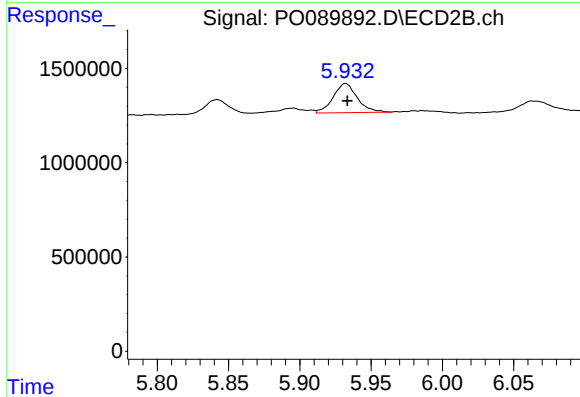


#28 AR-1254-3

R.T.: 5.932 min
Delta R.T.: -0.001 min
Response: 1823307
Conc: 23.12 ng/ml

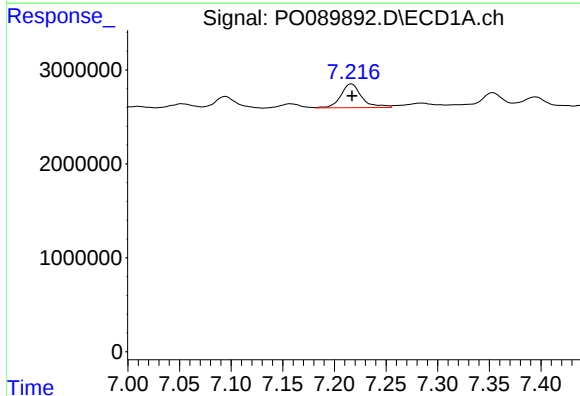


#29 AR-1254-4

R.T.: 7.217 min
Delta R.T.: 0.000 min
Response: 3581577
Conc: 28.25 ng/ml

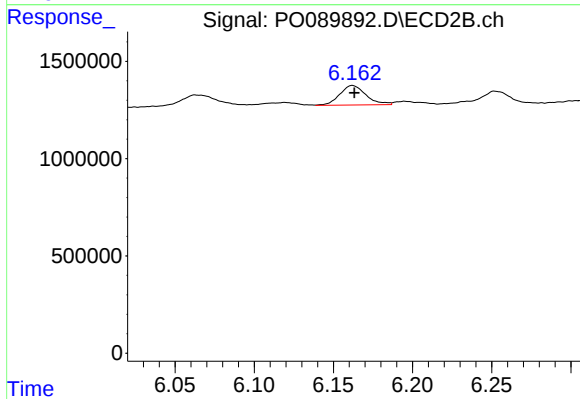

#29 AR-1254-4


R.T.: 6.162 min
Delta R.T.: -0.001 min
Response: 1154627
Conc: 24.23 ng/ml

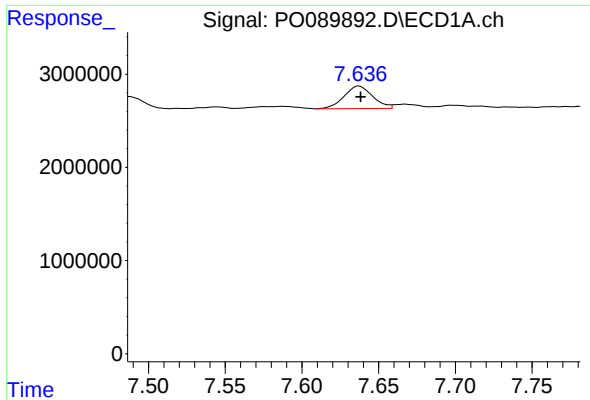

#30 AR-1254-5

R.T.: 7.637 min
Delta R.T.: -0.001 min
Response: 3154384
Conc: 22.65 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2022

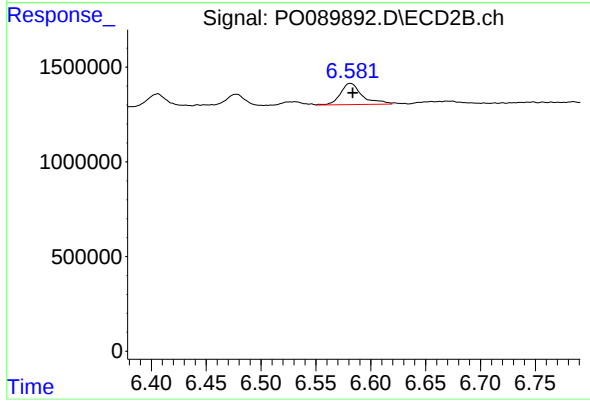

#30 AR-1254-5

R.T.: 6.581 min
Delta R.T.: -0.002 min
Response: 1550488
Conc: 21.94 ng/ml