

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102422\
 Data File : PO089893.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Oct 2022 04:45
 Operator : YP/AJ
 Sample : N4955-07
 Misc : AR1262 LOD 25 PPB
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 LOD-MDL-WATER-01-QT4-2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 25 05:37:02 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102422.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Oct 25 02:35:13 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.306	3.487	73778239	24227347	23.185	24.209
2) SA Decachlor...	10.053	8.497	61159943	23264041	25.553	25.604
Target Compounds						
36) L8 AR-1262-1	7.716	6.622	4107822	1871966	24.864	26.113
37) L8 AR-1262-2	8.257	7.125	7439061	3285806	26.712	27.092
38) L8 AR-1262-3	8.567	7.410	4820621	1835611	24.664	35.408 #
39) L8 AR-1262-4	8.655	7.473	2257494	2433881	24.376	26.693
40) L8 AR-1262-5	9.303	7.970	2555292	1492278	24.187	33.991 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102422\
Data File : P0089893.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Oct 2022 04:45
Operator : YP/AJ
Sample : N4955-07
Misc : AR1262 LOD 25 PPB
ALS Vial : 32 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 25 05:37:02 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102422.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Oct 25 02:35:13 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

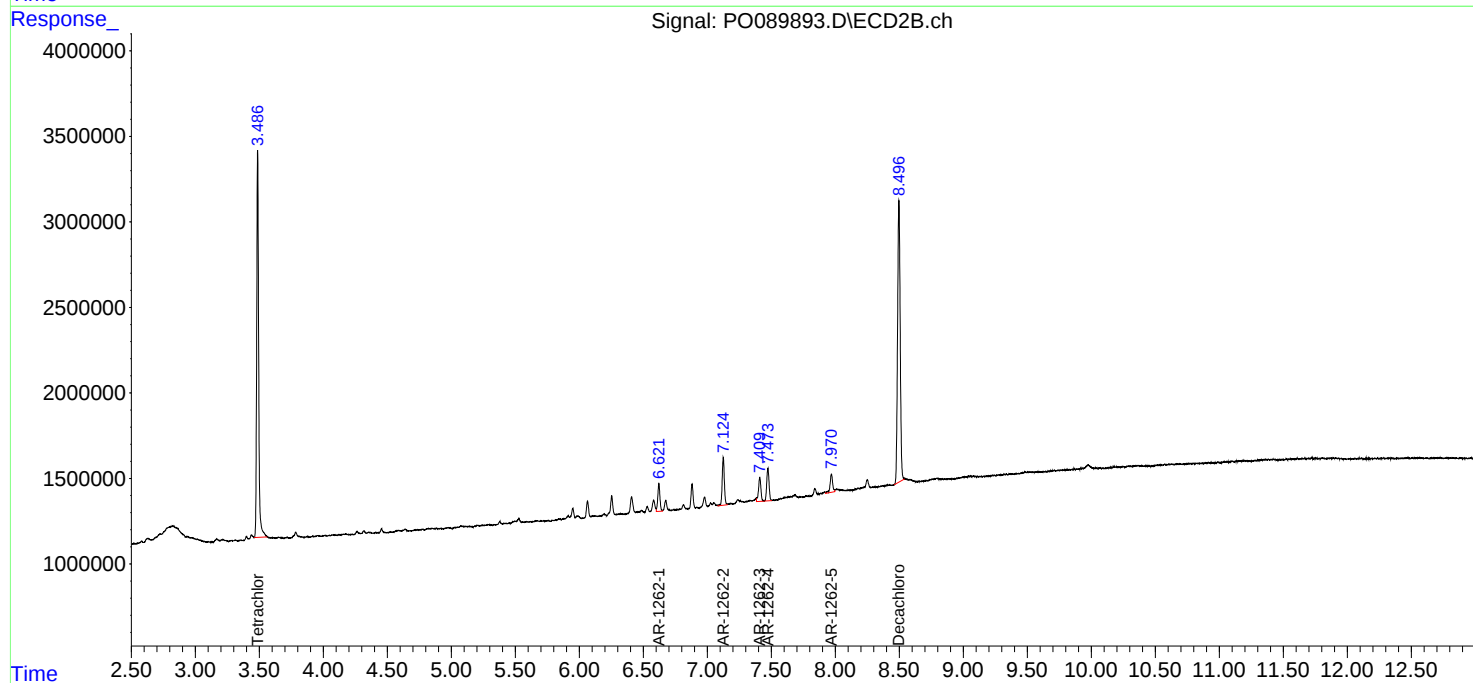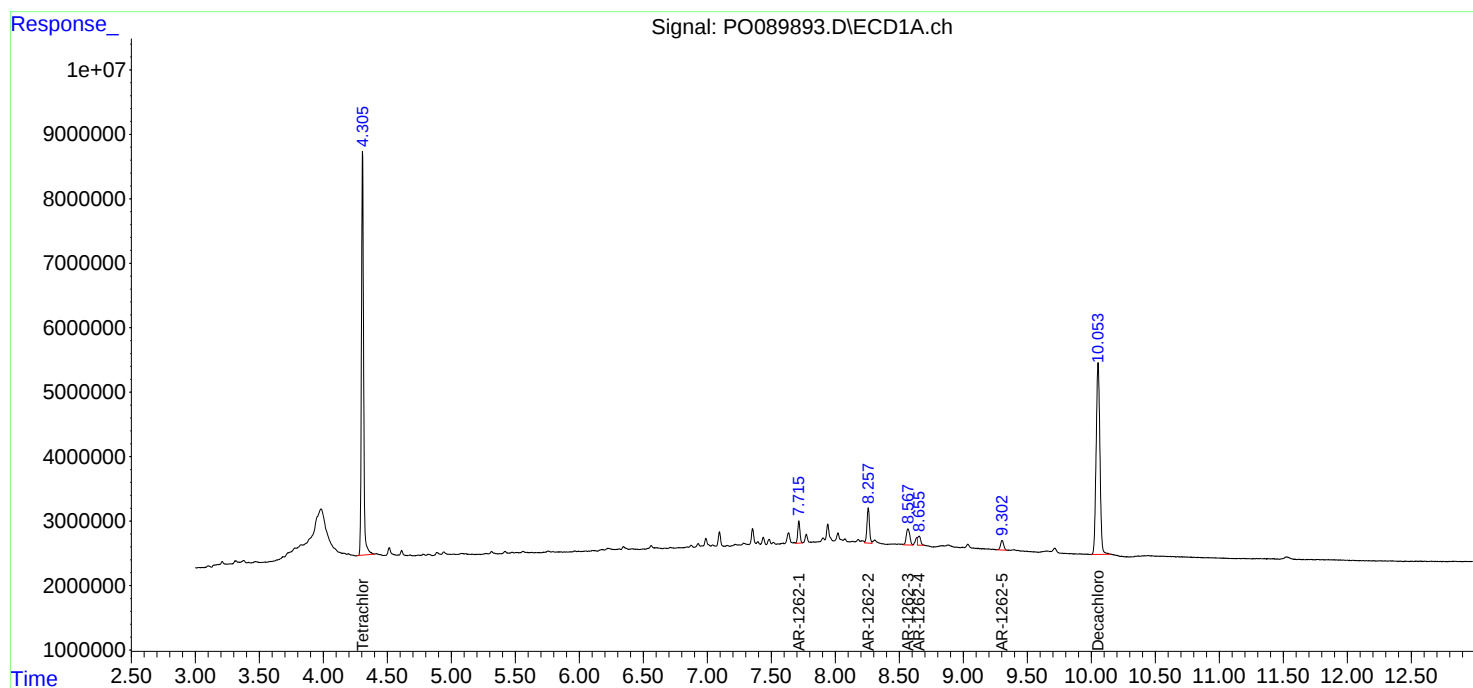


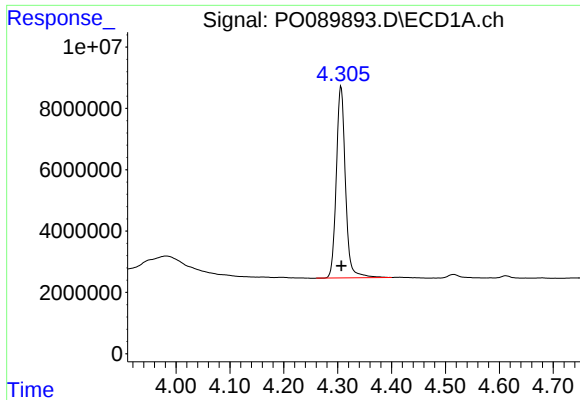

#1 Tetrachloro-m-xylene


R.T.: 4.306 min
Delta R.T.: 0.000 min
Response: 73778239
Conc: 23.18 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2022

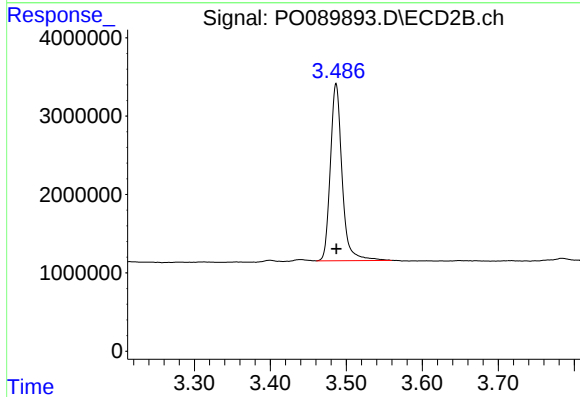


#1 Tetrachloro-m-xylene

R.T.: 3.487 min
Delta R.T.: 0.000 min
Response: 24227347
Conc: 24.21 ng/ml

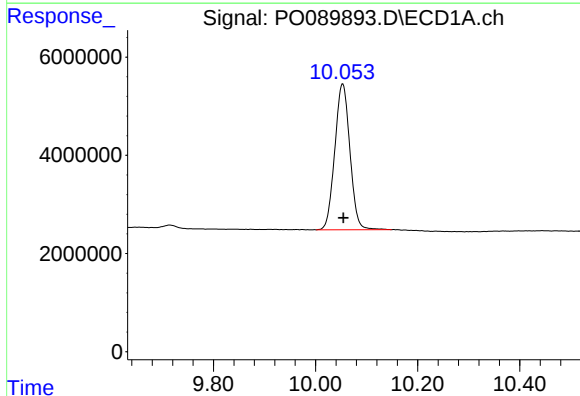


#2 Decachlorobiphenyl

R.T.: 10.053 min
Delta R.T.: -0.001 min
Response: 61159943
Conc: 25.55 ng/ml

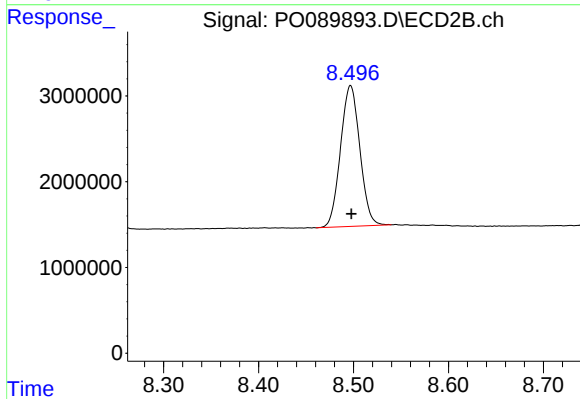

#2 Decachlorobiphenyl


R.T.: 8.497 min
Delta R.T.: 0.000 min
Response: 23264041
Conc: 25.60 ng/ml

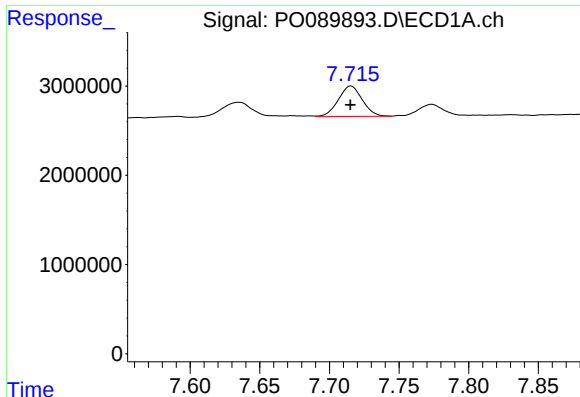

#36 AR-1262-1


R.T.: 7.716 min
Delta R.T.: 0.000 min
Response: 4107822
Conc: 24.86 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2022

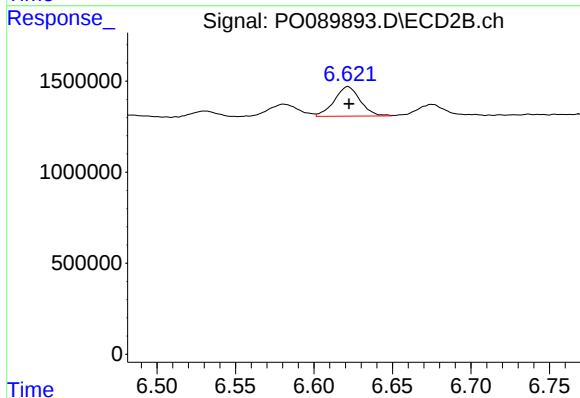


#36 AR-1262-1

R.T.: 6.622 min
Delta R.T.: 0.000 min
Response: 1871966
Conc: 26.11 ng/ml

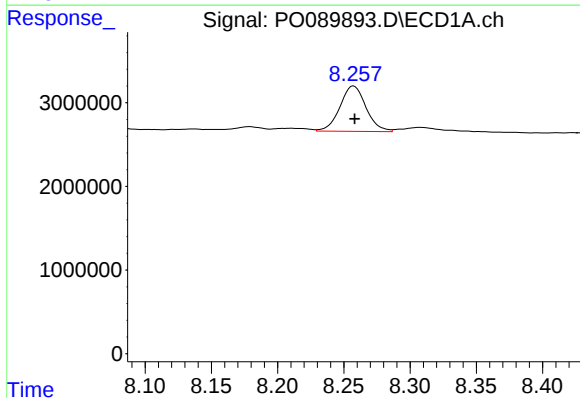


#37 AR-1262-2

R.T.: 8.257 min
Delta R.T.: 0.000 min
Response: 7439061
Conc: 26.71 ng/ml

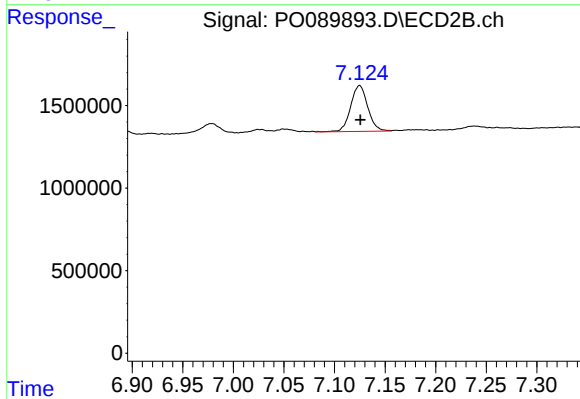

#37 AR-1262-2


R.T.: 7.125 min
Delta R.T.: 0.000 min
Response: 3285806
Conc: 27.09 ng/ml

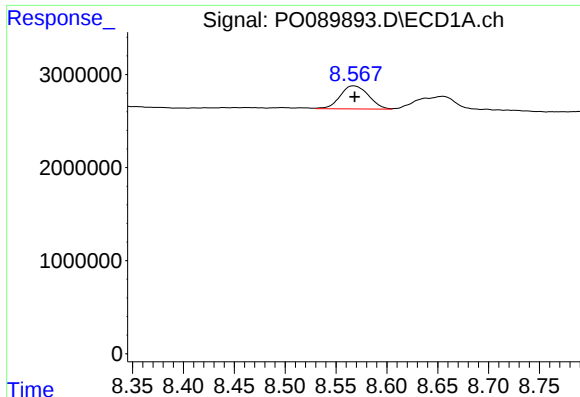

#38 AR-1262-3


R.T.: 8.567 min
Delta R.T.: 0.000 min
Response: 4820621
Conc: 24.66 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2022

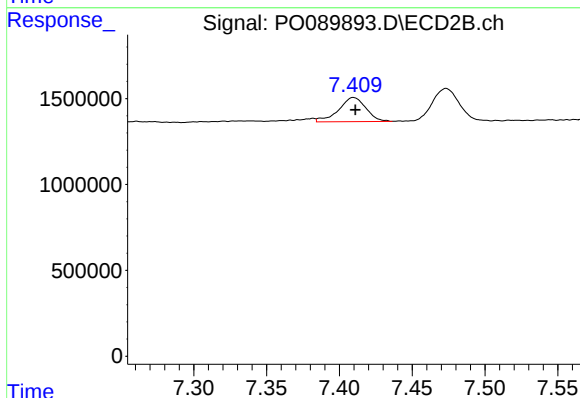


#38 AR-1262-3

R.T.: 7.410 min
Delta R.T.: -0.001 min
Response: 1835611
Conc: 35.41 ng/ml

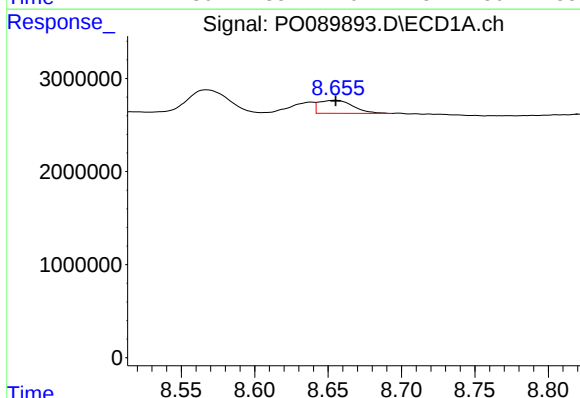


#39 AR-1262-4

R.T.: 8.655 min
Delta R.T.: 0.000 min
Response: 2257494
Conc: 24.38 ng/ml

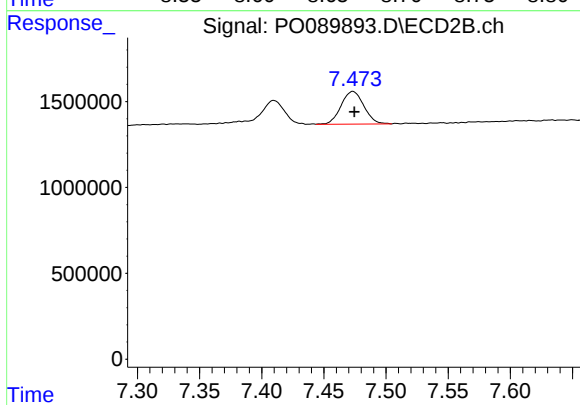

#39 AR-1262-4


R.T.: 7.473 min
Delta R.T.: -0.001 min
Response: 2433881
Conc: 26.69 ng/ml

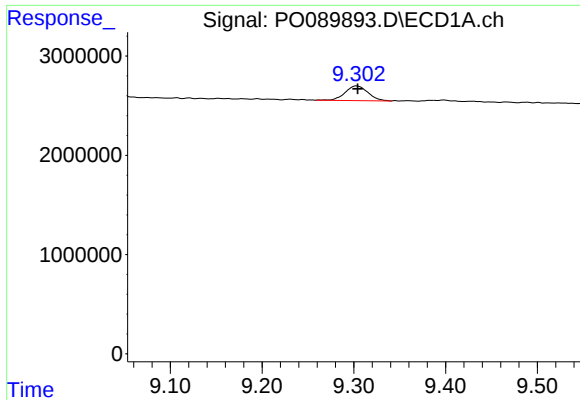

#40 AR-1262-5

R.T.: 9.303 min
Delta R.T.: -0.001 min
Response: 2555292
Conc: 24.19 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2022

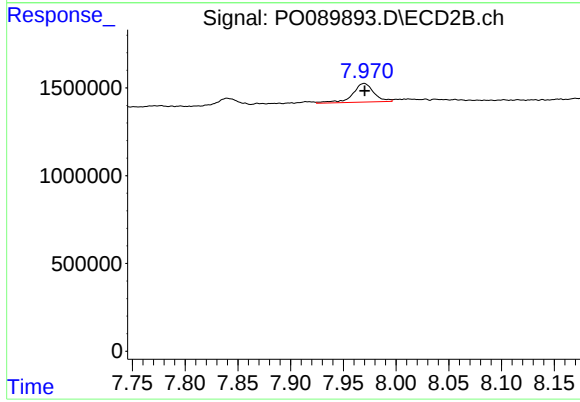

#40 AR-1262-5

R.T.: 7.970 min
Delta R.T.: 0.000 min
Response: 1492278
Conc: 33.99 ng/ml