

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0102518\
 Data File : P0050546.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 25 Oct 2018 18:02
 Operator : SM/SJ
 Sample : J5636-04
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 26 01:40:28 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101818.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Oct 19 02:02:26 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.359	3.353	7839535	5132865	26.273	26.108
2) SA Decachlor...	10.022	8.104	-663989	3401074	N.D.	17.793
Target Compounds						
7) L1 AR-1016-5	0.000	4.820	0	75723	N.D.	10.934 #
8) L2 AR-1221-1	0.000	3.630	0	83672	N.D.	38.734 #
9) L2 AR-1221-2	0.000	3.630	0	83672	N.D.	52.198 #
10) L2 AR-1221-3	0.000	3.746	0	84541	N.D.	16.114 #
11) L3 AR-1232-1	0.000	3.746	0	84541	N.D.	21.874 #
15) L3 AR-1232-5	0.000	4.820	0	75723	N.D.	34.384 #
24) L5 AR-1248-4	0.000	4.820	0	75723	N.D.	9.273 #
27) L6 AR-1254-2	6.594	0.000	411611	0	20.189	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102518\
Data File : PO050546.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 Oct 2018 18:02
Operator : SM/SJ
Sample : J5636-04
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 26 01:40:28 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101818.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Oct 19 02:02:26 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

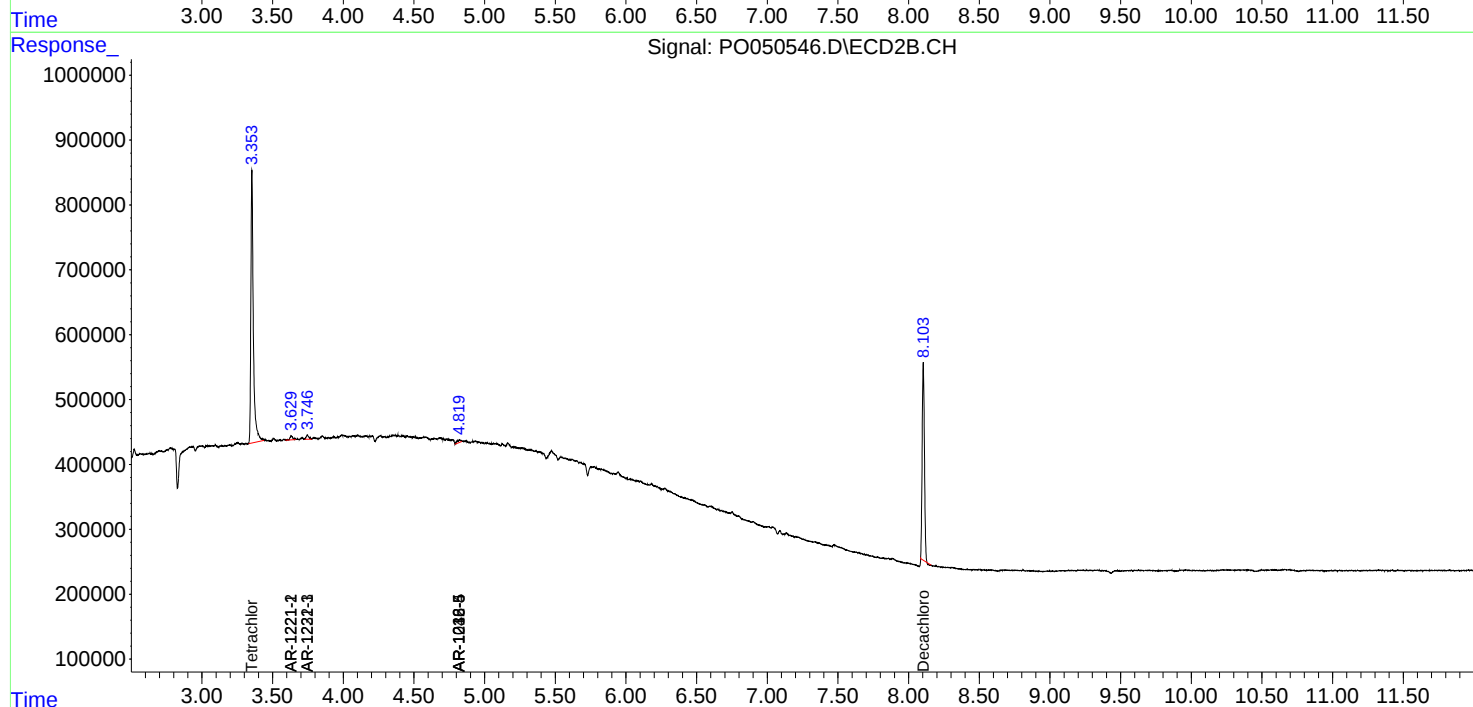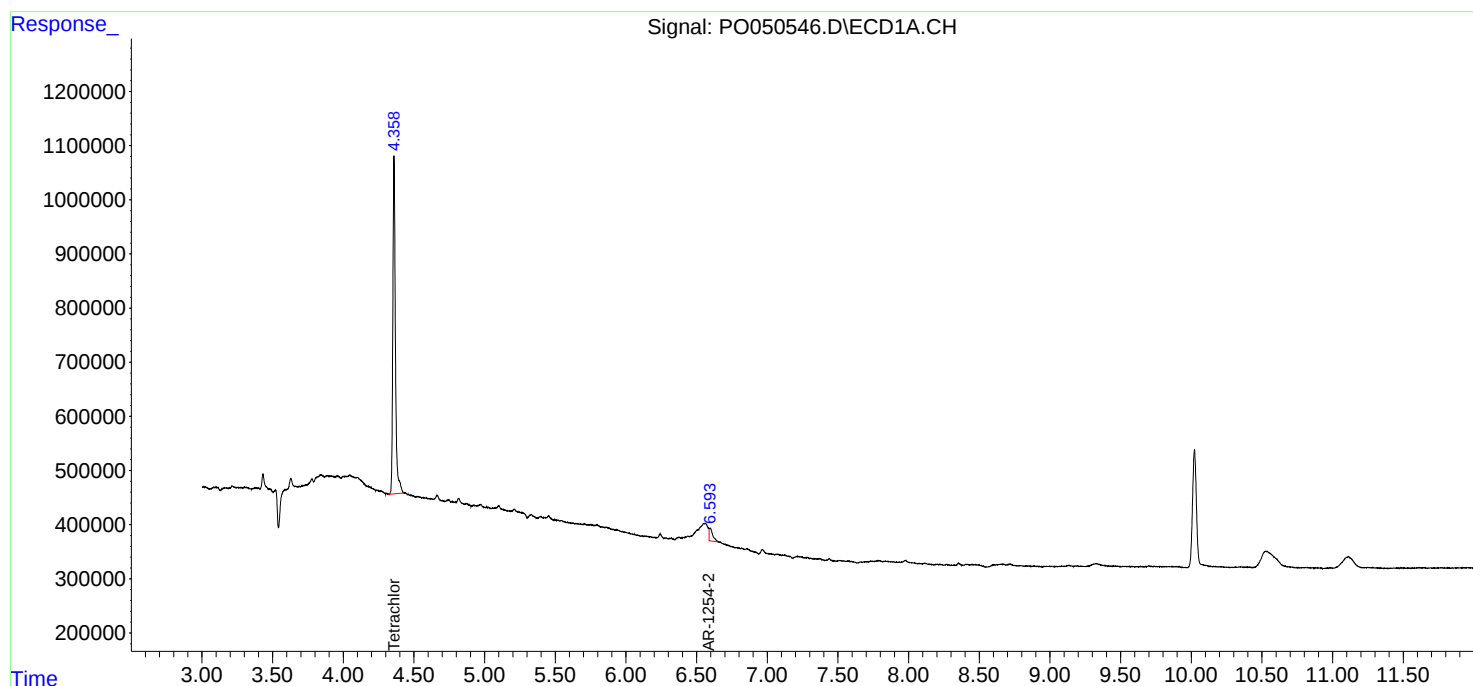


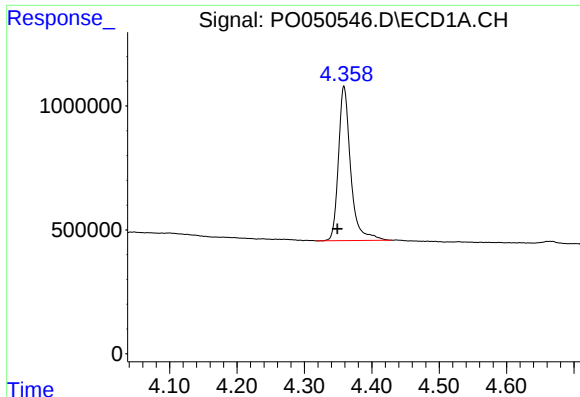

#1 Tetrachloro-m-xylene


R.T.: 4.359 min
Delta R.T.: 0.010 min
Response: 7839535
Conc: 26.27 ng/ml

Instrument :
ECD_O
ClientSampleId :

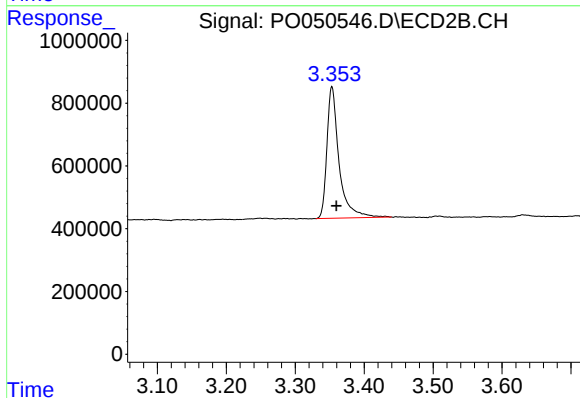


#1 Tetrachloro-m-xylene

R.T.: 3.353 min
Delta R.T.: -0.006 min
Response: 5132865
Conc: 26.11 ng/ml

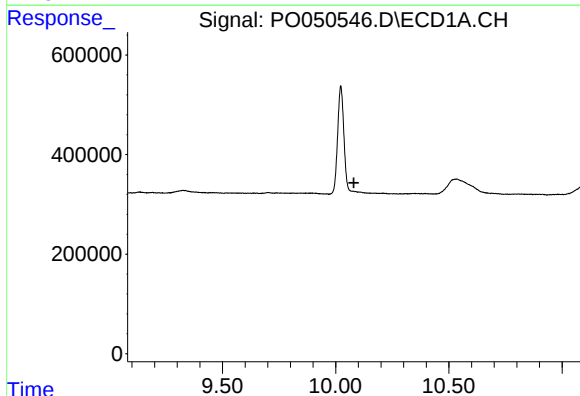


#2 Decachlorobiphenyl

R.T.: 10.022 min
Delta R.T.: -0.058 min
Response: -663989
Conc: N.D.

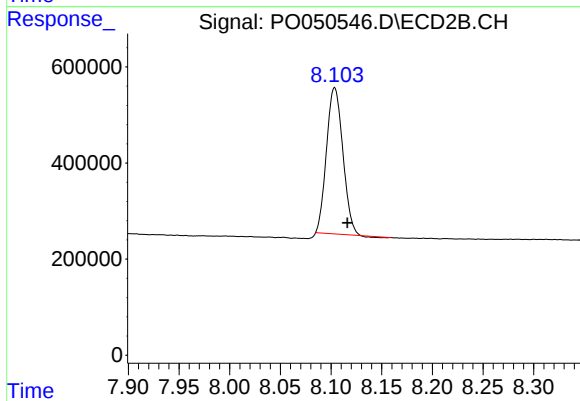

#2 Decachlorobiphenyl


R.T.: 8.104 min
Delta R.T.: -0.013 min
Response: 3401074
Conc: 17.79 ng/ml

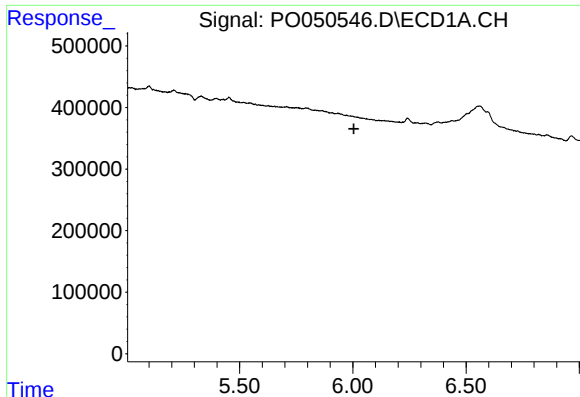

#7 AR-1016-5


R.T.: 0.000 min
Exp R.T.: 6.005 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

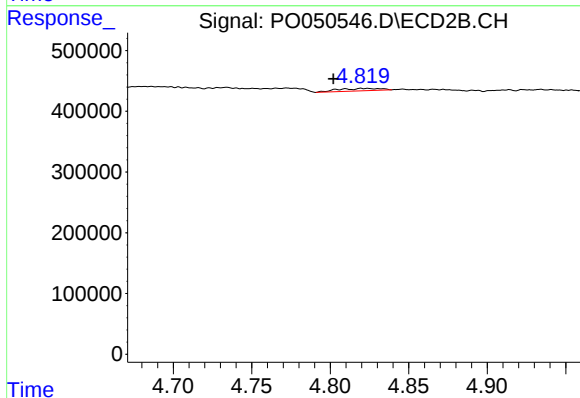


#7 AR-1016-5

R.T.: 4.820 min
Delta R.T.: 0.018 min
Response: 75723
Conc: 10.93 ng/ml

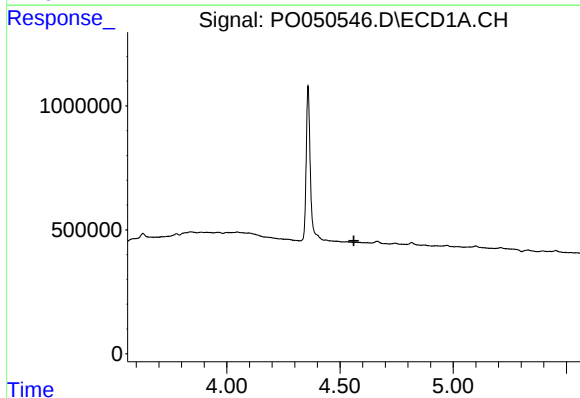


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T.: 4.561 min
Response: 0
Conc: N.D.

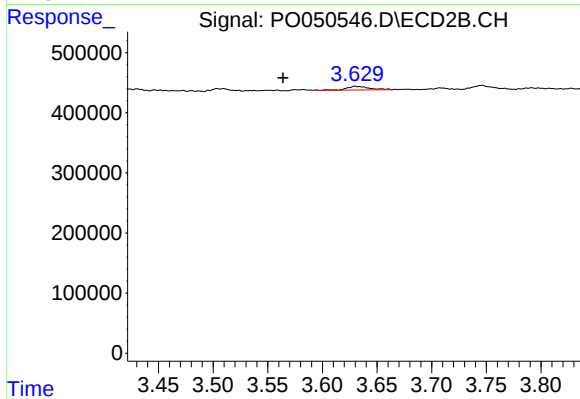

#8 AR-1221-1


R.T.: 3.630 min
Delta R.T.: 0.066 min
Response: 83672
Conc: 38.73 ng/ml

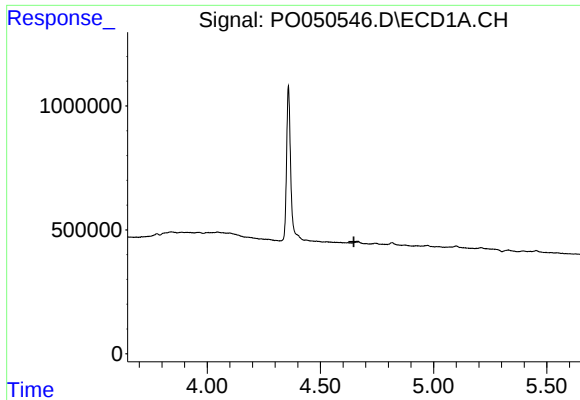

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T. : 4.648 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

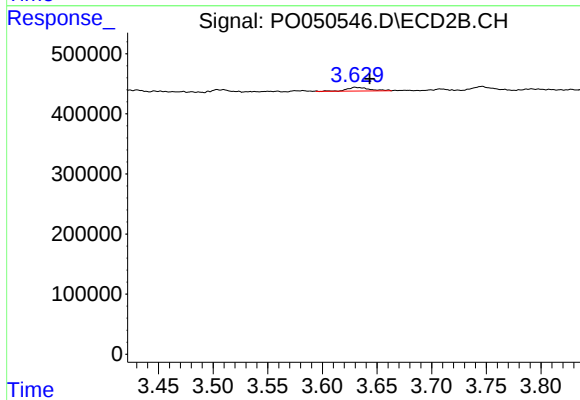


#9 AR-1221-2

R.T.: 3.630 min
Delta R.T.: -0.013 min
Response: 83672
Conc: 52.20 ng/ml

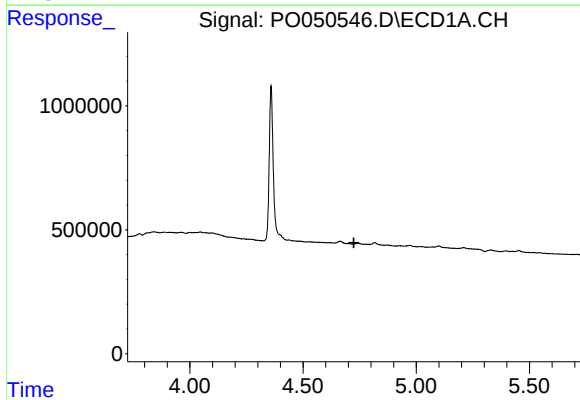


#10 AR-1221-3

R.T.: 0.000 min
Exp R.T. : 4.725 min
Response: 0
Conc: N.D.

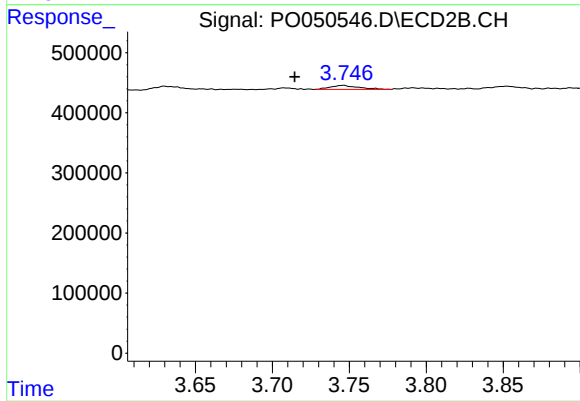

#10 AR-1221-3


R.T.: 3.746 min
Delta R.T.: 0.032 min
Response: 84541
Conc: 16.11 ng/ml

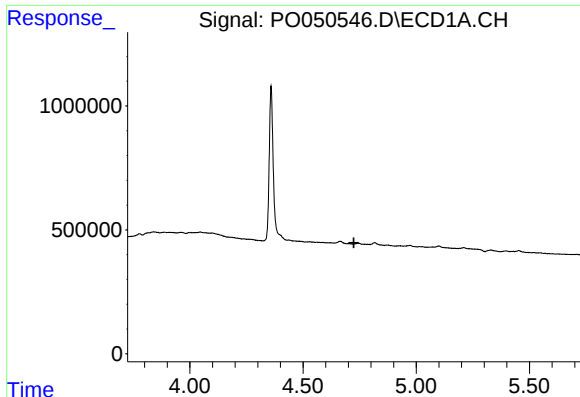

#11 AR-1232-1


R.T.: 0.000 min
Exp R.T. : 4.725 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

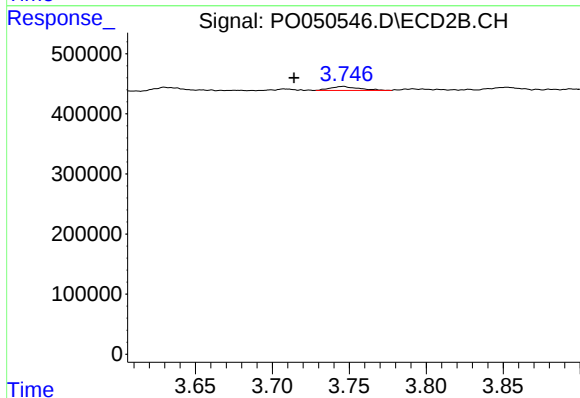


#11 AR-1232-1

R.T.: 3.746 min
Delta R.T.: 0.032 min
Response: 84541
Conc: 21.87 ng/ml

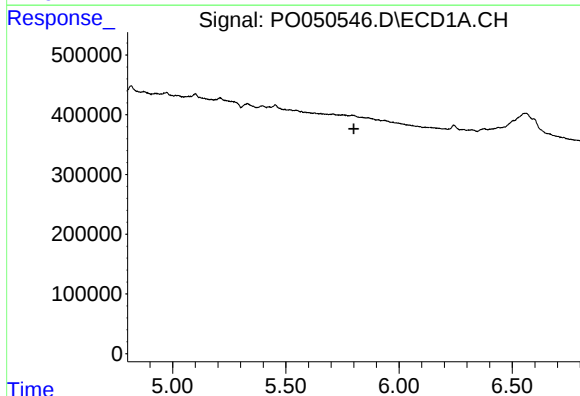


#15 AR-1232-5

R.T.: 0.000 min
Exp R.T. : 5.801 min
Response: 0
Conc: N.D.

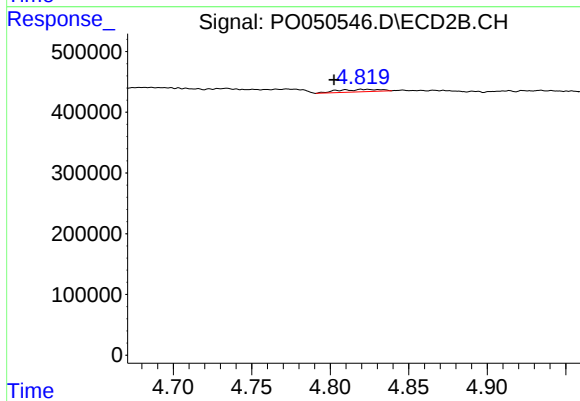

#15 AR-1232-5


R.T.: 4.820 min
Delta R.T.: 0.017 min
Response: 75723
Conc: 34.38 ng/ml

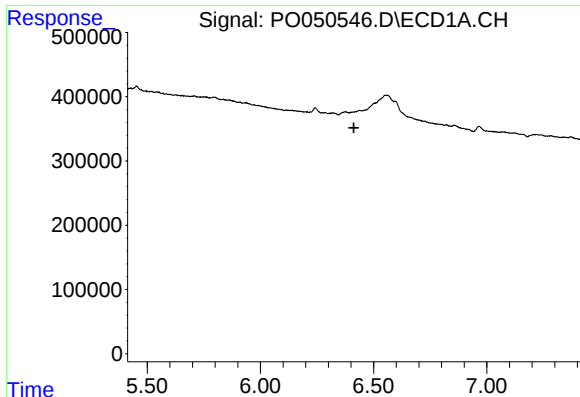

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T.: 6.413 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

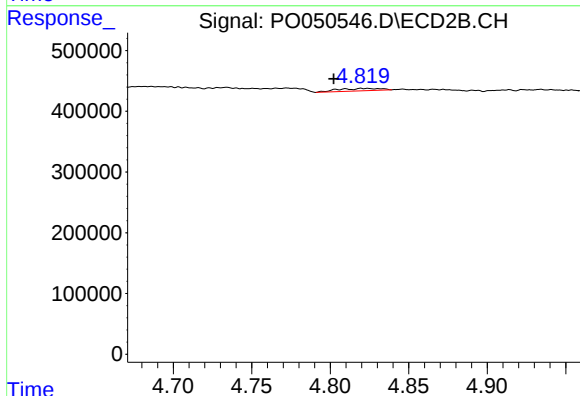


#24 AR-1248-4

R.T.: 4.820 min
Delta R.T.: 0.018 min
Response: 75723
Conc: 9.27 ng/ml

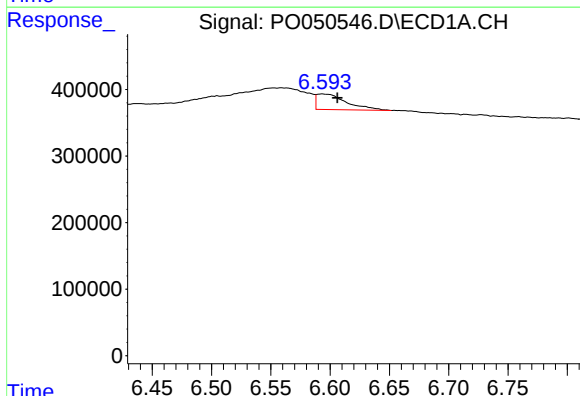

#27 AR-1254-2

R.T.: 6.594 min
Delta R.T.: -0.013 min
Response: 411611
Conc: 20.19 ng/ml

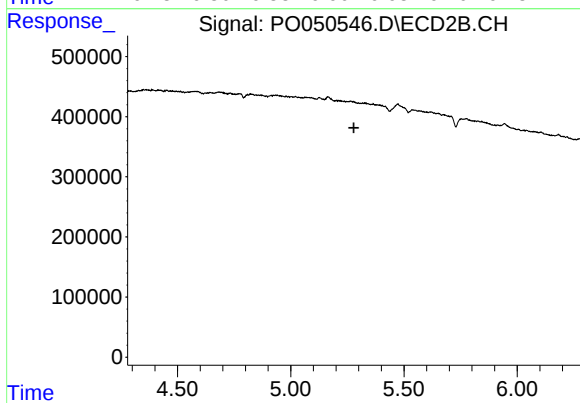

#27 AR-1254-2

R.T.: 0.000 min
Exp R.T.: 5.278 min
Response: 0
Conc: N.D.