

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0102518\
 Data File : P0050529.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 25 Oct 2018 12:47
 Operator : SM/SJ
 Sample : J5198-25RE
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CL-01-102318-CRE

Manual Integrations
 APPROVED

Sohil
 10/26/2018 5:57:41 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 25 13:19:50 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101818.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Oct 19 02:02:26 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.365	3.353	5573181	3445320	18.677m	17.524
2) SA Decachlor...	10.030	8.105	2515926	2010825	11.595m	10.520m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102518\
Data File : P0050529.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 Oct 2018 12:47
Operator : SM/SJ
Sample : J5198-25RE
Misc :
ALS Vial : 4 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
CL-01-102318-CRE


Manual Integrations
APPROVED

Sohil
10/26/2018 5:57:41 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 25 13:19:50 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101818.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Oct 19 02:02:26 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

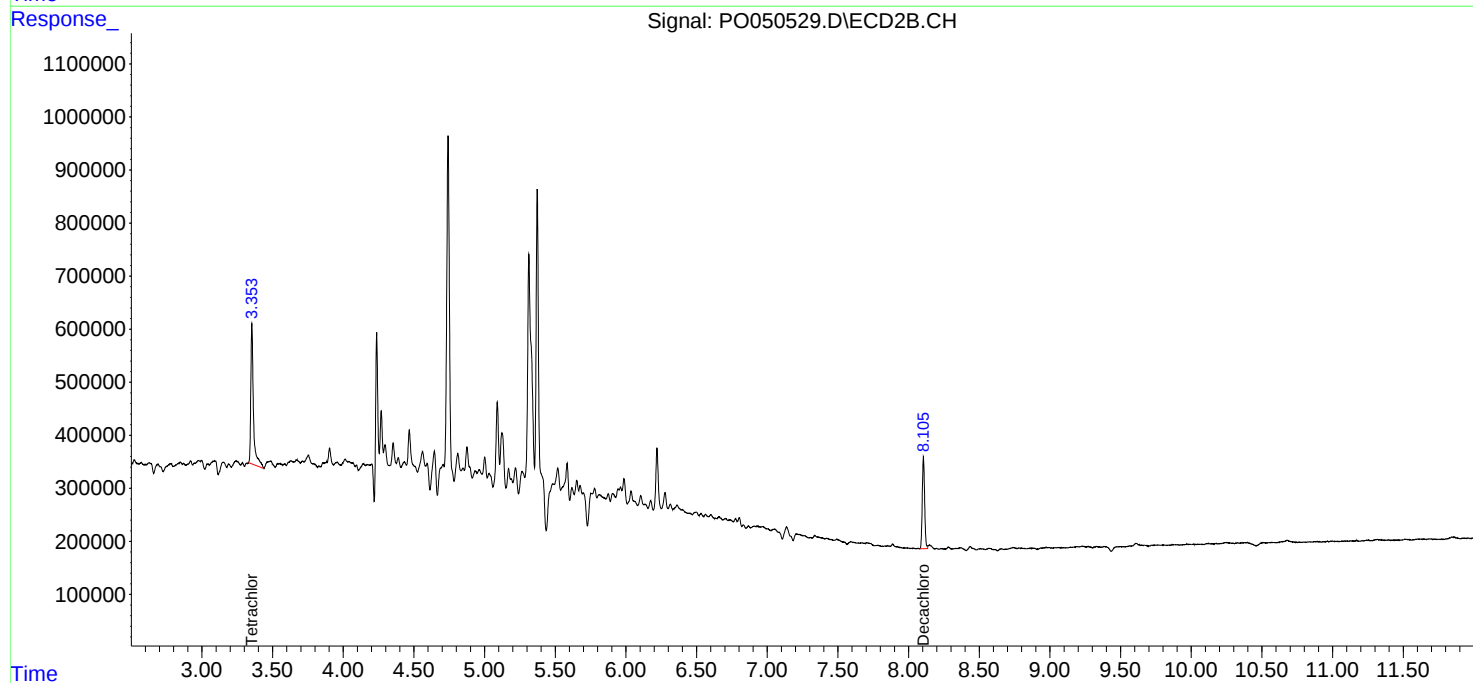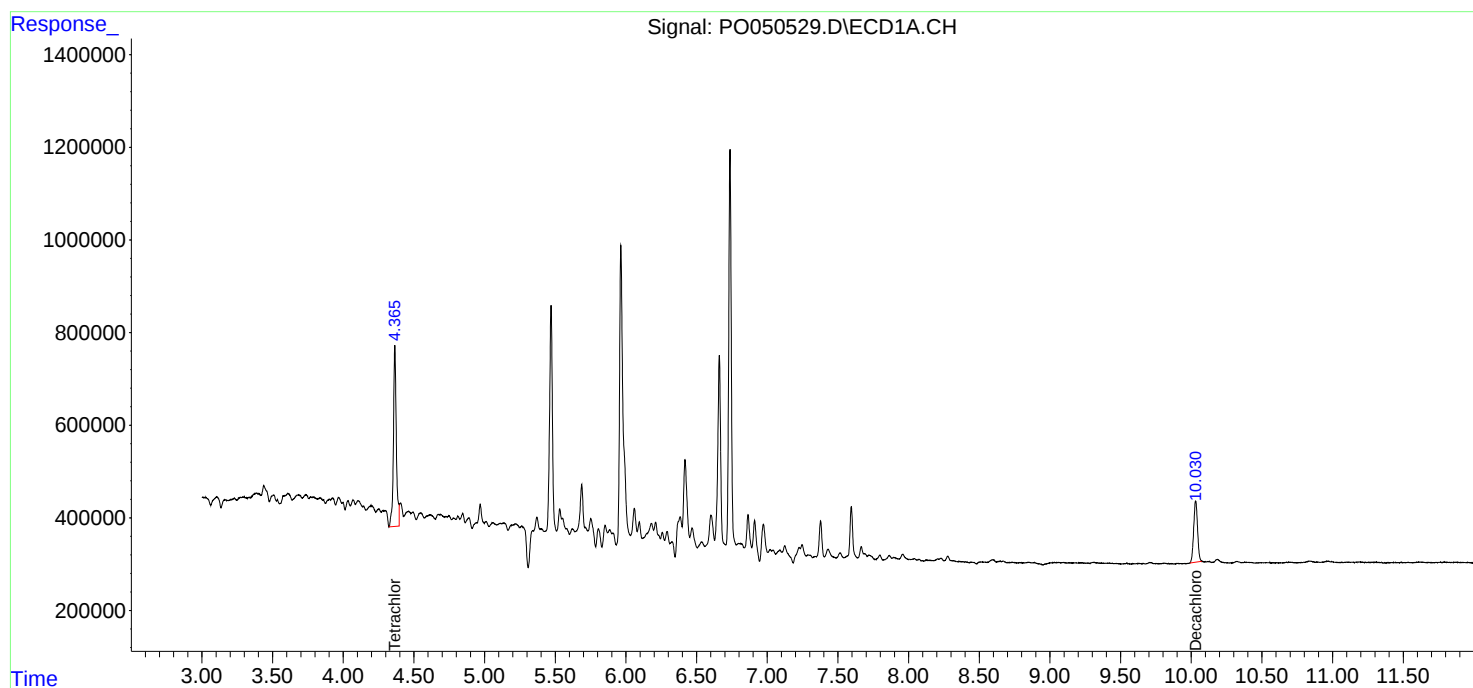

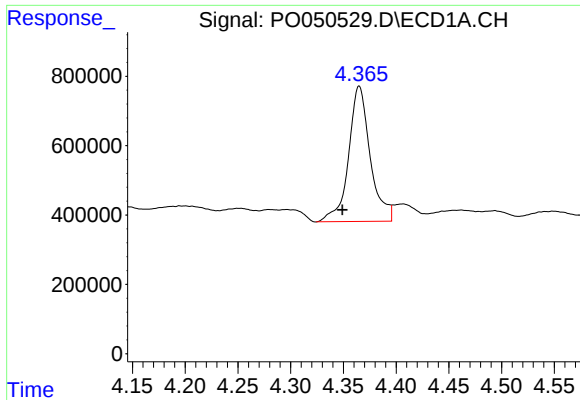


#1 Tetrachloro-m-xylene

R.T.: 4.365 min
Delta R.T.: 0.016 min
Response: 5573181
Conc: 18.68 ng/ml m

Instrument :
ECD_O
ClientSampleId :
CL-01-102318-CRE


Manual Integrations
APPROVED

Sohil
10/26/2018 5:57:41 PM

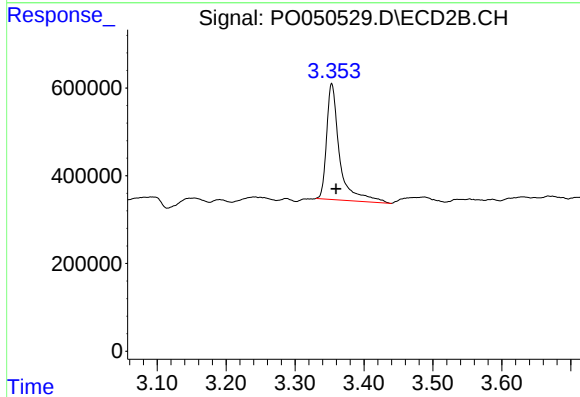


#1 Tetrachloro-m-xylene

R.T.: 3.353 min
Delta R.T.: -0.006 min
Response: 3445320
Conc: 17.52 ng/ml

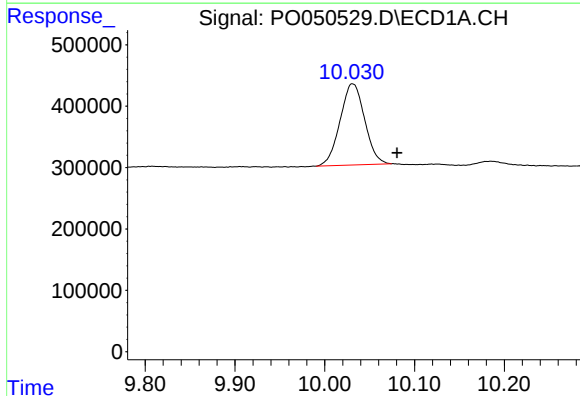

#2 Decachlorobiphenyl

R.T.: 10.030 min
Delta R.T.: -0.051 min
Response: 2515926
Conc: 11.59 ng/ml m

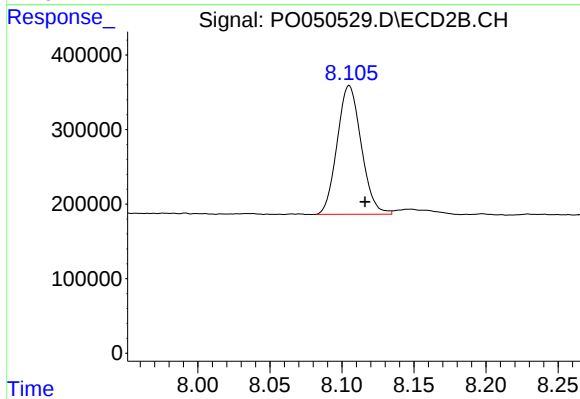

#2 Decachlorobiphenyl

R.T.: 8.105 min
Delta R.T.: -0.011 min
Response: 2010825
Conc: 10.52 ng/ml m