

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102521\
 Data File : P0082124.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 25 Oct 2021 10:55
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 26 02:53:01 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Oct 19 04:37:47 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.980	3.974	1785281	691804	22.094	23.447
2)	SA Decachlor...	11.097	9.300	1250467	675789	22.499	26.533
Target Compounds							
8)	L2 AR-1221-1	5.234	0.000	43687	0	50.552	N.D. #
9)	L2 AR-1221-2	5.338	0.000	34660	0	53.936	N.D. #
10)	L2 AR-1221-3	0.000	4.421	0	16780	N.D.	19.902 #
11)	L3 AR-1232-1	0.000	4.421	0	16780	N.D.	25.496 #
24)	L5 AR-1248-4	7.260	0.000	2285	0	0.969	N.D. #
26)	L6 AR-1254-1	7.242	0.000	8011	0	3.345	N.D. #
27)	L6 AR-1254-2	7.464	0.000	5795	0	1.589	N.D. #
28)	L6 AR-1254-3	7.840	0.000	1092	0	0.302	N.D. #
29)	L6 AR-1254-4	8.149	0.000	868	0	0.322	N.D. #
30)	L6 AR-1254-5	8.555f	0.000	6618	0	2.272	N.D. #
31)	L7 AR-1260-1	8.014	0.000	2177	0	0.771	N.D. #
32)	L7 AR-1260-2	8.276	0.000	9838	0	2.957	N.D. #
33)	L7 AR-1260-3	8.647	7.187	5479	26153	2.431	13.805 #
35)	L7 AR-1260-5	9.232	0.000	13790	0	2.517	N.D. #
36)	L8 AR-1262-1	8.647	0.000	5479	0	1.602	N.D. #
37)	L8 AR-1262-2	9.232	0.000	13790	0	2.196	N.D. #
38)	L8 AR-1262-3	9.548	0.000	9494	0	3.452	N.D. #
39)	L8 AR-1262-4	9.639	0.000	9936	0	5.934	N.D. #
41)	L9 AR-1268-1	9.548	0.000	9494	0	1.271	N.D. #
42)	L9 AR-1268-2	9.639	0.000	9936	0	1.469	N.D. #
43)	L9 AR-1268-3	9.859	0.000	5097	0	0.863	N.D. #
45)	L9 AR-1268-5	10.760	0.000	8503	0	0.423	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102521\
Data File : P0082124.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 Oct 2021 10:55
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampled :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 26 02:53:01 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101821.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Oct 19 04:37:47 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

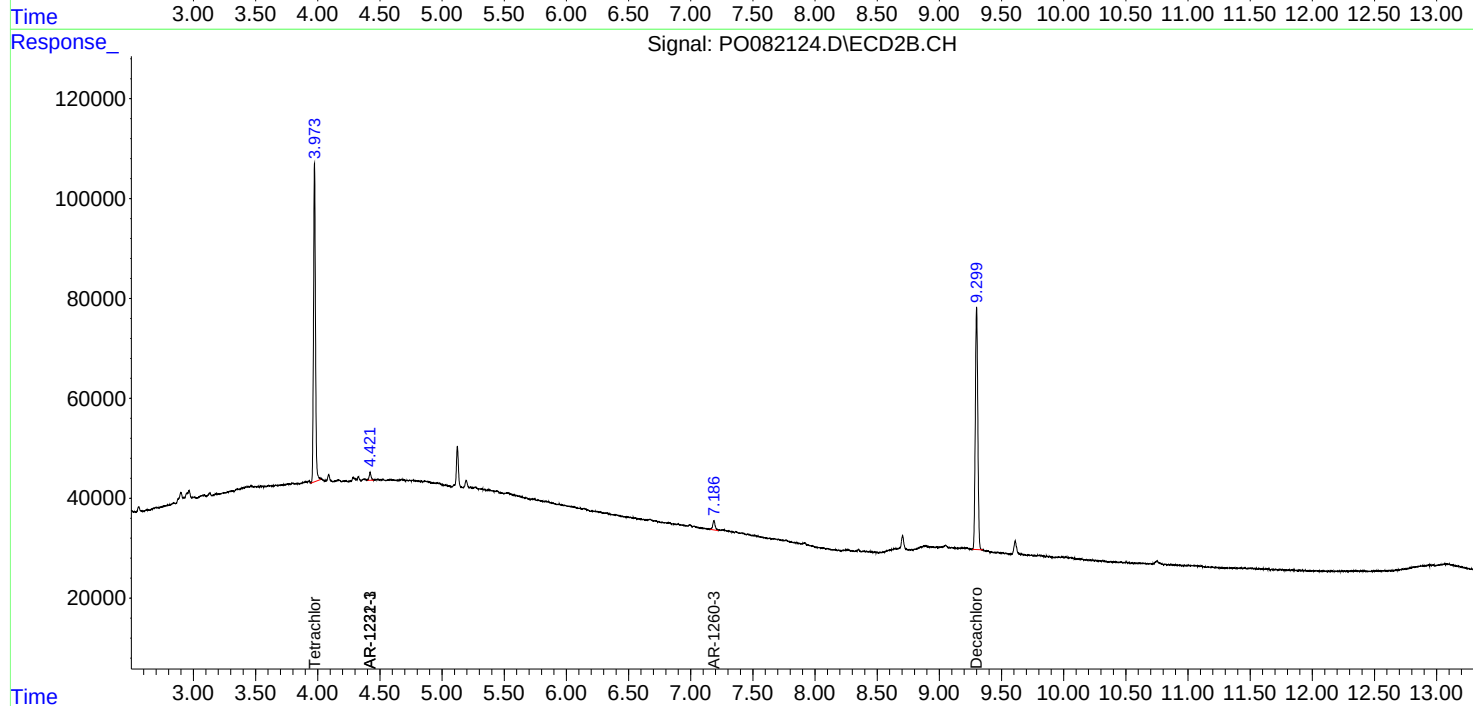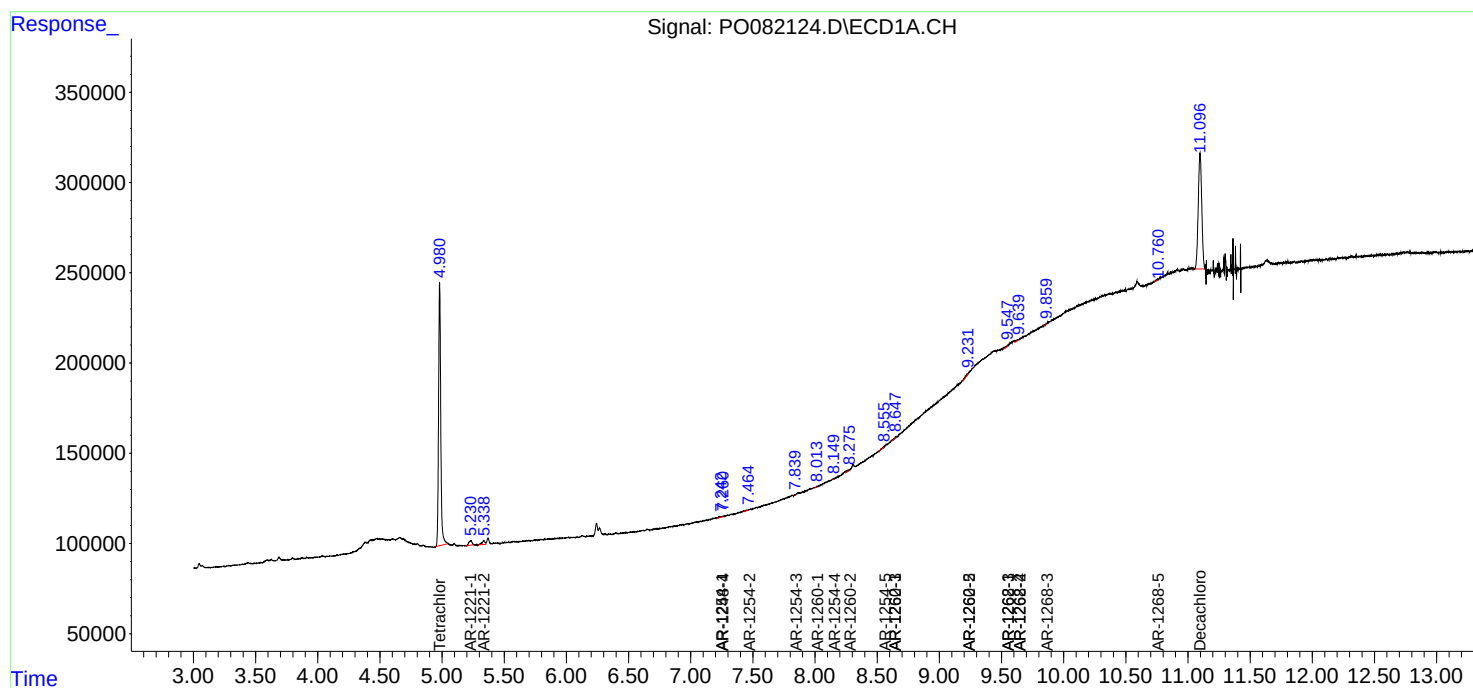


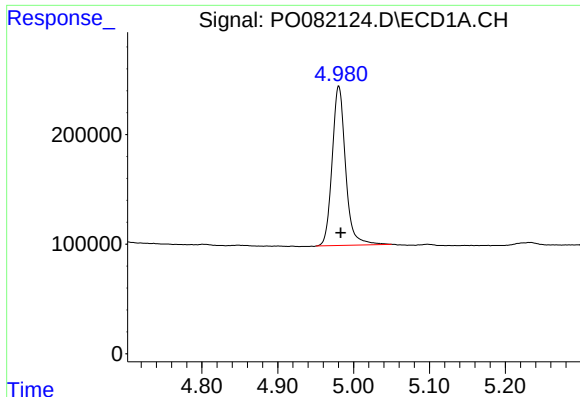

#1 Tetrachloro-m-xylene


R.T.: 4.980 min
Delta R.T.: -0.003 min
Response: 1785281
Conc: 22.09 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

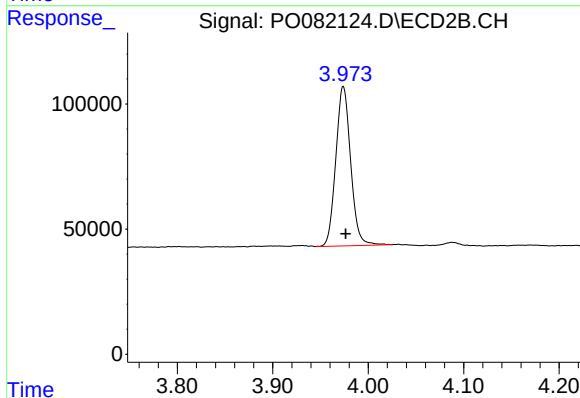


#1 Tetrachloro-m-xylene

R.T.: 3.974 min
Delta R.T.: -0.003 min
Response: 691804
Conc: 23.45 ng/ml

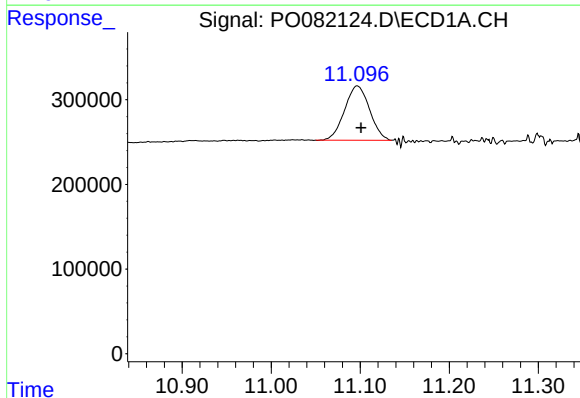


#2 Decachlorobiphenyl

R.T.: 11.097 min
Delta R.T.: -0.004 min
Response: 1250467
Conc: 22.50 ng/ml

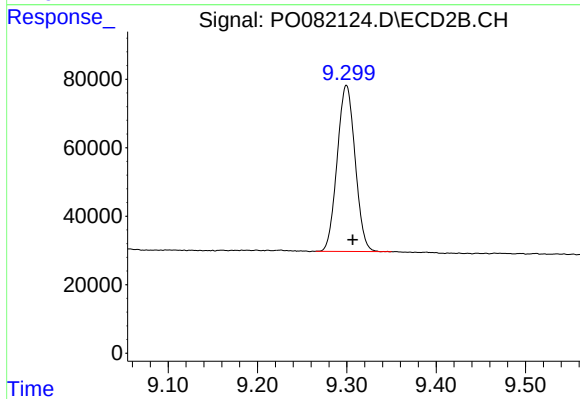

#2 Decachlorobiphenyl


R.T.: 9.300 min
Delta R.T.: -0.007 min
Response: 675789
Conc: 26.53 ng/ml

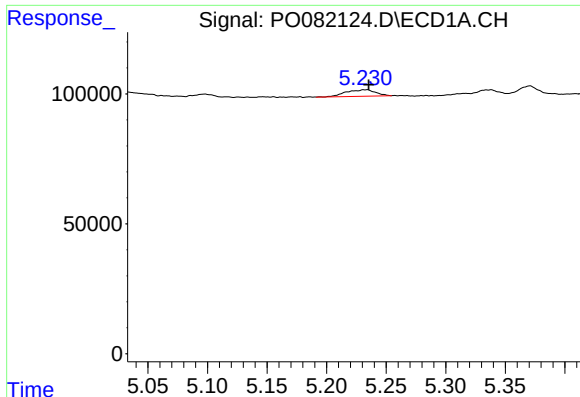

#8 AR-1221-1


R.T.: 5.234 min
Delta R.T.: -0.001 min
Response: 43687
Conc: 50.55 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

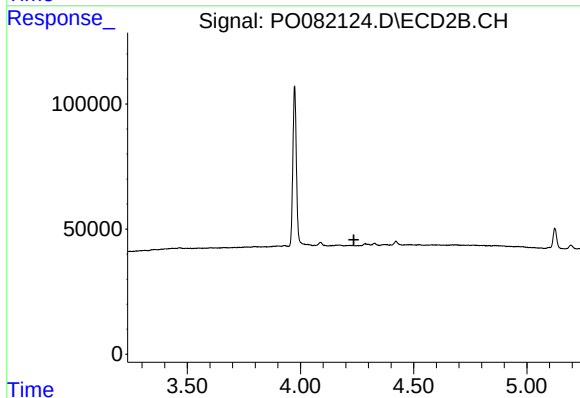


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.236 min
Response: 0
Conc: N.D.

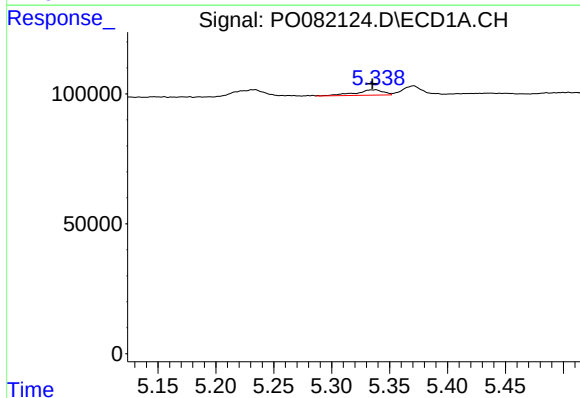


#9 AR-1221-2

R.T.: 5.338 min
Delta R.T.: 0.003 min
Response: 34660
Conc: 53.94 ng/ml

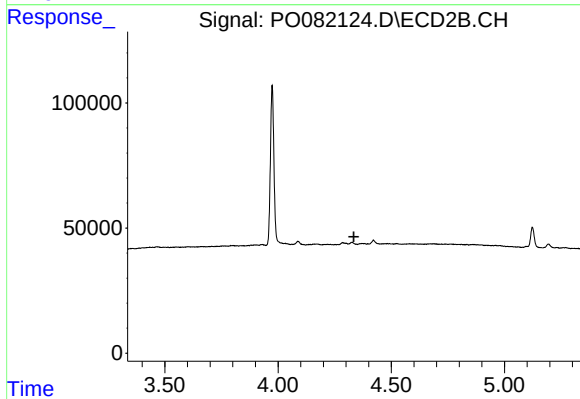

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T. : 4.335 min
Response: 0
Conc: N.D.

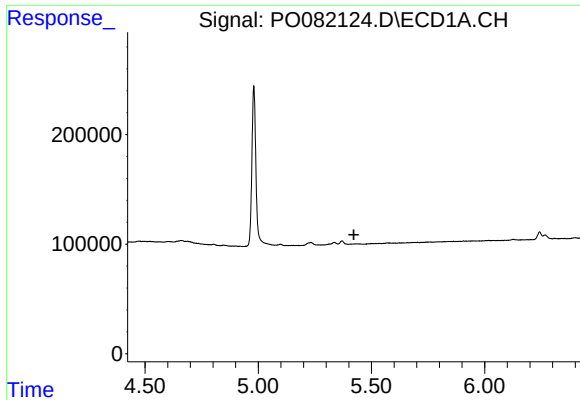

#10 AR-1221-3


R.T.: 0.000 min
Exp R.T. : 5.422 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

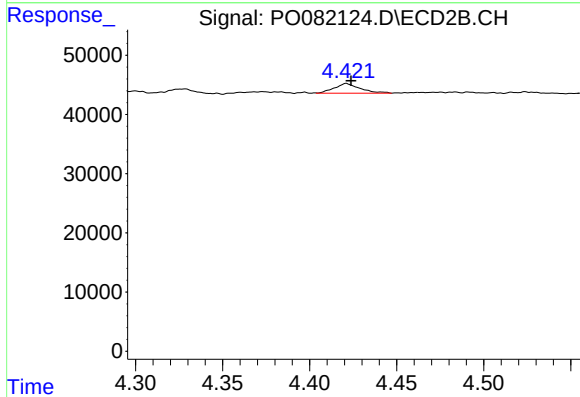


#10 AR-1221-3

R.T.: 4.421 min
Delta R.T.: -0.003 min
Response: 16780
Conc: 19.90 ng/ml

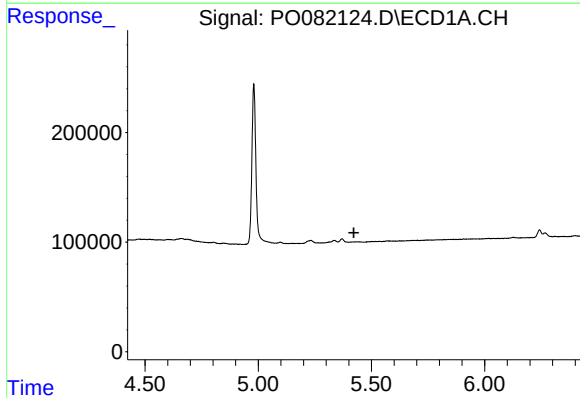


#11 AR-1232-1

R.T.: 0.000 min
Exp R.T. : 5.422 min
Response: 0
Conc: N.D.

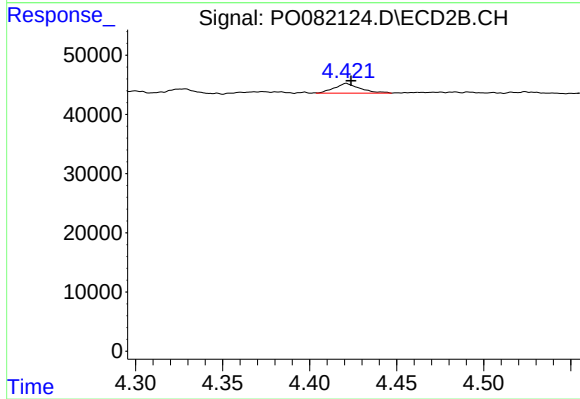

#11 AR-1232-1


R.T.: 4.421 min
Delta R.T.: -0.003 min
Response: 16780
Conc: 25.50 ng/ml

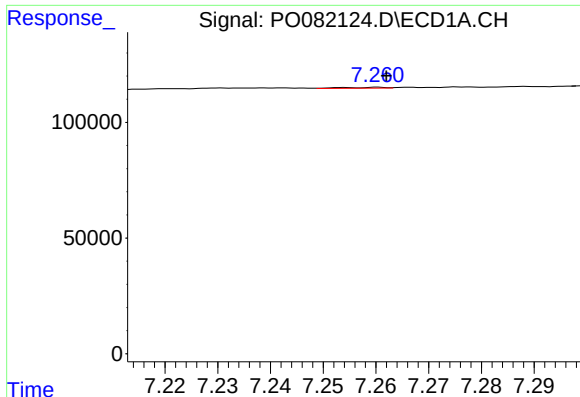

#24 AR-1248-4


R.T.: 7.260 min
Delta R.T.: -0.002 min
Response: 2285
Conc: 0.97 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

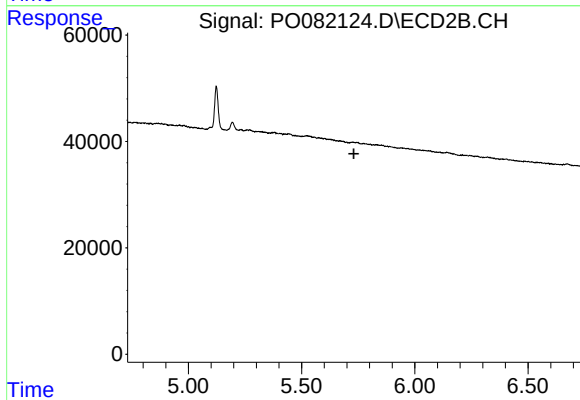


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T. : 5.731 min
Response: 0
Conc: N.D.

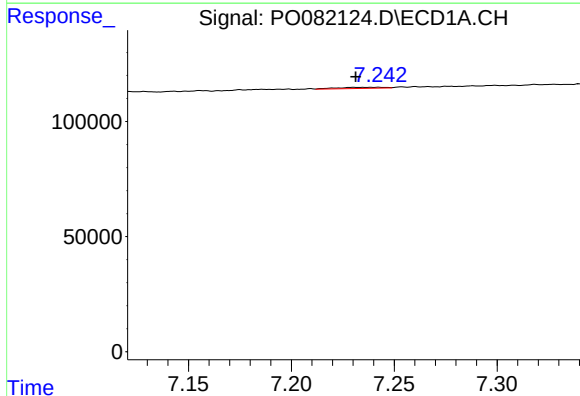


#26 AR-1254-1

R.T.: 7.242 min
Delta R.T.: 0.011 min
Response: 8011
Conc: 3.34 ng/ml

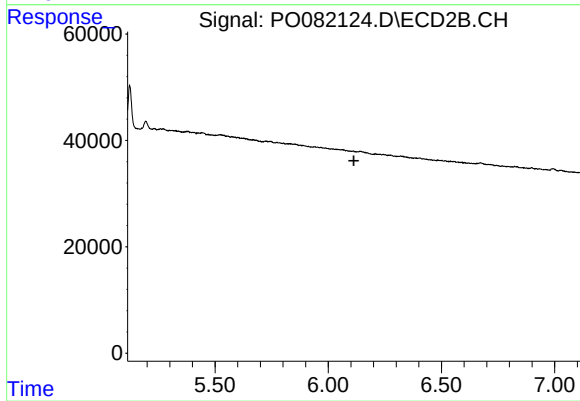

#26 AR-1254-1


R.T.: 0.000 min
Exp R.T. : 6.113 min
Response: 0
Conc: N.D.

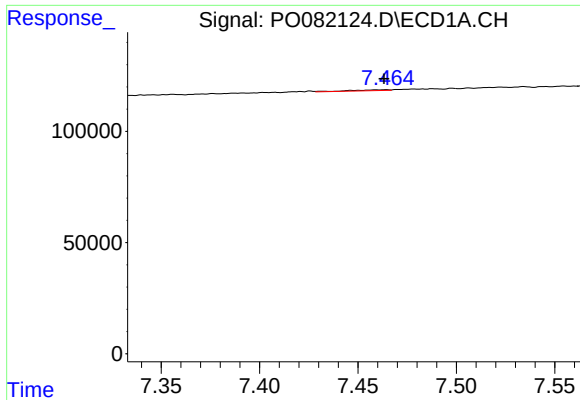

#27 AR-1254-2


R.T.: 7.464 min
Delta R.T.: 0.001 min
Response: 5795
Conc: 1.59 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

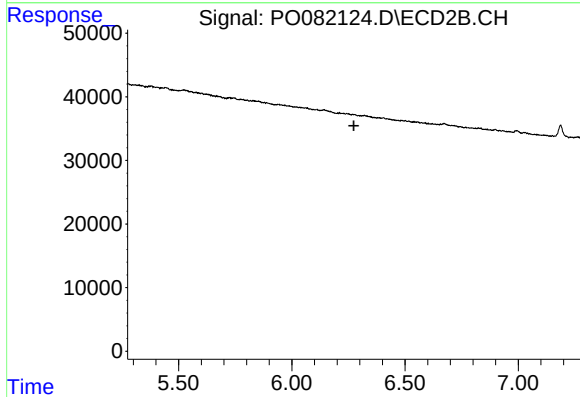


#27 AR-1254-2

R.T.: 0.000 min
Exp R.T. : 6.274 min
Response: 0
Conc: N.D.

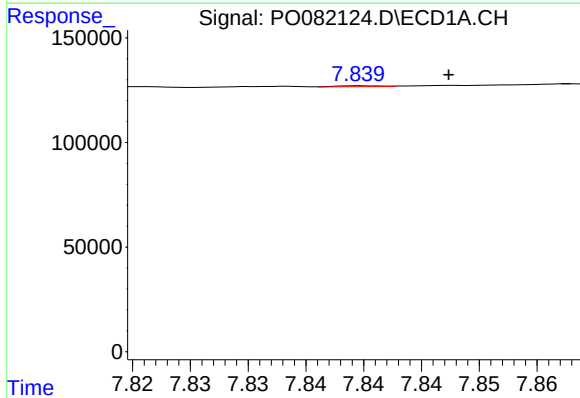


#28 AR-1254-3

R.T.: 7.840 min
Delta R.T.: -0.008 min
Response: 1092
Conc: 0.30 ng/ml

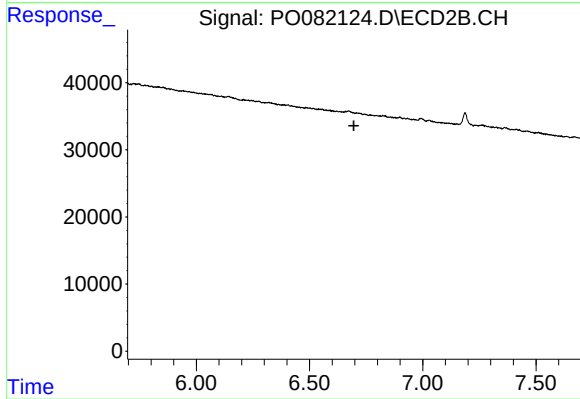

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T. : 6.696 min
Response: 0
Conc: N.D.

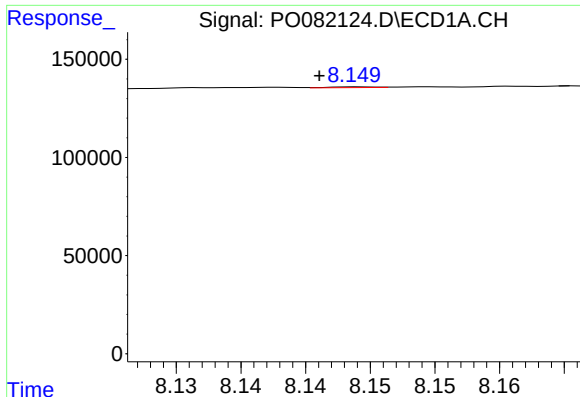

#29 AR-1254-4


R.T.: 8.149 min
Delta R.T.: 0.003 min
Response: 868
Conc: 0.32 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

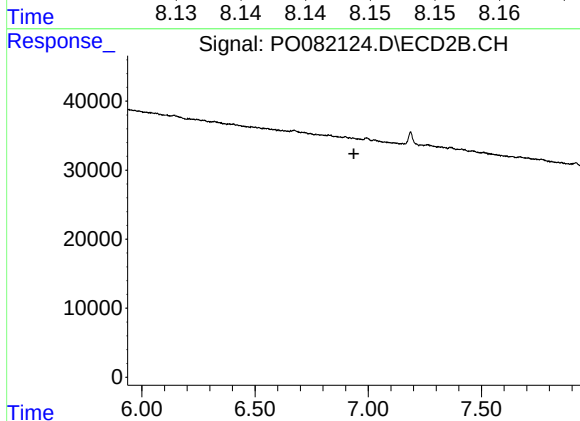


#29 AR-1254-4

R.T.: 0.000 min
Exp R.T. : 6.937 min
Response: 0
Conc: N.D.

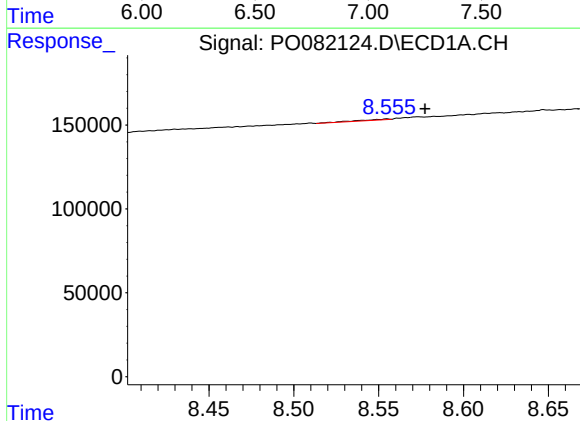


#30 AR-1254-5

R.T.: 8.555 min
Delta R.T.: -0.022 min
Response: 6618
Conc: 2.27 ng/ml

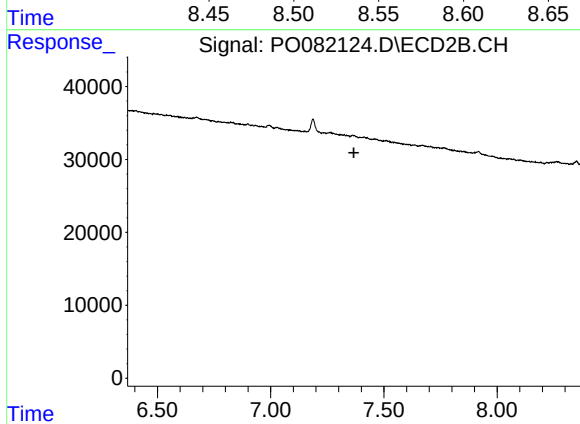

#30 AR-1254-5


R.T.: 0.000 min
Exp R.T. : 7.367 min
Response: 0
Conc: N.D.

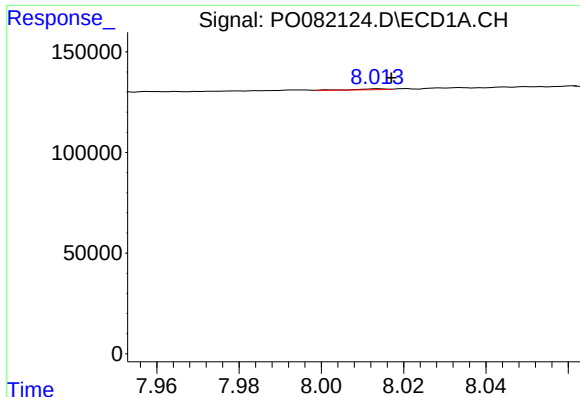

#31 AR-1260-1


R.T.: 8.014 min
Delta R.T.: -0.003 min
Response: 2177
Conc: 0.77 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

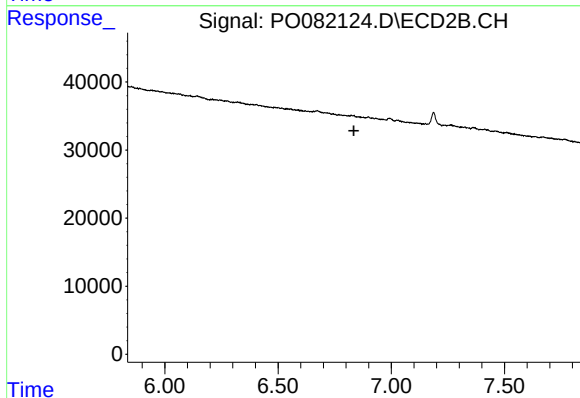


#31 AR-1260-1

R.T.: 0.000 min
Exp R.T. : 6.835 min
Response: 0
Conc: N.D.

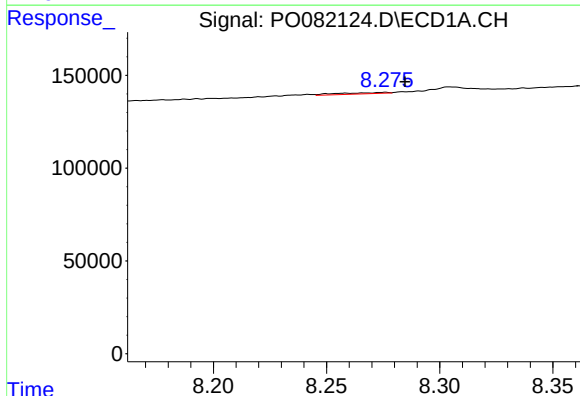


#32 AR-1260-2

R.T.: 8.276 min
Delta R.T.: -0.009 min
Response: 9838
Conc: 2.96 ng/ml

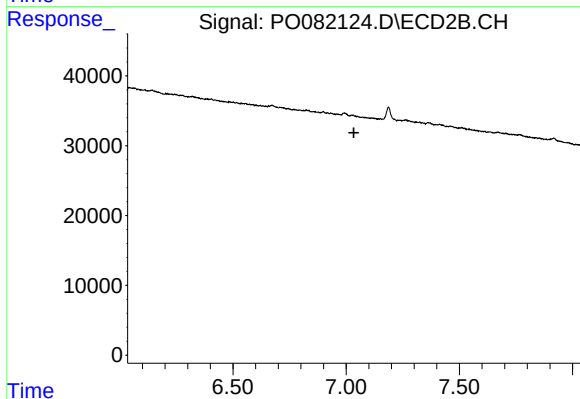

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T. : 7.034 min
Response: 0
Conc: N.D.

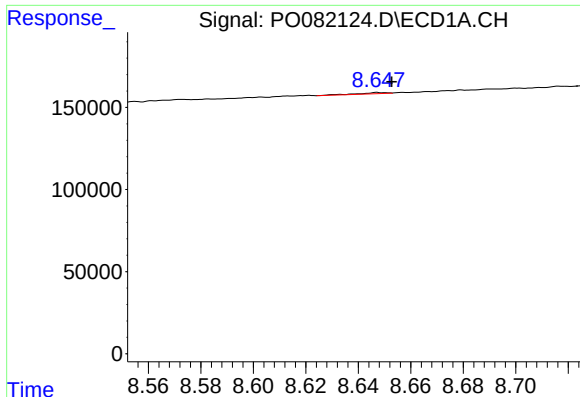

#33 AR-1260-3


R.T.: 8.647 min
Delta R.T.: -0.006 min
Response: 5479
Conc: 2.43 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

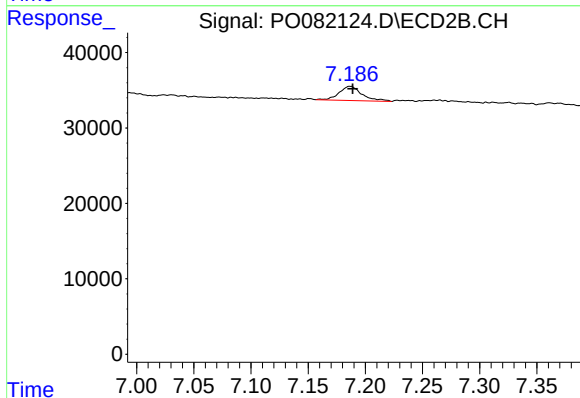


#33 AR-1260-3

R.T.: 7.187 min
Delta R.T.: -0.002 min
Response: 26153
Conc: 13.81 ng/ml

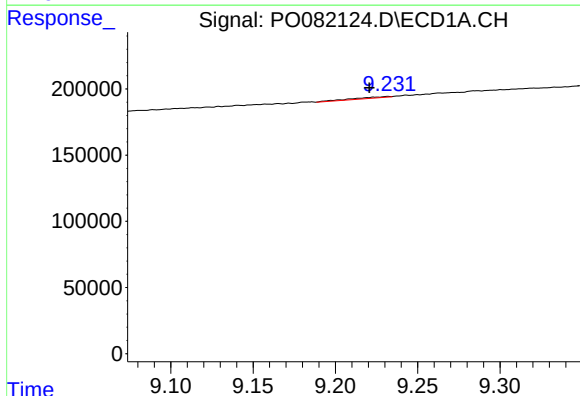


#35 AR-1260-5

R.T.: 9.232 min
Delta R.T.: 0.011 min
Response: 13790
Conc: 2.52 ng/ml

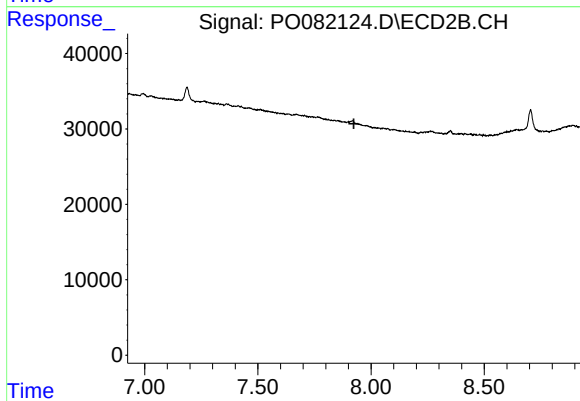

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T.: 7.924 min
Response: 0
Conc: N.D.

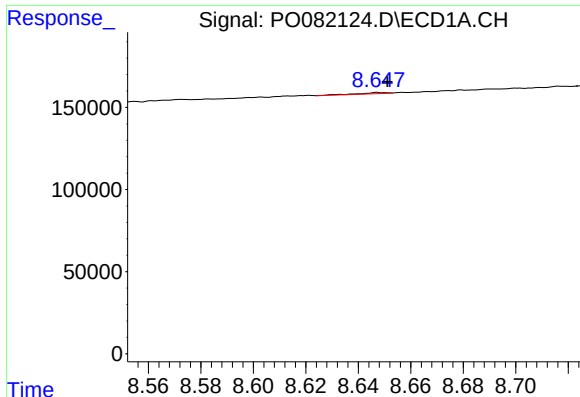

#36 AR-1262-1


R.T.: 8.647 min
Delta R.T.: -0.004 min
Response: 5479
Conc: 1.60 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

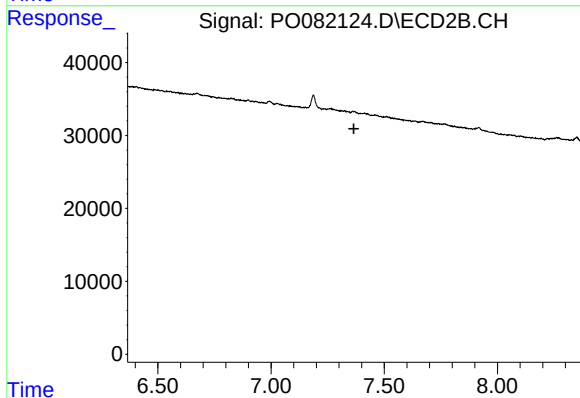


#36 AR-1262-1

R.T.: 0.000 min
Exp R.T. : 7.366 min
Response: 0
Conc: N.D.

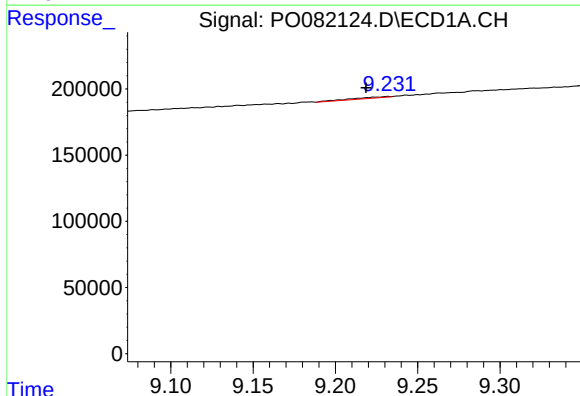


#37 AR-1262-2

R.T.: 9.232 min
Delta R.T.: 0.013 min
Response: 13790
Conc: 2.20 ng/ml

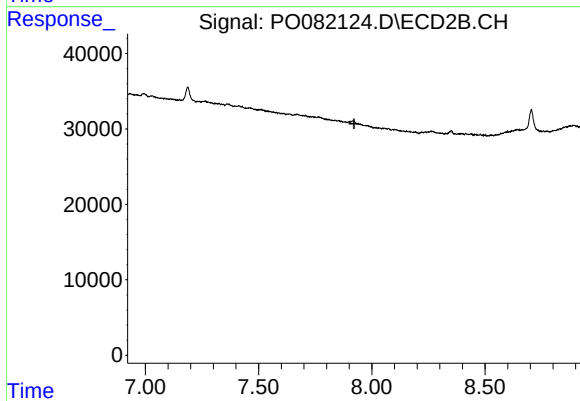

#37 AR-1262-2


R.T.: 0.000 min
Exp R.T. : 7.921 min
Response: 0
Conc: N.D.

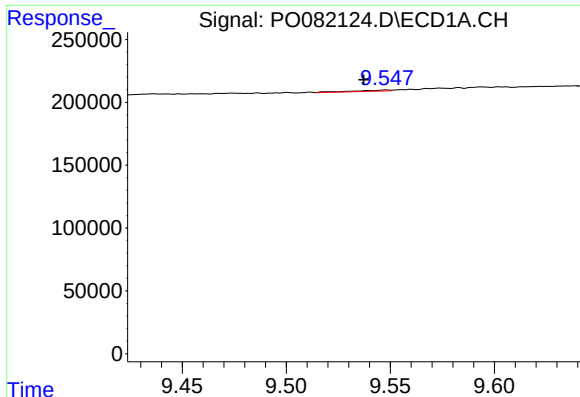

#38 AR-1262-3


R.T.: 9.548 min
Delta R.T.: 0.011 min
Response: 9494
Conc: 3.45 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

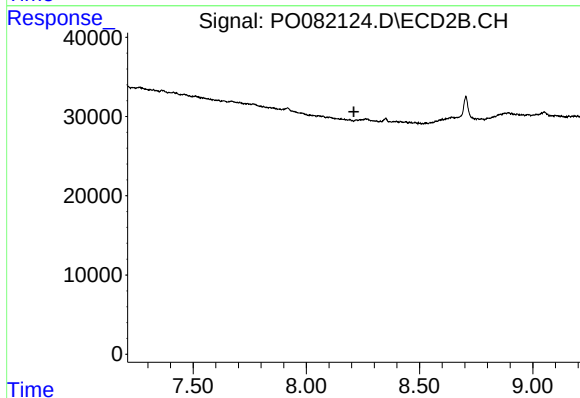


#38 AR-1262-3

R.T.: 0.000 min
Exp R.T. : 8.210 min
Response: 0
Conc: N.D.

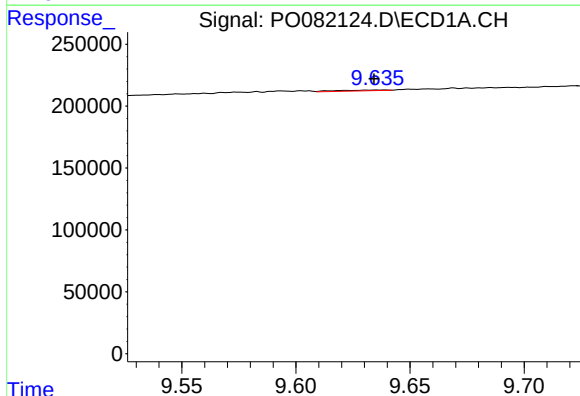


#39 AR-1262-4

R.T.: 9.639 min
Delta R.T.: 0.005 min
Response: 9936
Conc: 5.93 ng/ml

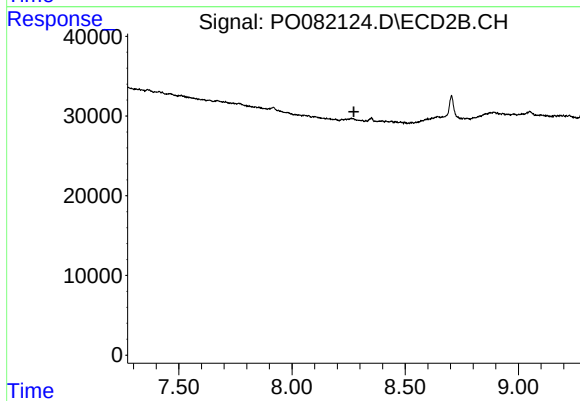

#39 AR-1262-4


R.T.: 0.000 min
Exp R.T. : 8.274 min
Response: 0
Conc: N.D.

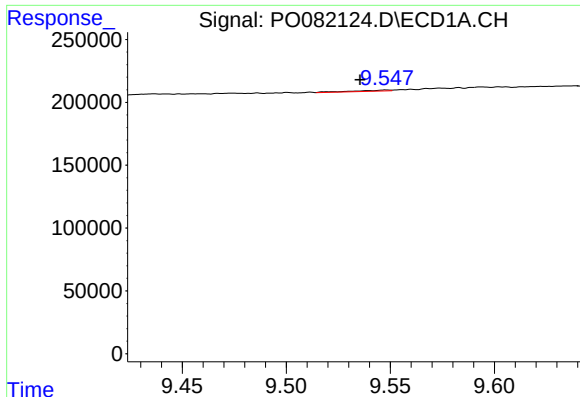

#41 AR-1268-1


R.T.: 9.548 min
Delta R.T.: 0.013 min
Response: 9494
Conc: 1.27 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

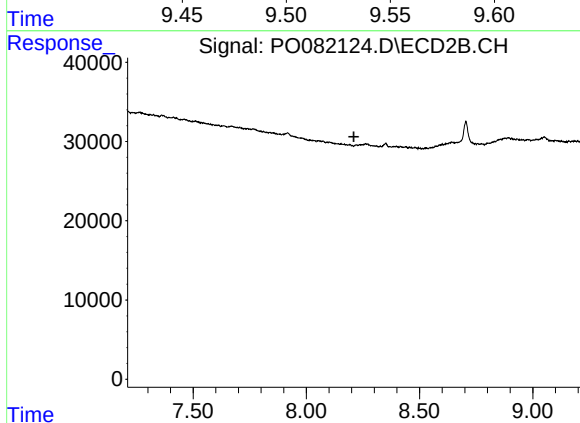


#41 AR-1268-1

R.T.: 0.000 min
Exp R.T. : 8.210 min
Response: 0
Conc: N.D.

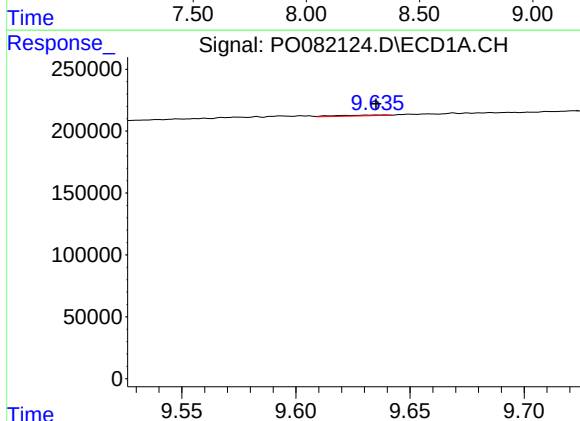


#42 AR-1268-2

R.T.: 9.639 min
Delta R.T.: 0.004 min
Response: 9936
Conc: 1.47 ng/ml

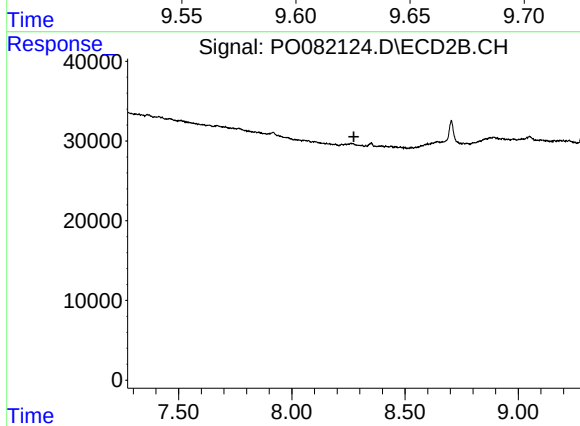

#42 AR-1268-2


R.T.: 0.000 min
Exp R.T. : 8.274 min
Response: 0
Conc: N.D.

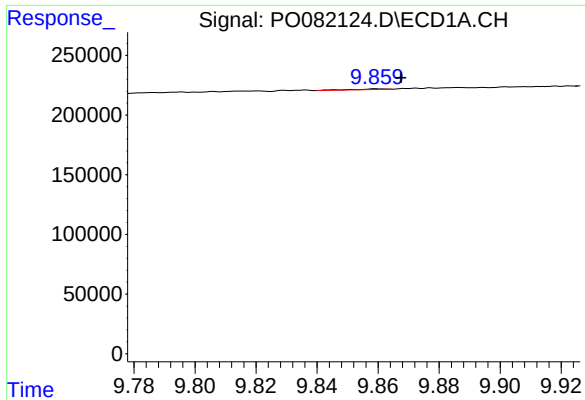

#43 AR-1268-3


R.T.: 9.859 min
Delta R.T.: -0.008 min
Response: 5097
Conc: 0.86 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

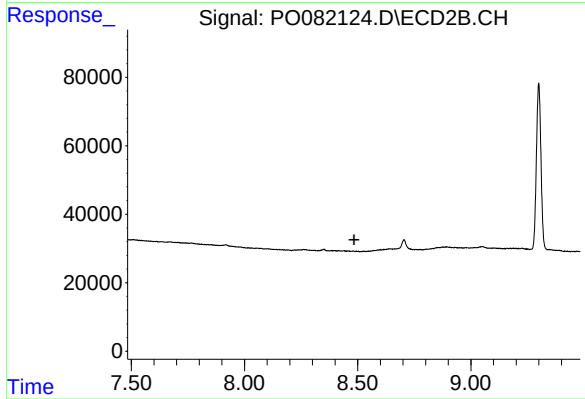


#43 AR-1268-3

R.T.: 0.000 min
Exp R.T. : 8.484 min
Response: 0
Conc: N.D.

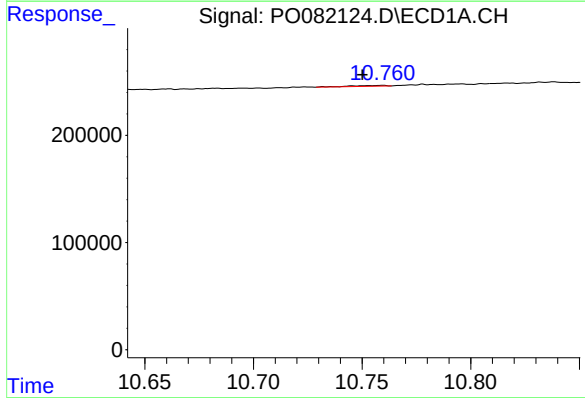

#45 AR-1268-5

R.T.: 10.760 min
Delta R.T.: 0.010 min
Response: 8503
Conc: 0.42 ng/ml

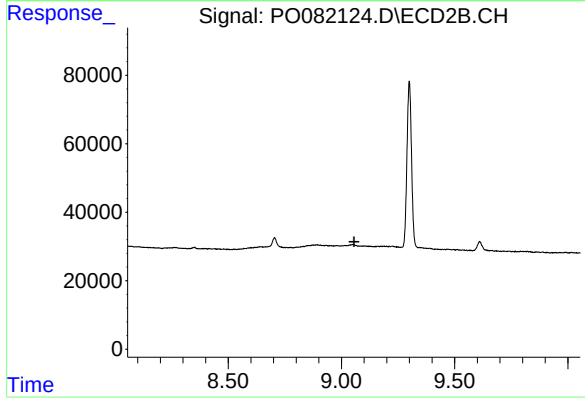

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T. : 9.055 min
Response: 0
Conc: N.D.