

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0102521\
 Data File : P0082147.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 25 Oct 2021 18:06
 Operator : AJ\MA
 Sample : M4332-14
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 BB-SAMPLE-4

Manual Integrations
 APPROVED

mohammad
 10/26/2021 10:36:56 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 26 03:01:26 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Oct 19 04:37:47 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.981	3.975	2353896	737962	29.131m	25.012
2) SA Decachlor...	11.103	9.302	1262135	584110	22.709	22.933

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102521\
Data File : PO082147.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 Oct 2021 18:06
Operator : AJ\MA
Sample : M4332-14
Misc :
ALS Vial : 24 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
BB-SAMPLE-4


Manual Integrations
APPROVED

mohammad
10/26/2021 10:36:56 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 26 03:01:26 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101821.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Oct 19 04:37:47 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

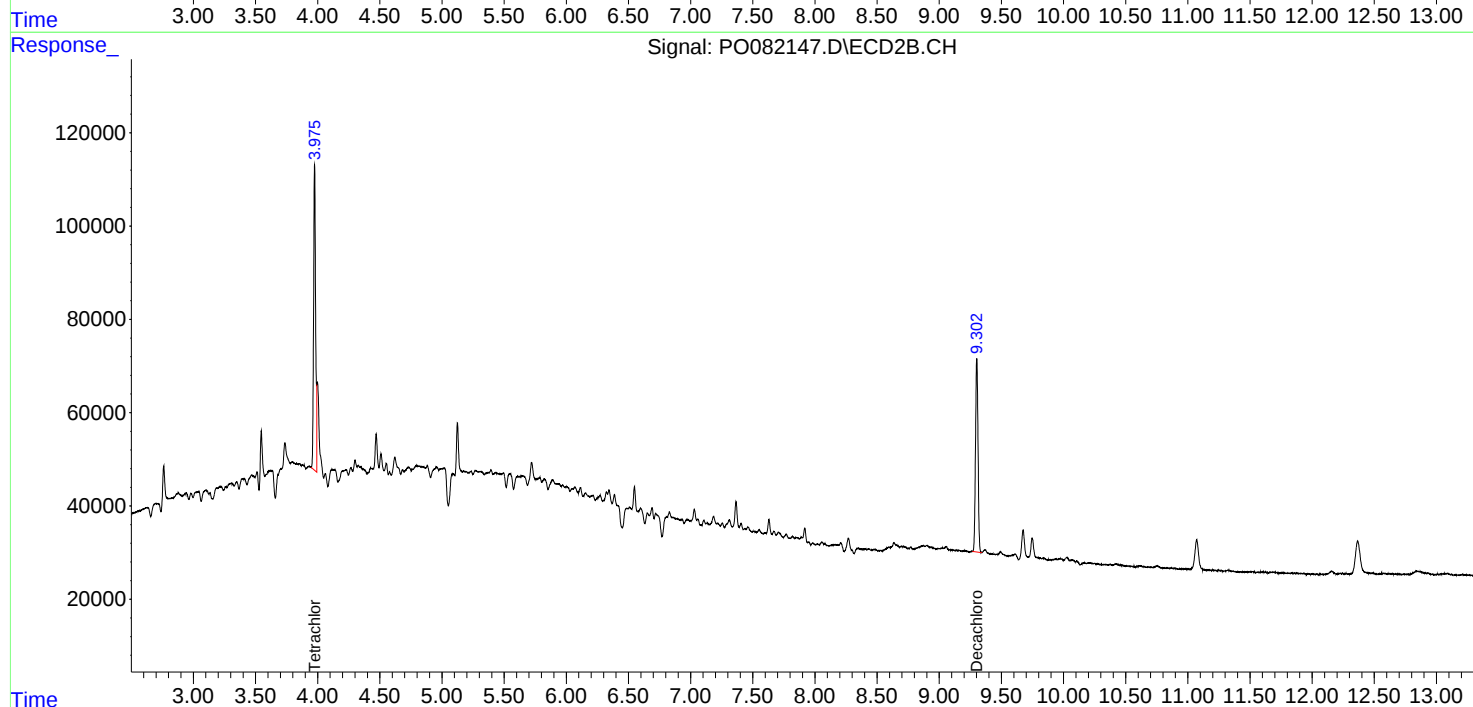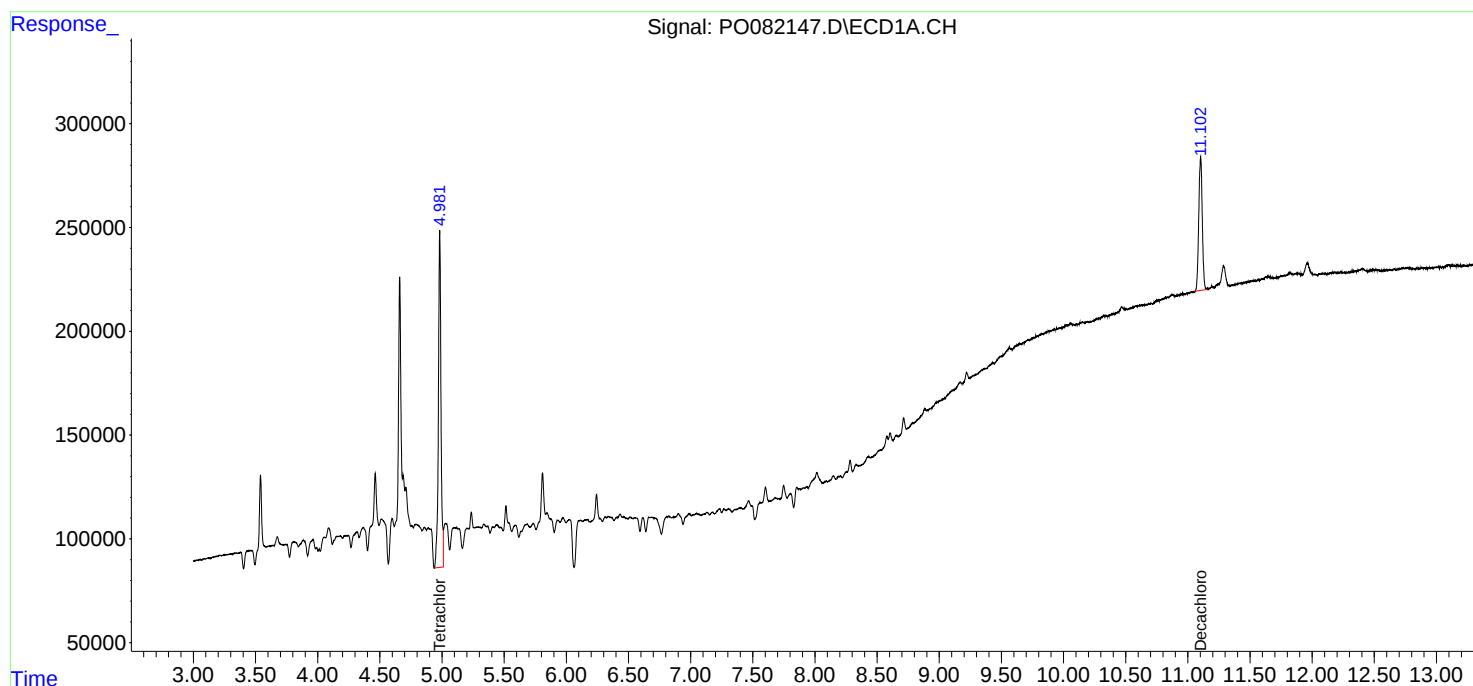

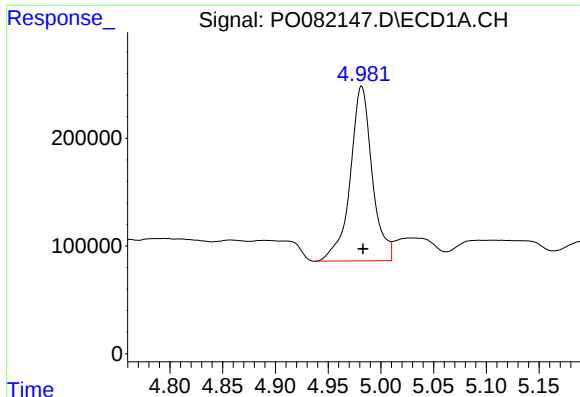


#1 Tetrachloro-m-xylene

R.T.: 4.981 min
Delta R.T.: -0.002 min
Response: 2353896
Conc: 29.13 ng/ml m

Instrument :
ECD_O
ClientSampleId :
BB-SAMPLE-4


Manual Integrations
APPROVED

mohammad
10/26/2021 10:36:56 AM

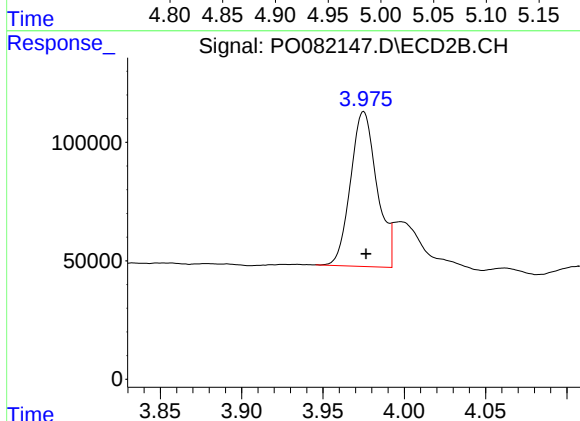


#1 Tetrachloro-m-xylene

R.T.: 3.975 min
Delta R.T.: -0.001 min
Response: 737962
Conc: 25.01 ng/ml

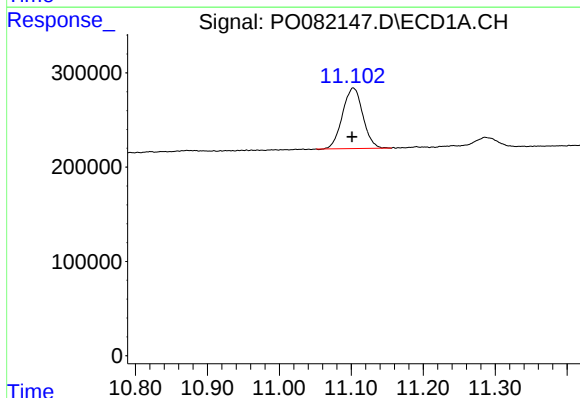

#2 Decachlorobiphenyl

R.T.: 11.103 min
Delta R.T.: 0.002 min
Response: 1262135
Conc: 22.71 ng/ml

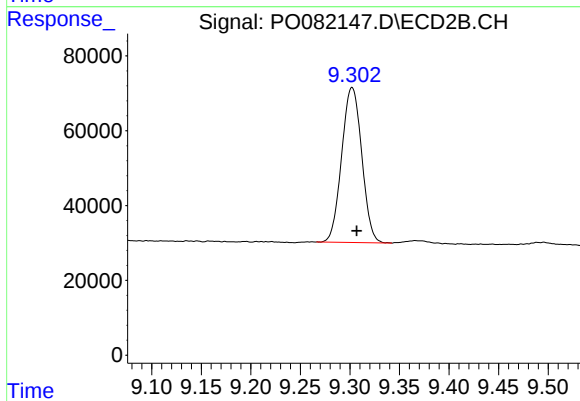

#2 Decachlorobiphenyl

R.T.: 9.302 min
Delta R.T.: -0.005 min
Response: 584110
Conc: 22.93 ng/ml