

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0102522\
 Data File : P0089904.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Oct 2022 11:02
 Operator : YP/AJ
 Sample : N5203-14 10X
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 KMH382K-1-2

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/26/2022
 Supervised By :Ankita Jodhani 10/27/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 25 14:04:19 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0102422.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Oct 25 02:35:13 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.305	3.485	3499327	1301981	1.100m	1.301
2) SA Decachlor...	10.057	8.499	6025701	2022989	2.518	2.226

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102522\
Data File : PO089904.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Oct 2022 11:02
Operator : YP/AJ
Sample : N5203-14 10X
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
KMH382K-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/26/2022
Supervised By :Ankita Jodhani 10/27/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 25 14:04:19 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102422.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Oct 25 02:35:13 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

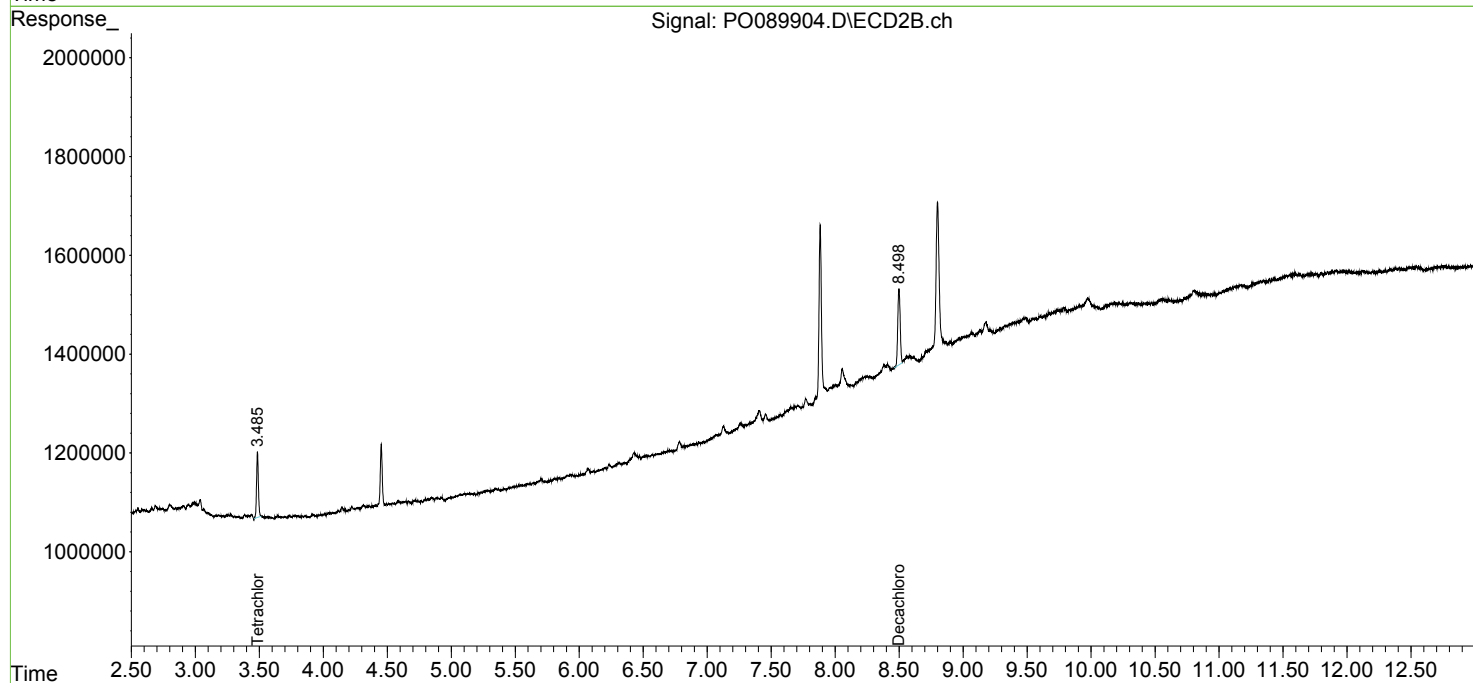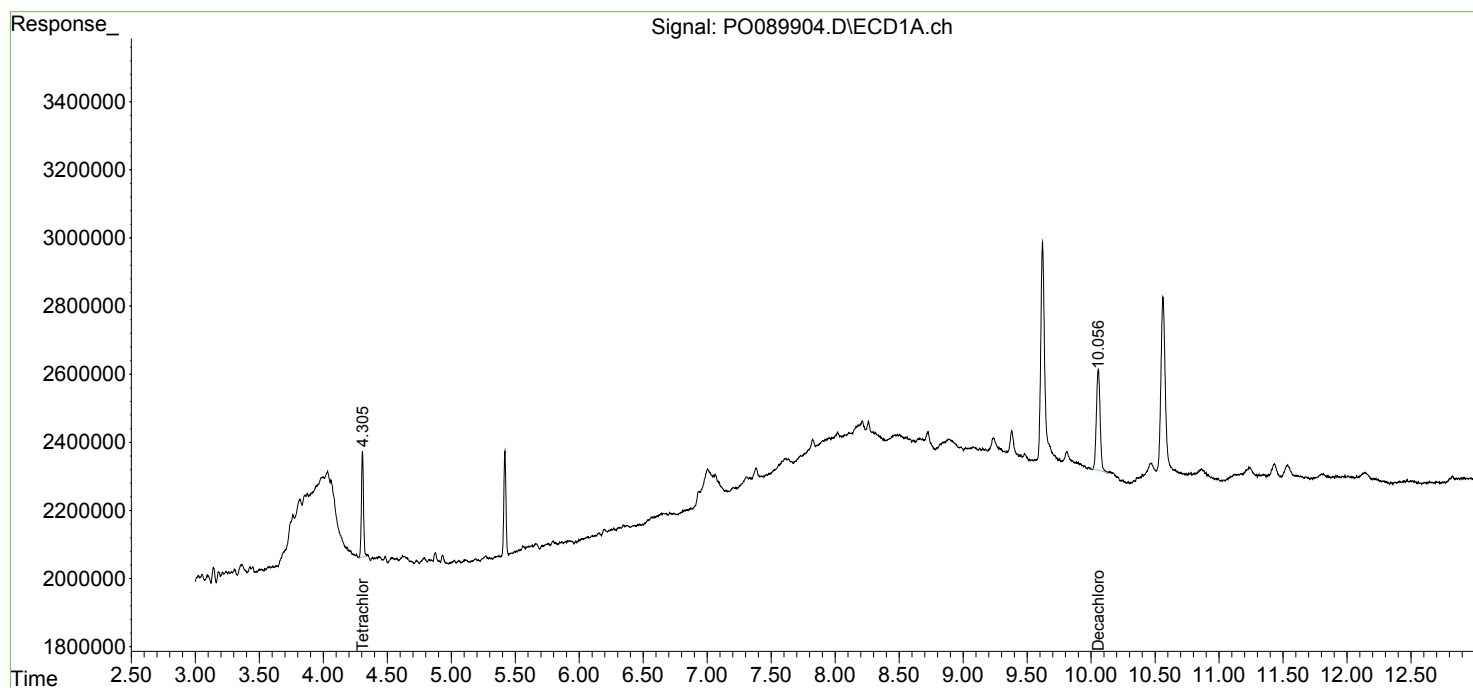

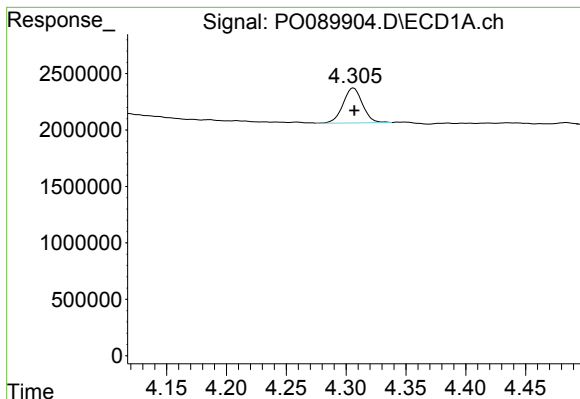


#1 Tetrachloro-m-xylene

R.T.: 4.305 min
Delta R.T.: -0.002 min
Response: 3499327
Conc: 1.10 ng/ml

Instrument :
ECD_O
ClientSampleId :
KMH382K-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/26/2022
Supervised By :Ankita Jodhani 10/27/2022

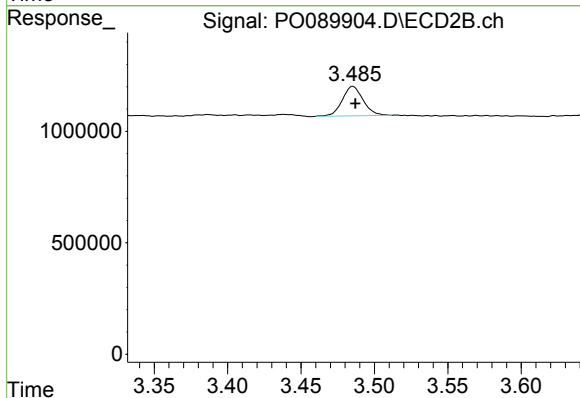


#1 Tetrachloro-m-xylene

R.T.: 3.485 min
Delta R.T.: -0.002 min
Response: 1301981
Conc: 1.30 ng/ml

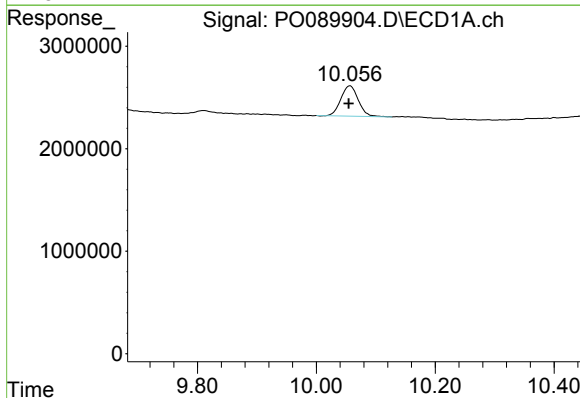

#2 Decachlorobiphenyl

R.T.: 10.057 min
Delta R.T.: 0.002 min
Response: 6025701
Conc: 2.52 ng/ml

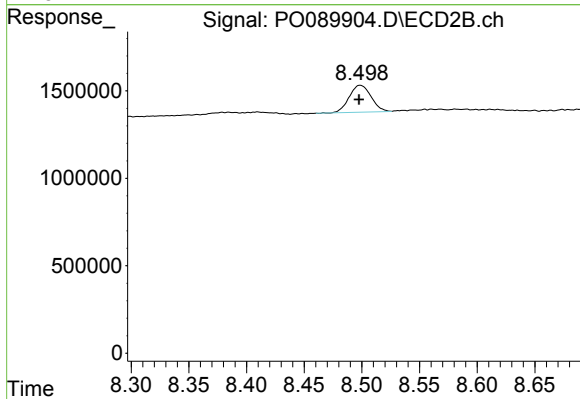

#2 Decachlorobiphenyl

R.T.: 8.499 min
Delta R.T.: 0.000 min
Response: 2022989
Conc: 2.23 ng/ml