

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\PO102522\
 Data File : PO089914.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Oct 2022 13:52
 Operator : YP/AJ
 Sample : N5257-01
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 HOLLAND-RD-COMP-1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/26/2022
 Supervised By :Ankita Jodhani 10/27/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 25 14:47:19 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\PO102422.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Oct 25 02:35:13 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.307	3.487	63455082	22347432	19.941	22.330
2) SA Decachlor...	10.053	8.497	37797021	15901432	15.792	17.501
Target Compounds						
26) L6 AR-1254-1	6.341	5.379	3472249	1721094	30.225	30.071
27) L6 AR-1254-2	6.562	5.527	5632691	1534436	32.699	30.003
28) L6 AR-1254-3	6.929	5.932	6866363	3391084	39.640	43.004
29) L6 AR-1254-4	7.216	6.161	3561043	1344722	28.092	28.221
30) L6 AR-1254-5	7.645	6.582	4537212	5231479	32.583m	74.033 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102522\
Data File : P0089914.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Oct 2022 13:52
Operator : YP/AJ
Sample : N5257-01
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
HOLLAND-RD-COMP-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/26/2022
Supervised By :Ankita Jodhani 10/27/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 25 14:47:19 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102422.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Oct 25 02:35:13 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

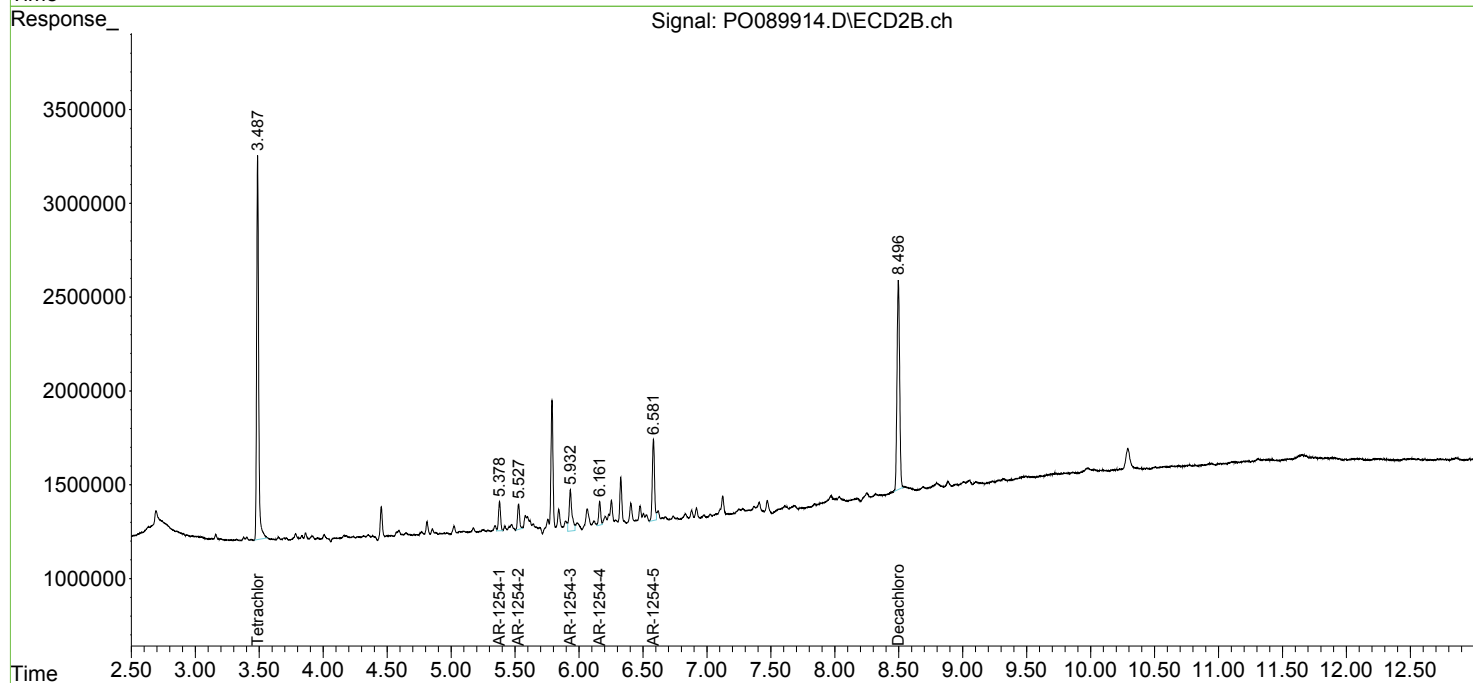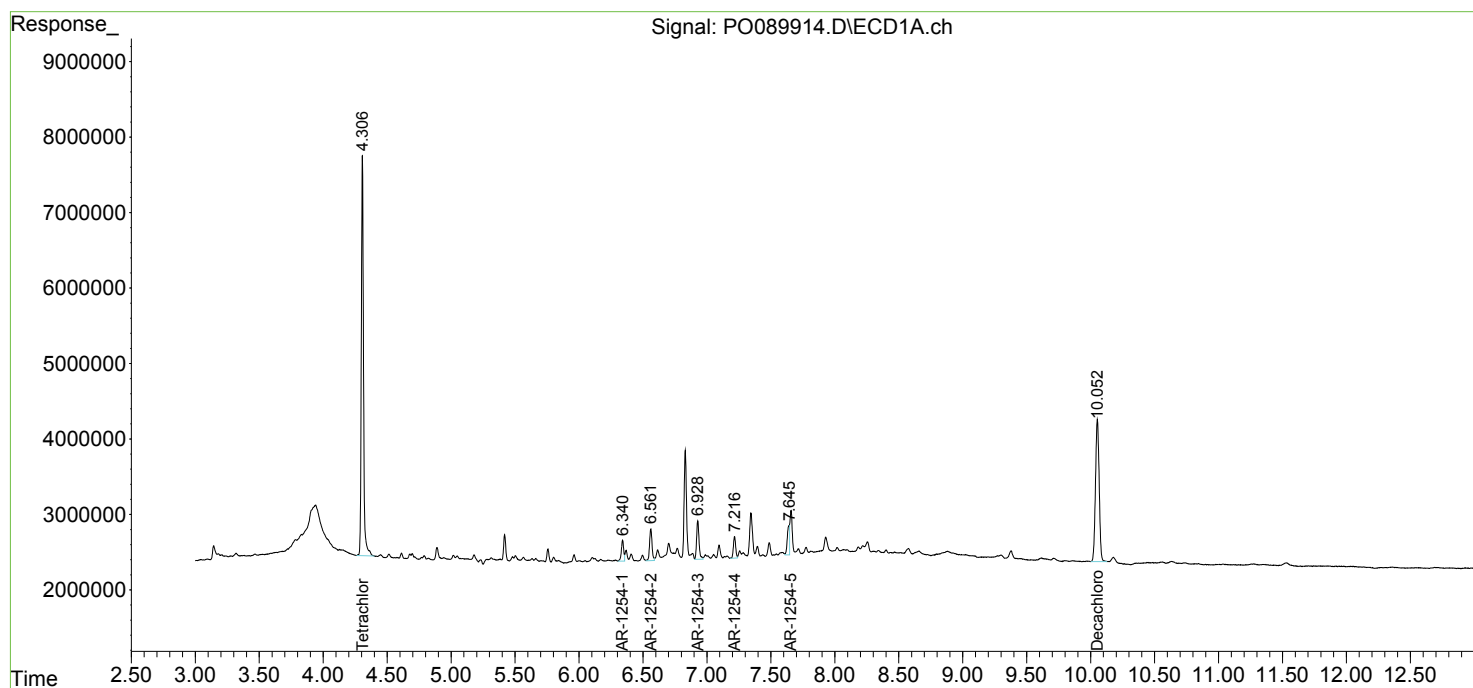

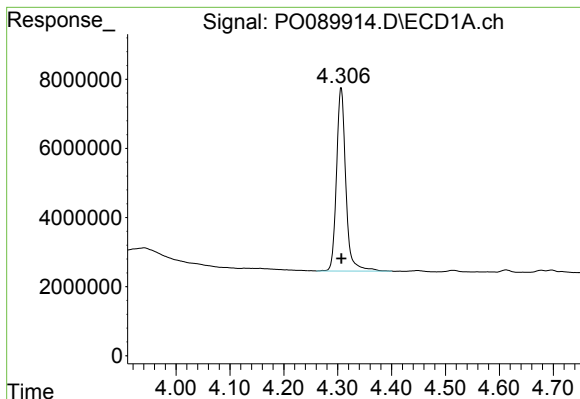


#1 Tetrachloro-m-xylene

R.T.: 4.307 min
Delta R.T.: 0.000 min
Response: 63455082
Conc: 19.94 ng/ml

Instrument :
ECD_O
ClientSampleId :
HOLLAND-RD-COMP-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/26/2022
Supervised By :Ankita Jodhani 10/27/2022

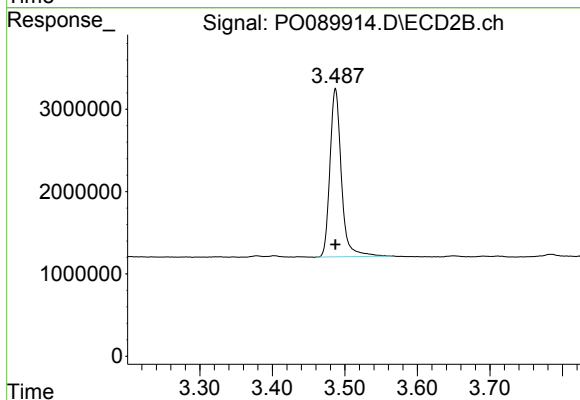


#1 Tetrachloro-m-xylene

R.T.: 3.487 min
Delta R.T.: 0.000 min
Response: 22347432
Conc: 22.33 ng/ml

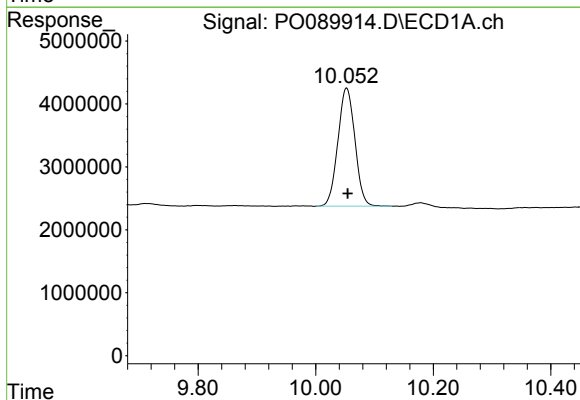


#2 Decachlorobiphenyl

R.T.: 10.053 min
Delta R.T.: -0.002 min
Response: 37797021
Conc: 15.79 ng/ml

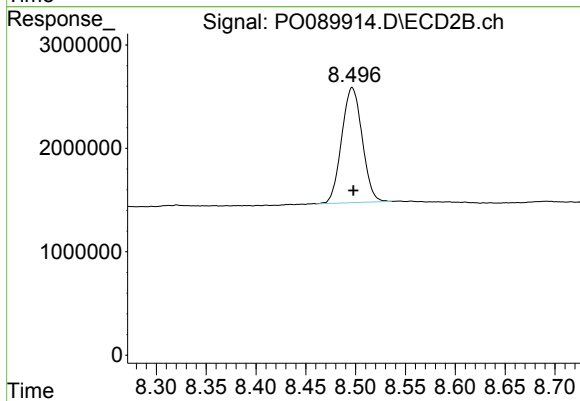

#2 Decachlorobiphenyl

R.T.: 8.497 min
Delta R.T.: -0.001 min
Response: 15901432
Conc: 17.50 ng/ml

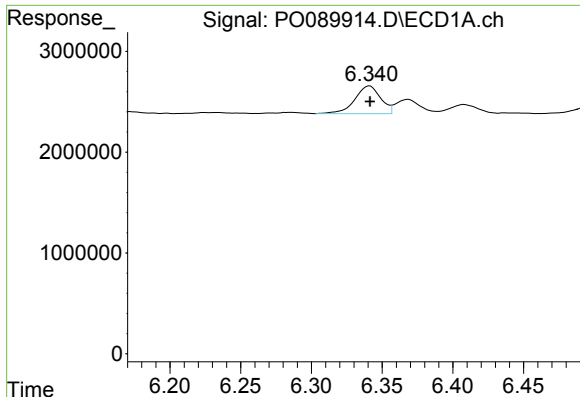


#26 AR-1254-1

R.T.: 6.341 min
Delta R.T.: 0.000 min
Response: 3472249
Conc: 30.22 ng/ml

Instrument :
ECD_O
ClientSampleId :
HOLLAND-RD-COMP-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/26/2022
Supervised By :Ankita Jodhani 10/27/2022

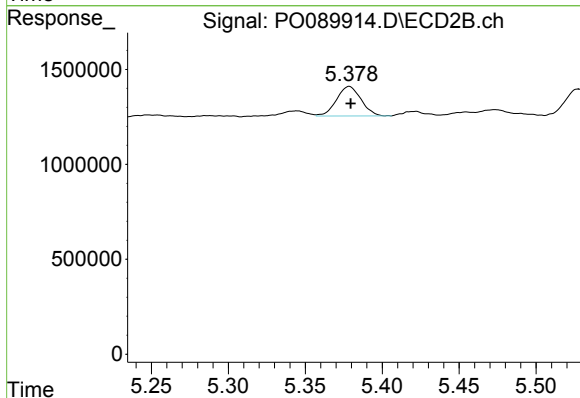


#26 AR-1254-1

R.T.: 5.379 min
Delta R.T.: 0.000 min
Response: 1721094
Conc: 30.07 ng/ml

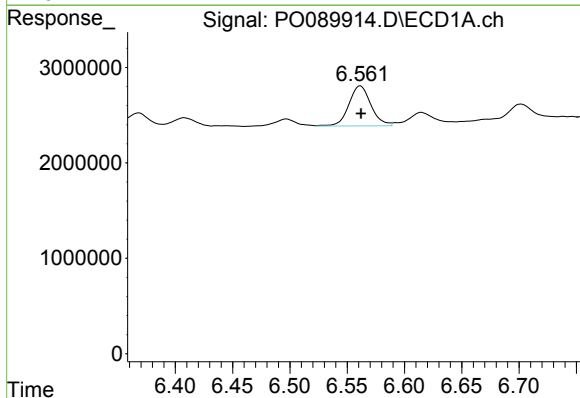


#27 AR-1254-2

R.T.: 6.562 min
Delta R.T.: 0.000 min
Response: 5632691
Conc: 32.70 ng/ml

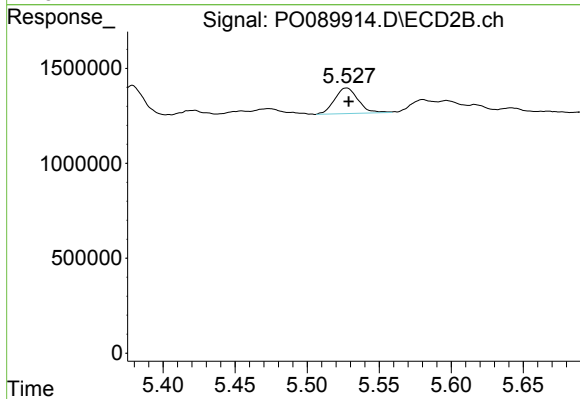

#27 AR-1254-2

R.T.: 5.527 min
Delta R.T.: -0.001 min
Response: 1534436
Conc: 30.00 ng/ml

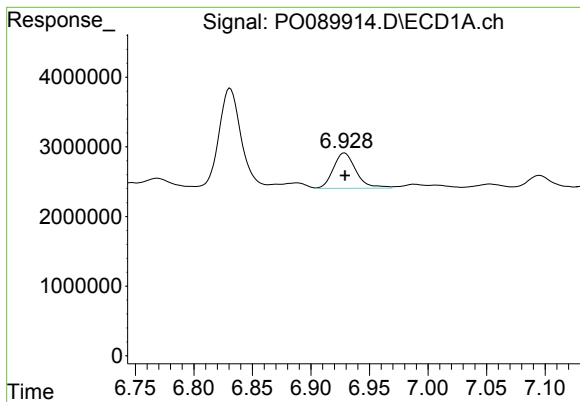


#28 AR-1254-3

R.T.: 6.929 min
Delta R.T.: 0.000 min
Response: 6866363
Conc: 39.64 ng/ml

Instrument :
ECD_O
ClientSampleId :
HOLLAND-RD-COMP-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/26/2022
Supervised By :Ankita Jodhani 10/27/2022

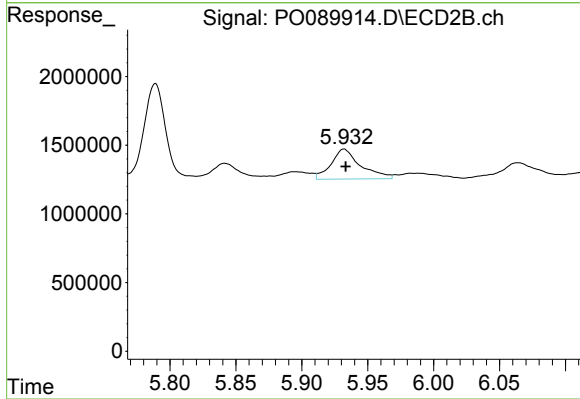


#28 AR-1254-3

R.T.: 5.932 min
Delta R.T.: -0.001 min
Response: 3391084
Conc: 43.00 ng/ml

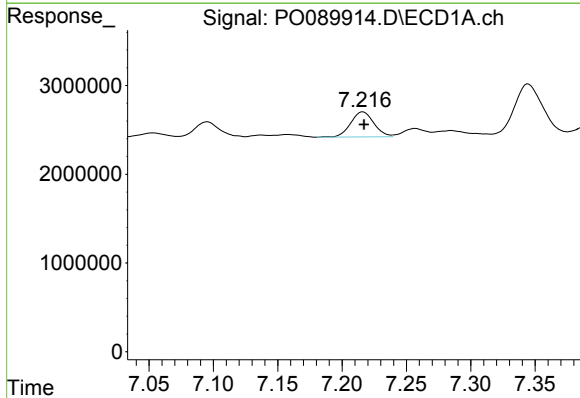


#29 AR-1254-4

R.T.: 7.216 min
Delta R.T.: 0.000 min
Response: 3561043
Conc: 28.09 ng/ml

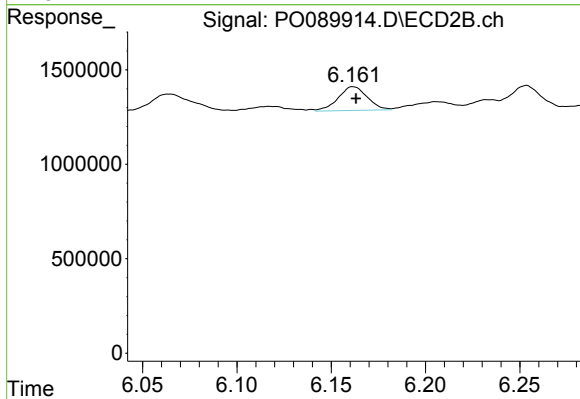

#29 AR-1254-4

R.T.: 6.161 min
Delta R.T.: -0.002 min
Response: 1344722
Conc: 28.22 ng/ml

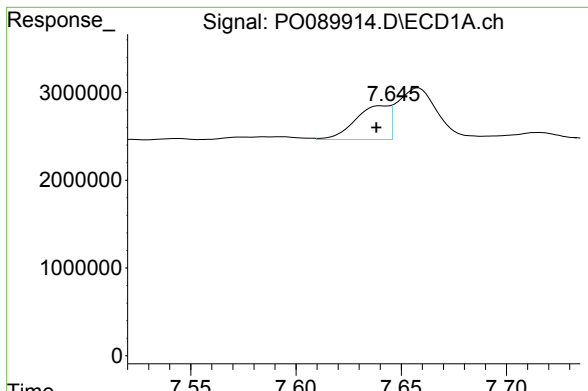


#30 AR-1254-5

R.T.: 7.645 min
Delta R.T.: 0.007 min
Response: 4537212
Conc: 32.58 ng/ml

Instrument :
ECD_O
ClientSampleId :
HOLLAND-RD-COMP-1

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/26/2022
Supervised By :Ankita Jodhani 10/27/2022

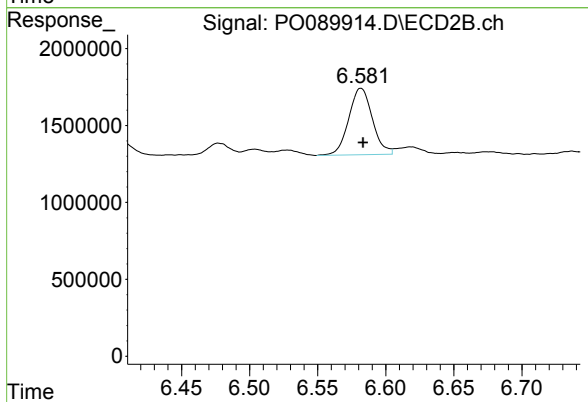

#30 AR-1254-5

R.T.: 6.582 min
Delta R.T.: -0.002 min
Response: 5231479
Conc: 74.03 ng/ml