

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\PO102522\
 Data File : PO089915.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Oct 2022 14:09
 Operator : YP/AJ
 Sample : N5257-03
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 HOLLAND-RD-COMP-2

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/26/2022
 Supervised By :Ankita Jodhani 10/27/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 25 14:47:46 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\PO102422.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Oct 25 02:35:13 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.306	3.487	67700861	24149376	21.275	24.131
2) SA Decachlor...	10.051	8.496	41005148	17506444	17.133	19.267m
Target Compounds						
26) L6 AR-1254-1	6.338	5.378	3038931	912544	26.453	15.944m#
27) L6 AR-1254-2	6.562	5.527	4331667	803585	25.146	15.713m#
28) L6 AR-1254-3	6.929	5.932	3484199	1188560	20.115	15.073m#
29) L6 AR-1254-4	7.216	6.161	1702042	531490	13.427	11.154m
30) L6 AR-1254-5	7.639	6.582	1313621	2127629	9.434	30.109 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102522\
Data File : PO089915.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Oct 2022 14:09
Operator : YP/AJ
Sample : N5257-03
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
HOLLAND-RD-COMP-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/26/2022
Supervised By :Ankita Jodhani 10/27/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 25 14:47:46 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102422.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Oct 25 02:35:13 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

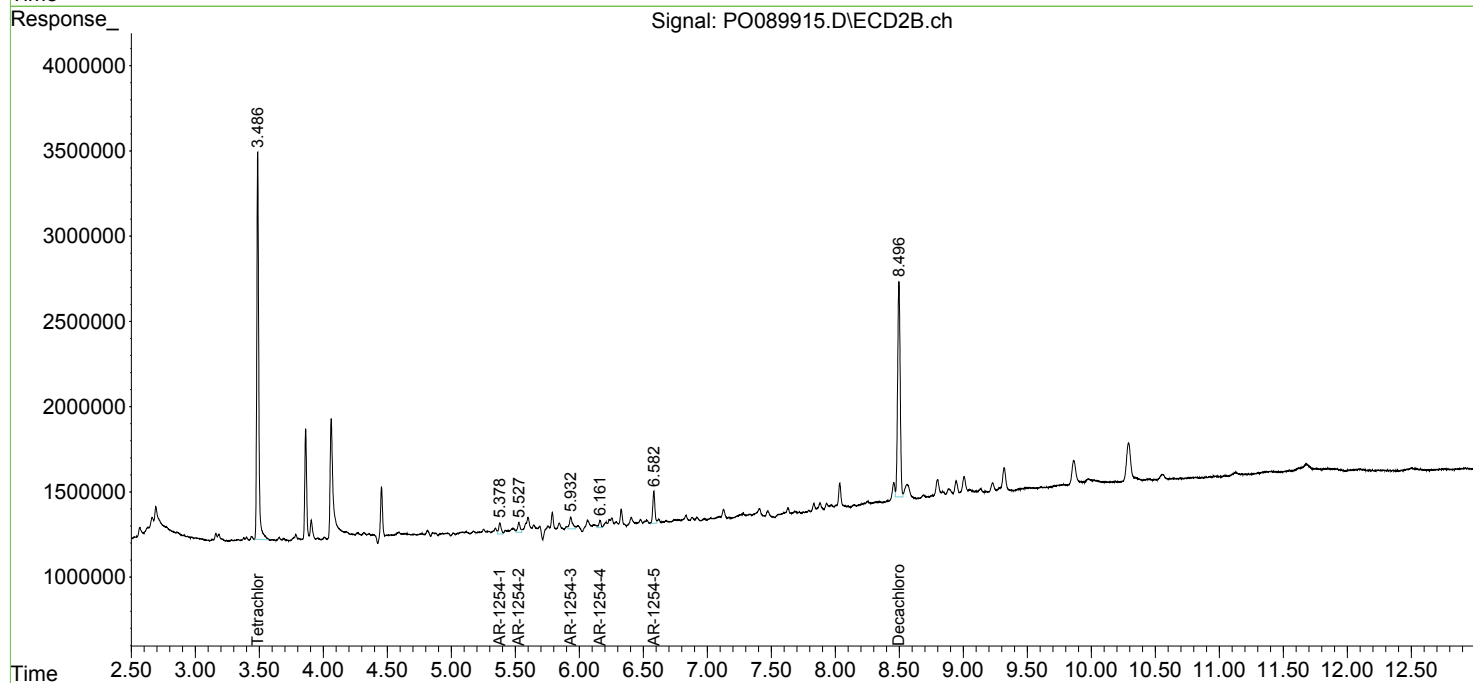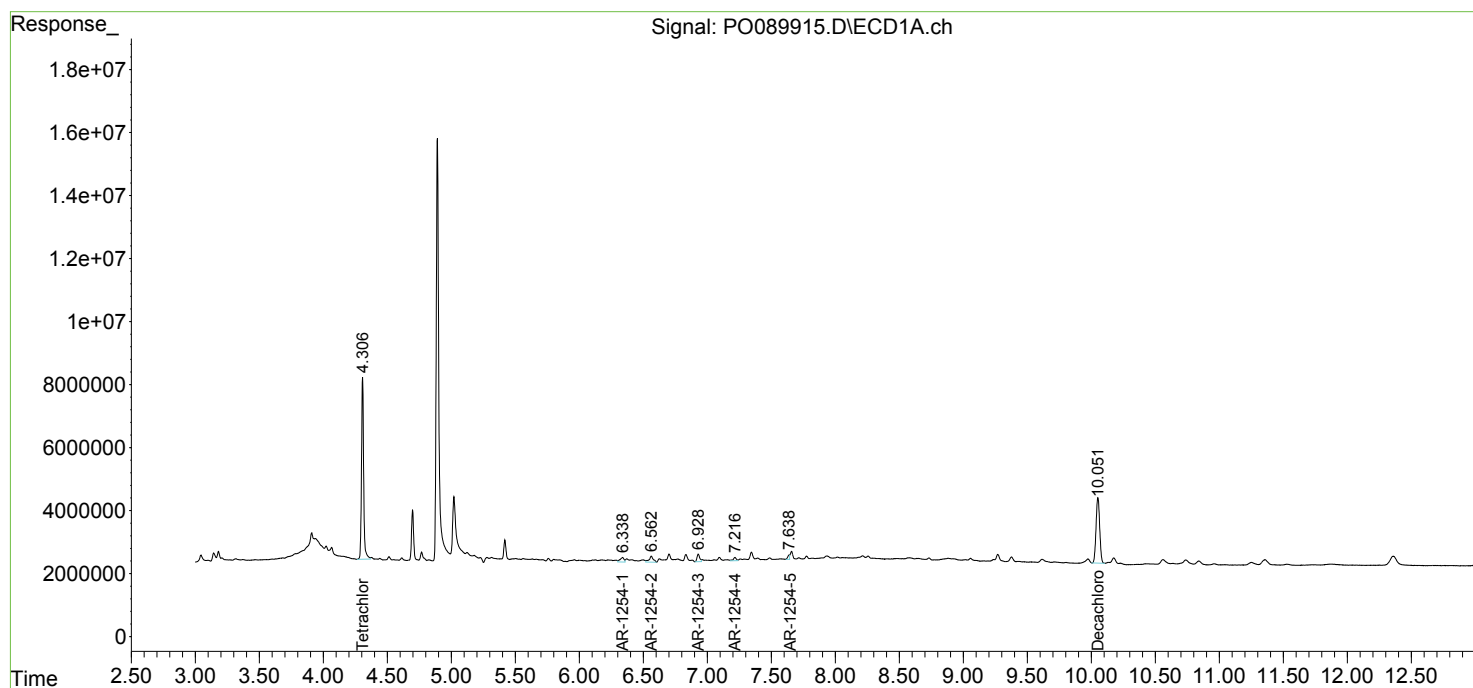

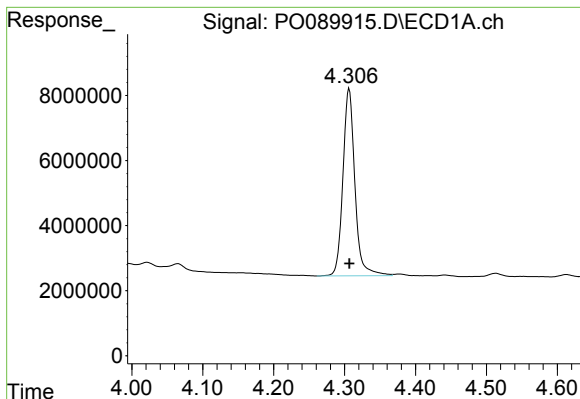


#1 Tetrachloro-m-xylene

R.T.: 4.306 min
Delta R.T.: 0.000 min
Response: 67700861
Conc: 21.27 ng/ml

Instrument :
ECD_O
ClientSampleId :
HOLLAND-RD-COMP-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/26/2022
Supervised By :Ankita Jodhani 10/27/2022

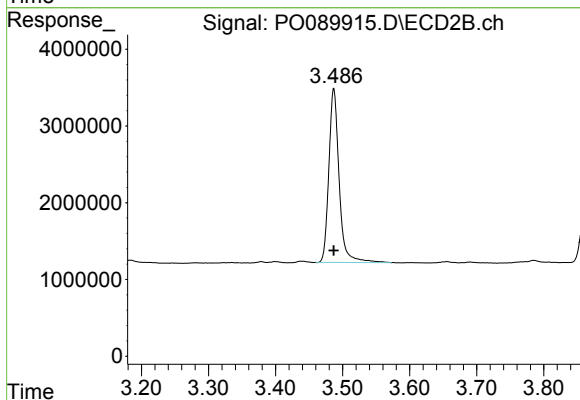


#1 Tetrachloro-m-xylene

R.T.: 3.487 min
Delta R.T.: 0.000 min
Response: 24149376
Conc: 24.13 ng/ml

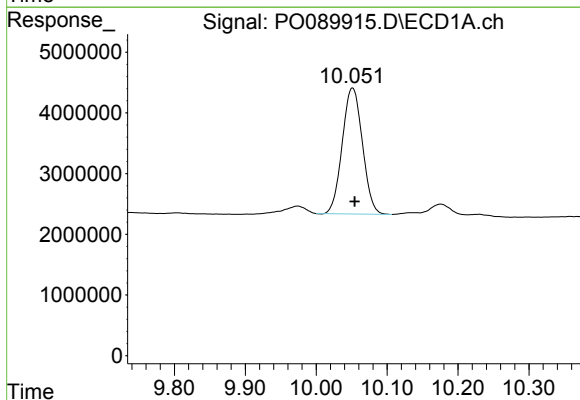


#2 Decachlorobiphenyl

R.T.: 10.051 min
Delta R.T.: -0.003 min
Response: 41005148
Conc: 17.13 ng/ml

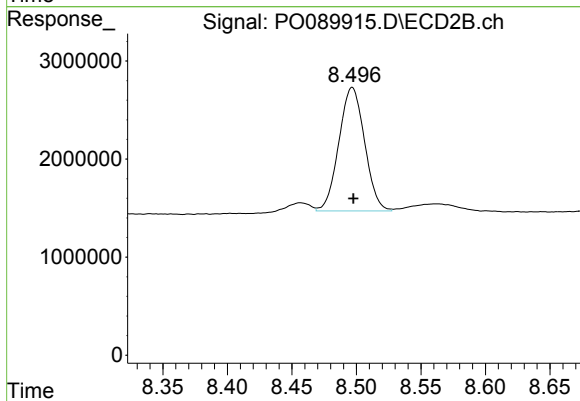

#2 Decachlorobiphenyl

R.T.: 8.496 min
Delta R.T.: -0.001 min
Response: 17506444
Conc: 19.27 ng/ml m

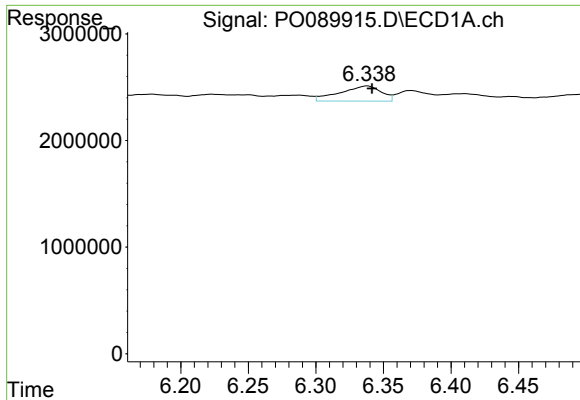


#26 AR-1254-1

R.T.: 6.338 min
Delta R.T.: -0.003 min
Response: 3038931
Conc: 26.45 ng/ml

Instrument :
ECD_O
ClientSampleId :
HOLLAND-RD-COMP-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/26/2022
Supervised By :Ankita Jodhani 10/27/2022

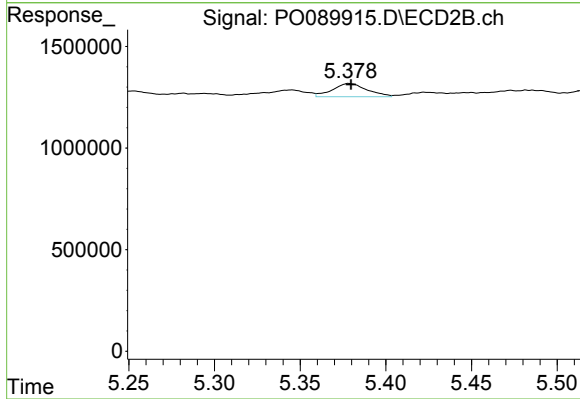


#26 AR-1254-1

R.T.: 5.378 min
Delta R.T.: -0.002 min
Response: 912544
Conc: 15.94 ng/ml m

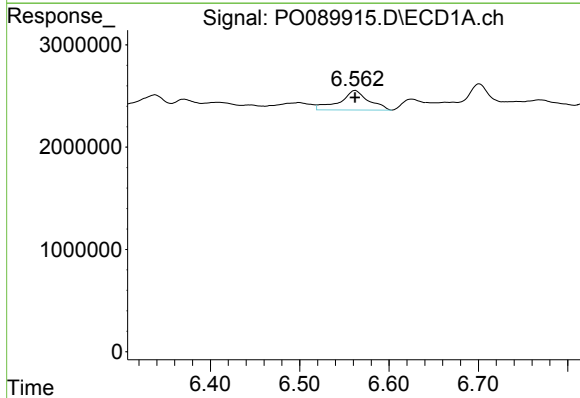


#27 AR-1254-2

R.T.: 6.562 min
Delta R.T.: 0.000 min
Response: 4331667
Conc: 25.15 ng/ml

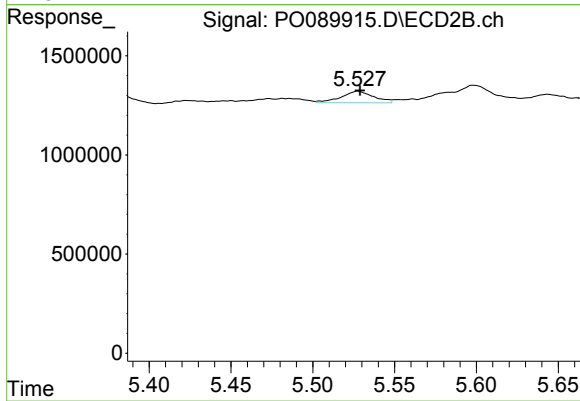

#27 AR-1254-2

R.T.: 5.527 min
Delta R.T.: -0.002 min
Response: 803585
Conc: 15.71 ng/ml m

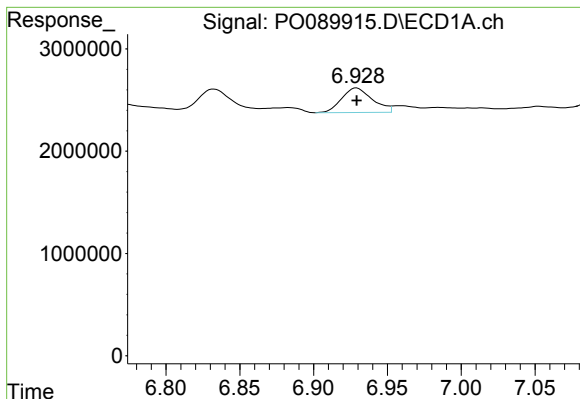


#28 AR-1254-3

R.T.: 6.929 min
Delta R.T.: 0.000 min
Response: 3484199
Conc: 20.11 ng/ml

Instrument :
ECD_O
ClientSampleId :
HOLLAND-RD-COMP-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/26/2022
Supervised By :Ankita Jodhani 10/27/2022

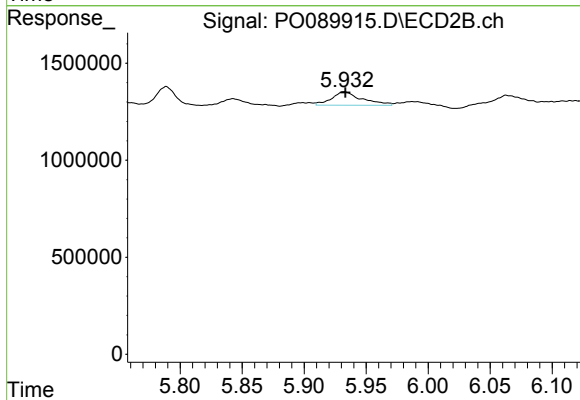


#28 AR-1254-3

R.T.: 5.932 min
Delta R.T.: 0.000 min
Response: 1188560
Conc: 15.07 ng/ml m

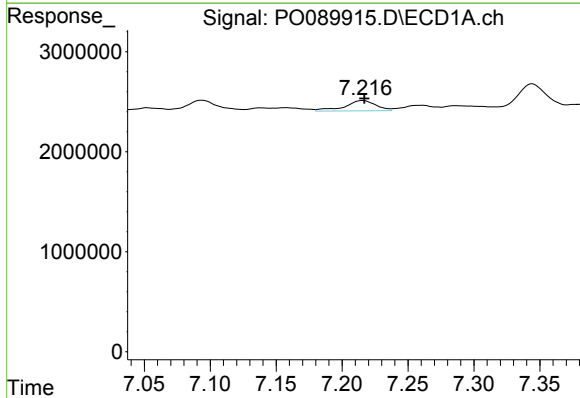


#29 AR-1254-4

R.T.: 7.216 min
Delta R.T.: 0.000 min
Response: 1702042
Conc: 13.43 ng/ml

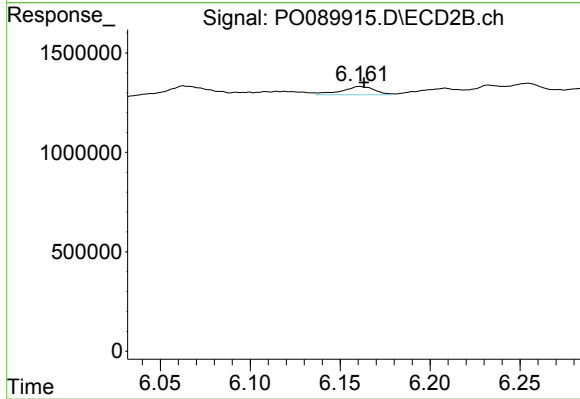

#29 AR-1254-4

R.T.: 6.161 min
Delta R.T.: -0.002 min
Response: 531490
Conc: 11.15 ng/ml m

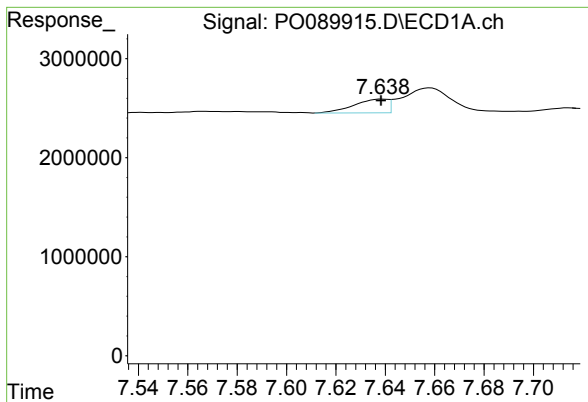


#30 AR-1254-5

R.T.: 7.639 min
Delta R.T.: 0.000 min
Response: 1313621
Conc: 9.43 ng/ml

Instrument :
ECD_O
ClientSampleId :
HOLLAND-RD-COMP-2

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/26/2022
Supervised By :Ankita Jodhani 10/27/2022

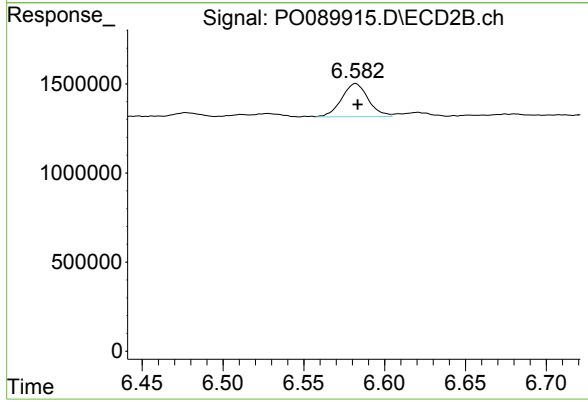

#30 AR-1254-5

R.T.: 6.582 min
Delta R.T.: -0.001 min
Response: 2127629
Conc: 30.11 ng/ml