

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\PO102522\
 Data File : PO089917.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Oct 2022 14:43
 Operator : YP/AJ
 Sample : N5257-07
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 HOLLAND-RD-COMP-4

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/26/2022
 Supervised By :Ankita Jodhani 10/27/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 25 16:18:44 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\PO102422.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Oct 25 02:35:13 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.310	3.489	51458335	18803272	16.171	18.789
2) SA Decachlor...	10.057	8.498	28417027	12425306	11.873	13.675
Target Compounds						
26) L6 AR-1254-1	6.343	5.382	4005058	1695079	34.863	29.617
27) L6 AR-1254-2	6.565	5.529	4157984	1447402	24.138	28.302m
28) L6 AR-1254-3	6.932	5.935	6952151	4006870	40.136	50.813m#
29) L6 AR-1254-4	7.219	6.165	3026056	855295	23.871	17.950
30) L6 AR-1254-5	7.640	6.585	9333186	6107610	67.025	86.431 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102522\
Data File : P0089917.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Oct 2022 14:43
Operator : YP/AJ
Sample : N5257-07
Misc :
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
HOLLAND-RD-COMP-4


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/26/2022
Supervised By :Ankita Jodhani 10/27/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 25 16:18:44 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102422.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Oct 25 02:35:13 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

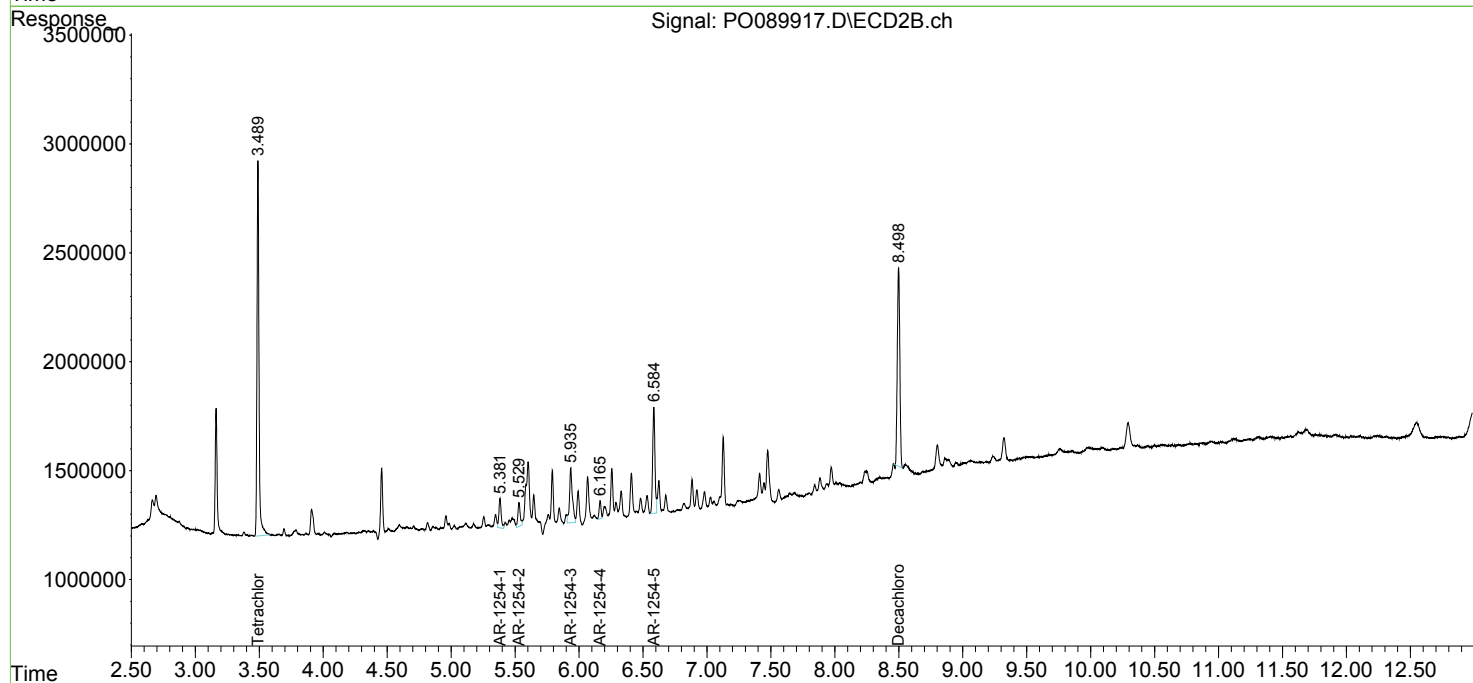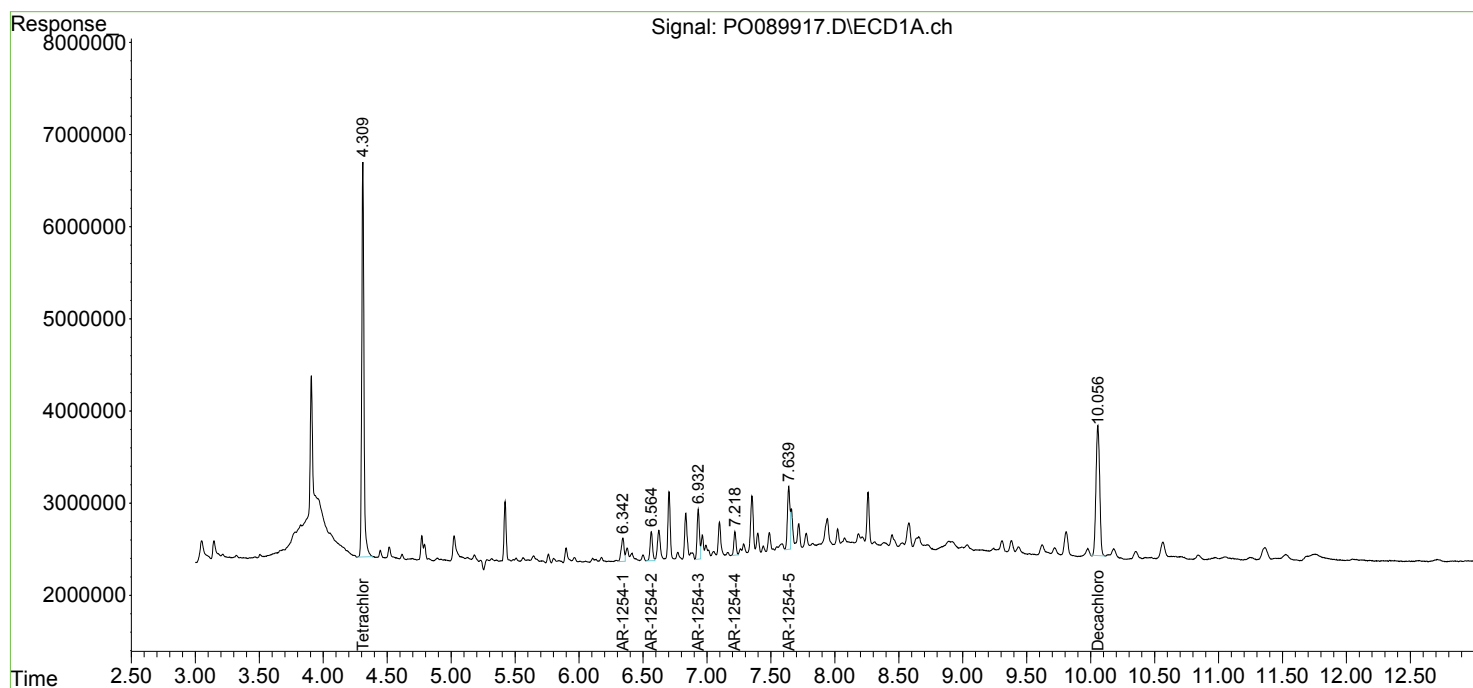

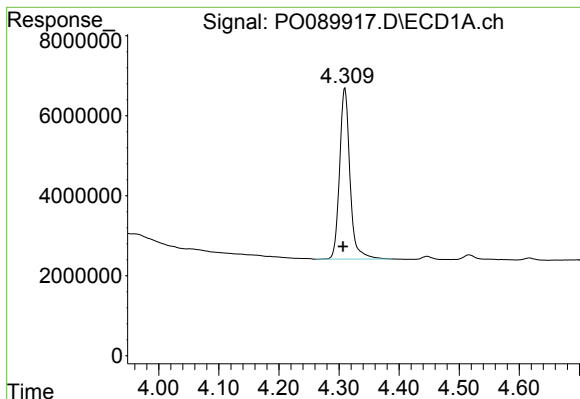


#1 Tetrachloro-m-xylene

R.T.: 4.310 min
Delta R.T.: 0.003 min
Response: 51458335
Conc: 16.17 ng/ml

Instrument :
ECD_O
ClientSampleId :
HOLLAND-RD-COMP-4


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/26/2022
Supervised By :Ankita Jodhani 10/27/2022

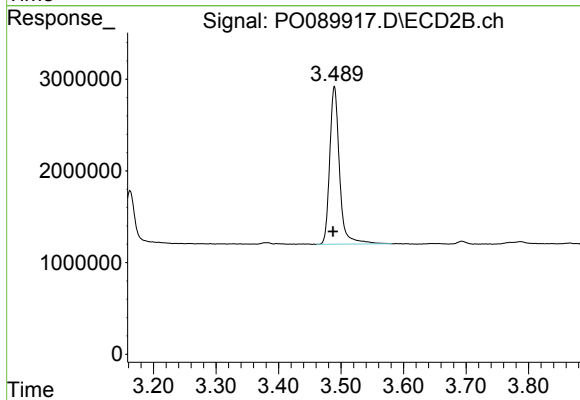


#1 Tetrachloro-m-xylene

R.T.: 3.489 min
Delta R.T.: 0.002 min
Response: 18803272
Conc: 18.79 ng/ml

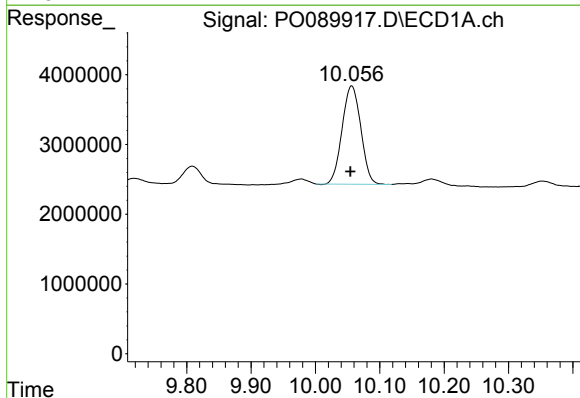


#2 Decachlorobiphenyl

R.T.: 10.057 min
Delta R.T.: 0.002 min
Response: 28417027
Conc: 11.87 ng/ml

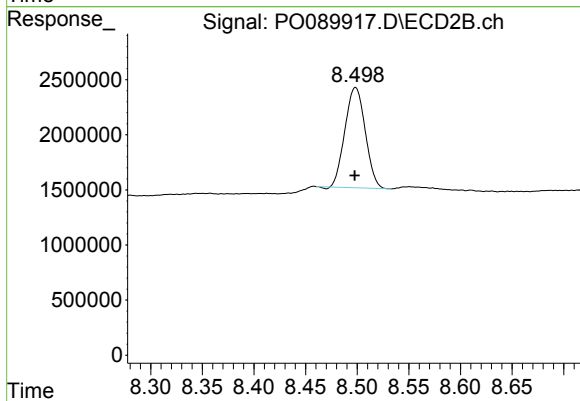

#2 Decachlorobiphenyl

R.T.: 8.498 min
Delta R.T.: 0.000 min
Response: 12425306
Conc: 13.67 ng/ml

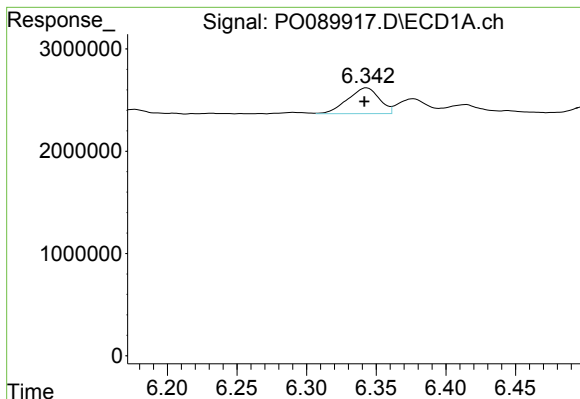


#26 AR-1254-1

R.T.: 6.343 min
Delta R.T.: 0.002 min
Response: 4005058
Conc: 34.86 ng/ml

Instrument :
ECD_O
ClientSampleId :
HOLLAND-RD-COMP-4


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/26/2022
Supervised By :Ankita Jodhani 10/27/2022

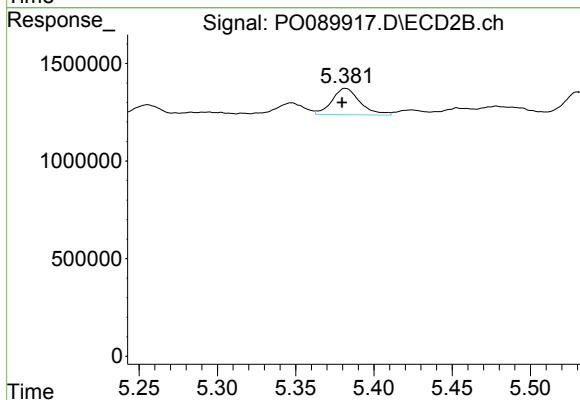


#26 AR-1254-1

R.T.: 5.382 min
Delta R.T.: 0.002 min
Response: 1695079
Conc: 29.62 ng/ml

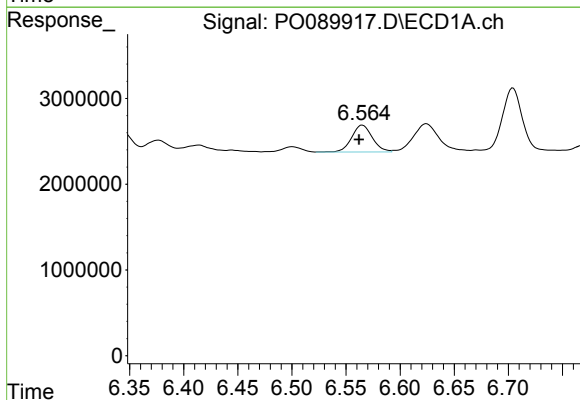


#27 AR-1254-2

R.T.: 6.565 min
Delta R.T.: 0.003 min
Response: 4157984
Conc: 24.14 ng/ml

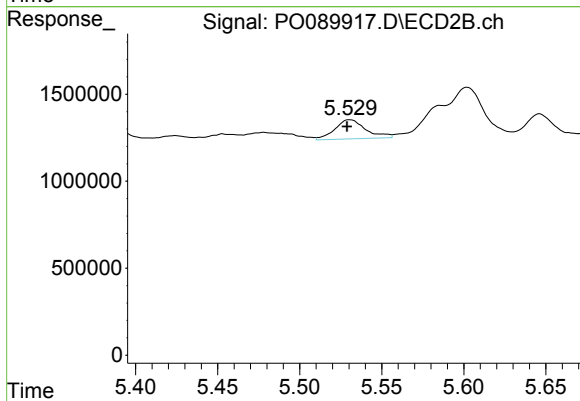

#27 AR-1254-2

R.T.: 5.529 min
Delta R.T.: 0.000 min
Response: 1447402
Conc: 28.30 ng/ml m

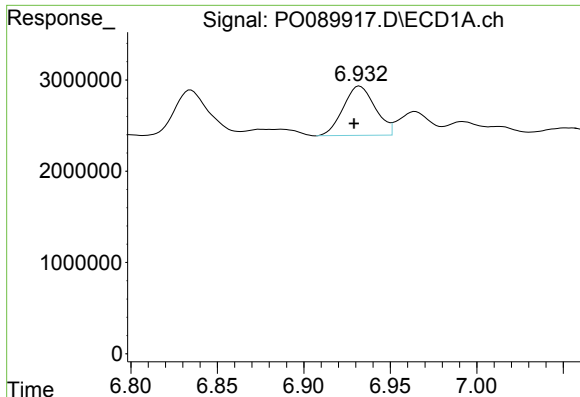


#28 AR-1254-3

R.T.: 6.932 min
Delta R.T.: 0.003 min
Response: 6952151
Conc: 40.14 ng/ml

Instrument :
ECD_O
ClientSampleId :
HOLLAND-RD-COMP-4


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/26/2022
Supervised By :Ankita Jodhani 10/27/2022

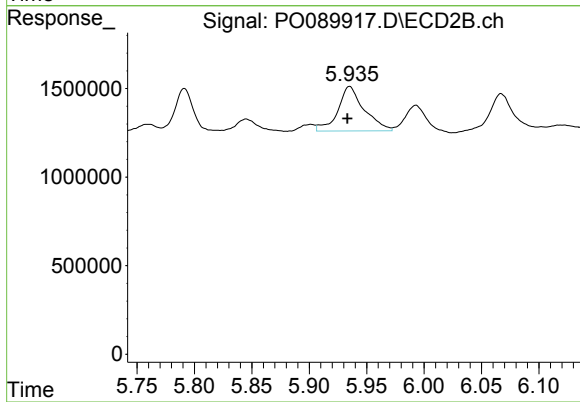


#28 AR-1254-3

R.T.: 5.935 min
Delta R.T.: 0.002 min
Response: 4006870
Conc: 50.81 ng/ml m

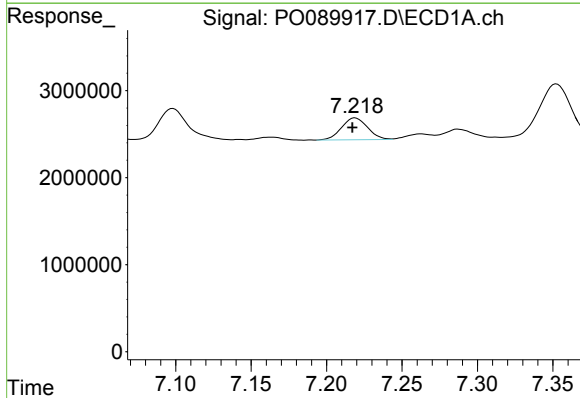


#29 AR-1254-4

R.T.: 7.219 min
Delta R.T.: 0.002 min
Response: 3026056
Conc: 23.87 ng/ml

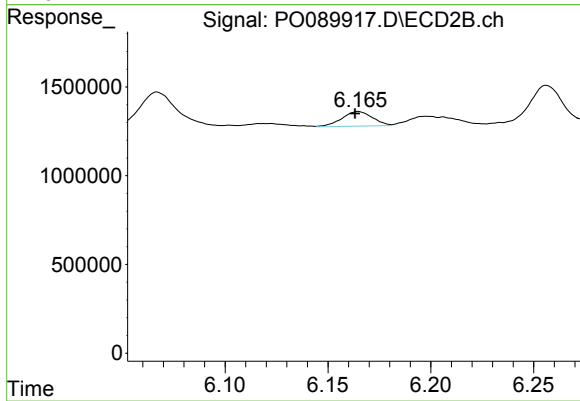

#29 AR-1254-4

R.T.: 6.165 min
Delta R.T.: 0.002 min
Response: 855295
Conc: 17.95 ng/ml

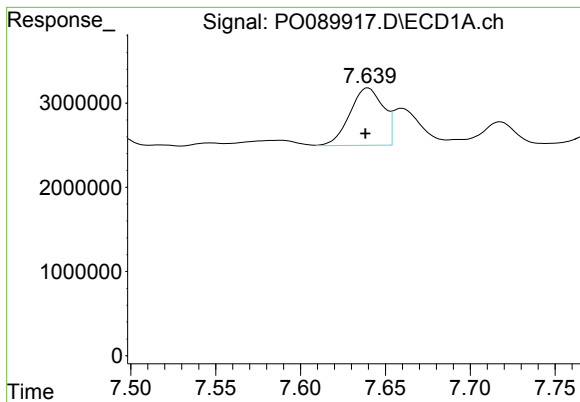


#30 AR-1254-5

R.T.: 7.640 min
Delta R.T.: 0.002 min
Response: 9333186
Conc: 67.03 ng/ml

Instrument :
ECD_O
ClientSampleId :
HOLLAND-RD-COMP-4

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/26/2022
Supervised By :Ankita Jodhani 10/27/2022

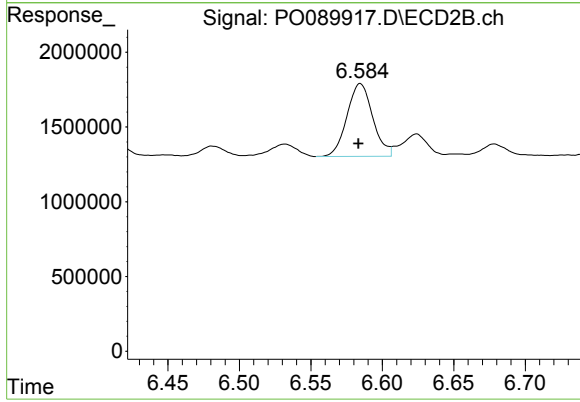

#30 AR-1254-5

R.T.: 6.585 min
Delta R.T.: 0.001 min
Response: 6107610
Conc: 86.43 ng/ml