

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102522\
 Data File : P0089927.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Oct 2022 17:45
 Operator : YP/AJ
 Sample : N4955-07
 Misc : AR1254 LOD 25 PPB
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 LOD-MDL-WATER-01-QT4-2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 25 23:31:43 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102422.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Oct 25 02:35:13 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.307	3.488	61436347	22259432	19.306	22.242
2) SA Decachlor...	10.054	8.498	52182575	21521822	21.803	23.686
Target Compounds						
26) L6 AR-1254-1	6.342	5.379	2557987	1389986	22.267	24.286
27) L6 AR-1254-2	6.563	5.529	3916328	1292378	22.735	25.270
28) L6 AR-1254-3	6.929	5.933	4081210	1884138	23.561	23.894
29) L6 AR-1254-4	7.217	6.164	2796967	1070090	22.064	22.458
30) L6 AR-1254-5	7.639	6.584	2740622	1283400	19.681	18.162



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102522\
Data File : PO089927.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Oct 2022 17:45
Operator : YP/AJ
Sample : N4955-07
Misc : AR1254 LOD 25 PPB
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 25 23:31:43 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102422.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Oct 25 02:35:13 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

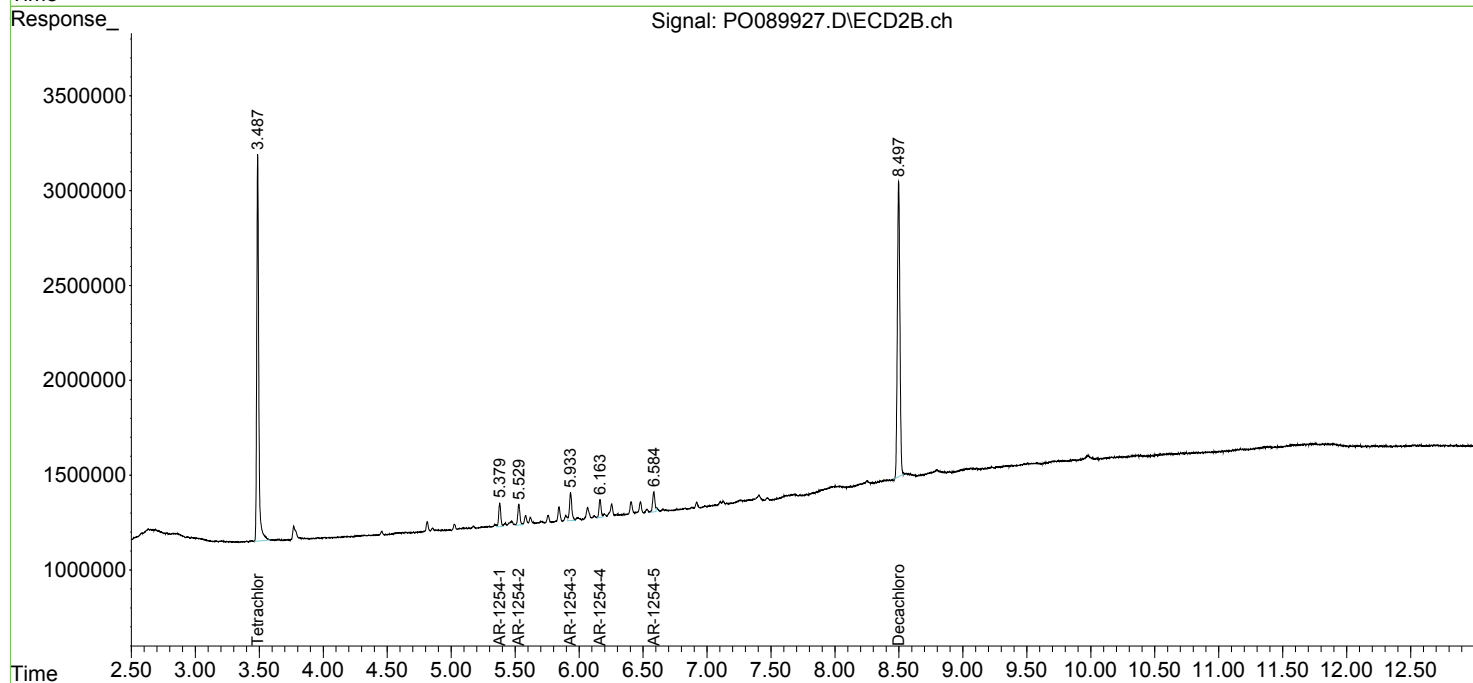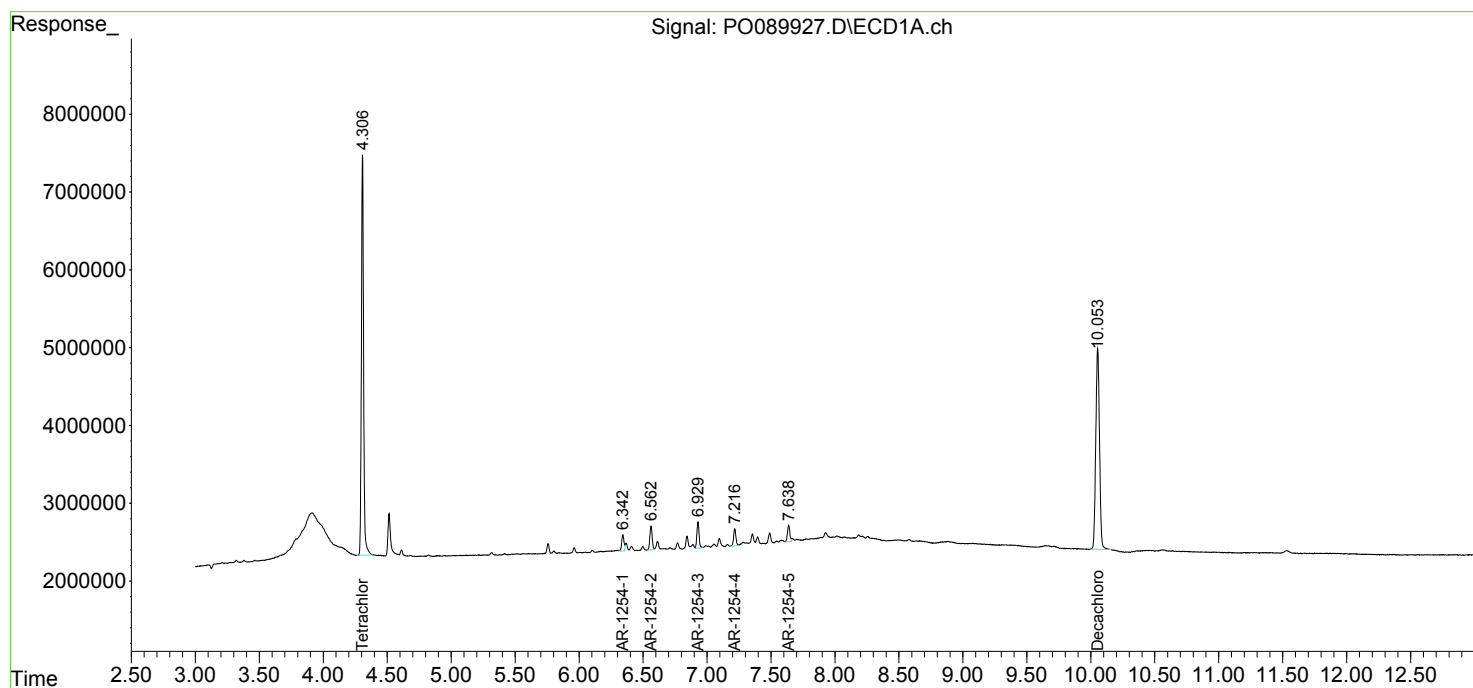


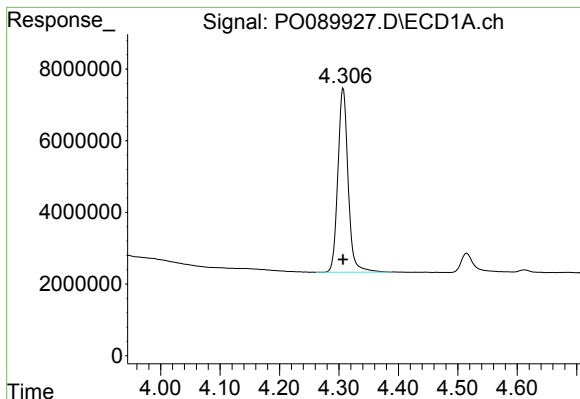

#1 Tetrachloro-m-xylene


R.T.: 4.307 min
Delta R.T.: 0.000 min
Response: 61436347
Conc: 19.31 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2022

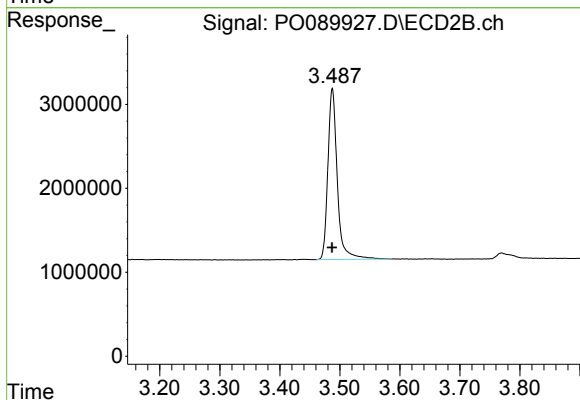


#1 Tetrachloro-m-xylene

R.T.: 3.488 min
Delta R.T.: 0.000 min
Response: 22259432
Conc: 22.24 ng/ml

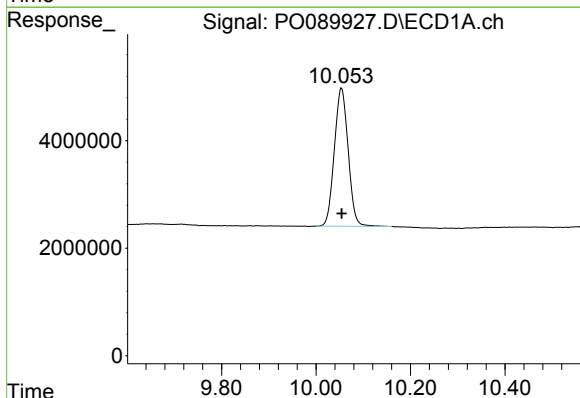


#2 Decachlorobiphenyl

R.T.: 10.054 min
Delta R.T.: 0.000 min
Response: 52182575
Conc: 21.80 ng/ml

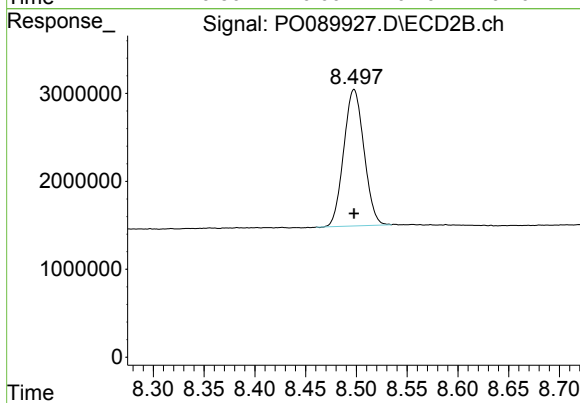

#2 Decachlorobiphenyl


R.T.: 8.498 min
Delta R.T.: 0.000 min
Response: 21521822
Conc: 23.69 ng/ml

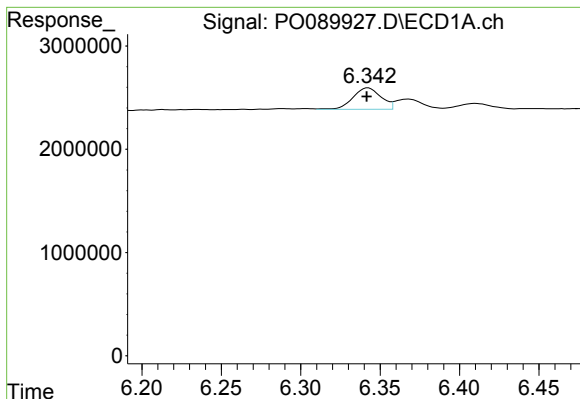

#26 AR-1254-1


R.T.: 6.342 min
Delta R.T.: 0.000 min
Response: 2557987
Conc: 22.27 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2022

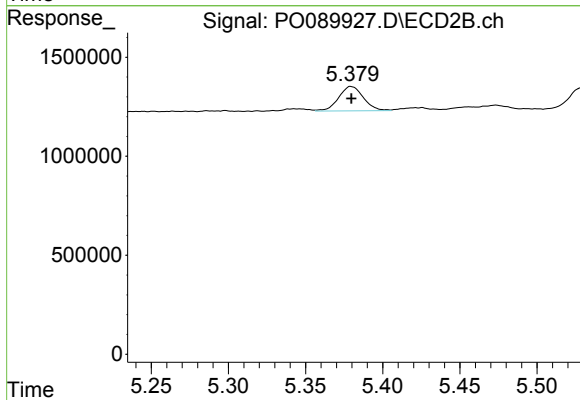


#26 AR-1254-1

R.T.: 5.379 min
Delta R.T.: 0.000 min
Response: 1389986
Conc: 24.29 ng/ml

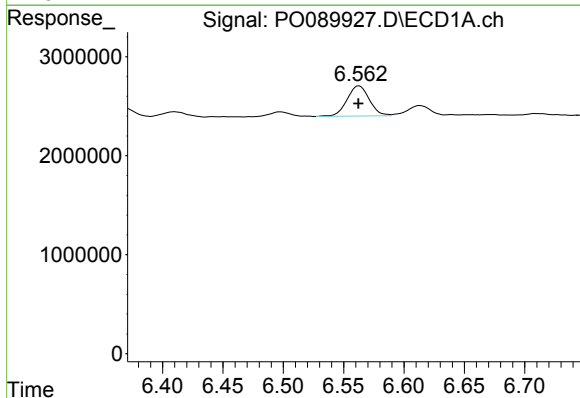


#27 AR-1254-2

R.T.: 6.563 min
Delta R.T.: 0.000 min
Response: 3916328
Conc: 22.74 ng/ml

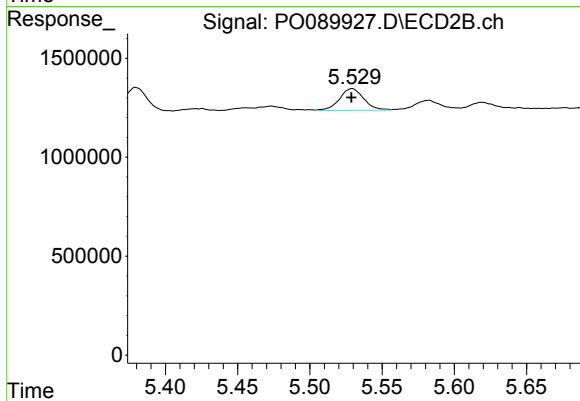

#27 AR-1254-2


R.T.: 5.529 min
Delta R.T.: 0.000 min
Response: 1292378
Conc: 25.27 ng/ml

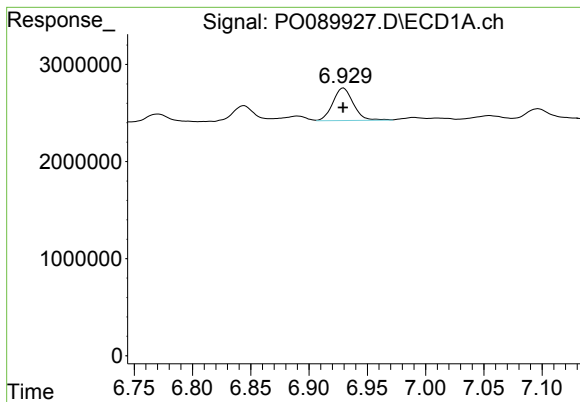

#28 AR-1254-3


R.T.: 6.929 min
Delta R.T.: 0.000 min
Response: 4081210
Conc: 23.56 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2022

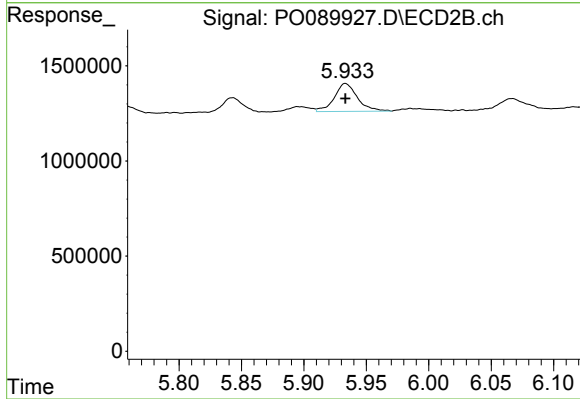


#28 AR-1254-3

R.T.: 5.933 min
Delta R.T.: 0.000 min
Response: 1884138
Conc: 23.89 ng/ml

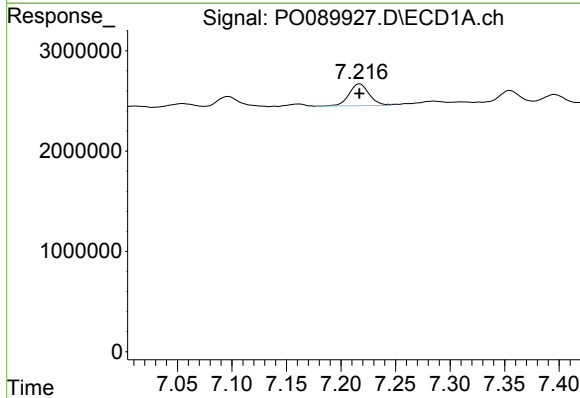


#29 AR-1254-4

R.T.: 7.217 min
Delta R.T.: 0.000 min
Response: 2796967
Conc: 22.06 ng/ml

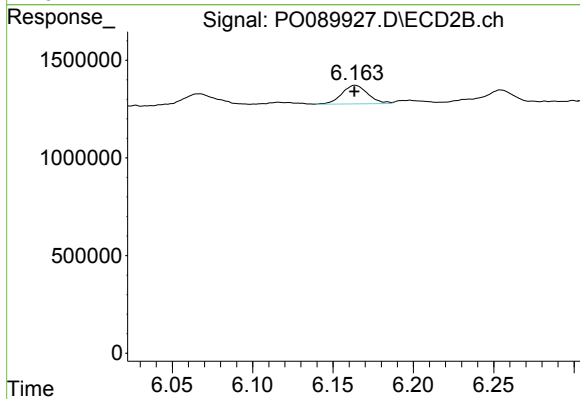

#29 AR-1254-4


R.T.: 6.164 min
Delta R.T.: 0.000 min
Response: 1070090
Conc: 22.46 ng/ml

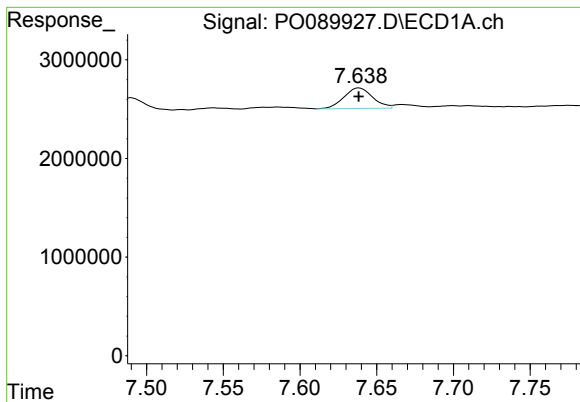

#30 AR-1254-5

R.T.: 7.639 min
Delta R.T.: 0.000 min
Response: 2740622
Conc: 19.68 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2022

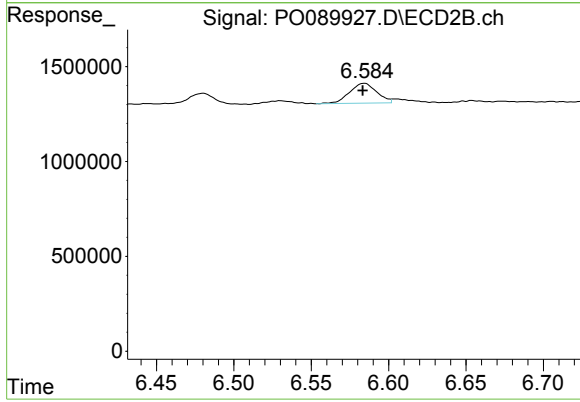

#30 AR-1254-5

R.T.: 6.584 min
Delta R.T.: 0.001 min
Response: 1283400
Conc: 18.16 ng/ml