

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\PO102522\
 Data File : PO089937.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Oct 2022 20:36
 Operator : YP/AJ
 Sample : N5267-04
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 TP2-1024

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/26/2022
 Supervised By :Ankita Jodhani 10/27/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 25 23:41:07 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\PO102422.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Oct 25 02:35:13 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.307	3.487	48231634	18514858	15.157	18.500
2) SA Decachlor...	10.052	8.498	42167605	16030976	17.618	17.643
Target Compounds						
26) L6 AR-1254-1	6.343	5.381	6822406	3712924	59.387	64.872
27) L6 AR-1254-2	6.563	5.528	11449841	2977077	66.469	58.212
28) L6 AR-1254-3	6.931	5.933	12635501	6488459	72.946	82.283
29) L6 AR-1254-4	7.216	6.163	7382734	1977187	58.239	41.495 #
30) L6 AR-1254-5	7.636	6.582	12084728	5877904	86.785m	83.181

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102522\
Data File : P0089937.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Oct 2022 20:36
Operator : YP/AJ
Sample : N5267-04
Misc :
ALS Vial : 35 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
TP2-1024


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/26/2022
Supervised By :Ankita Jodhani 10/27/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 25 23:41:07 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102422.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Oct 25 02:35:13 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

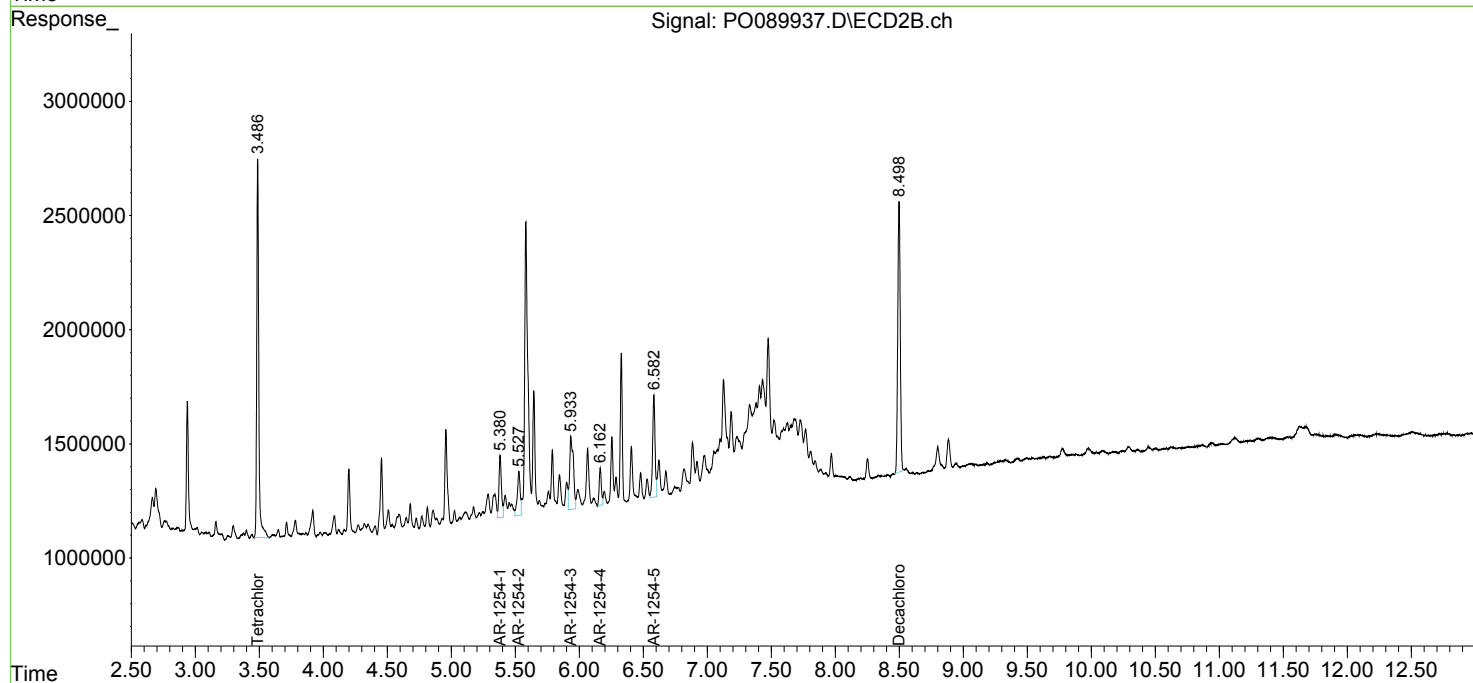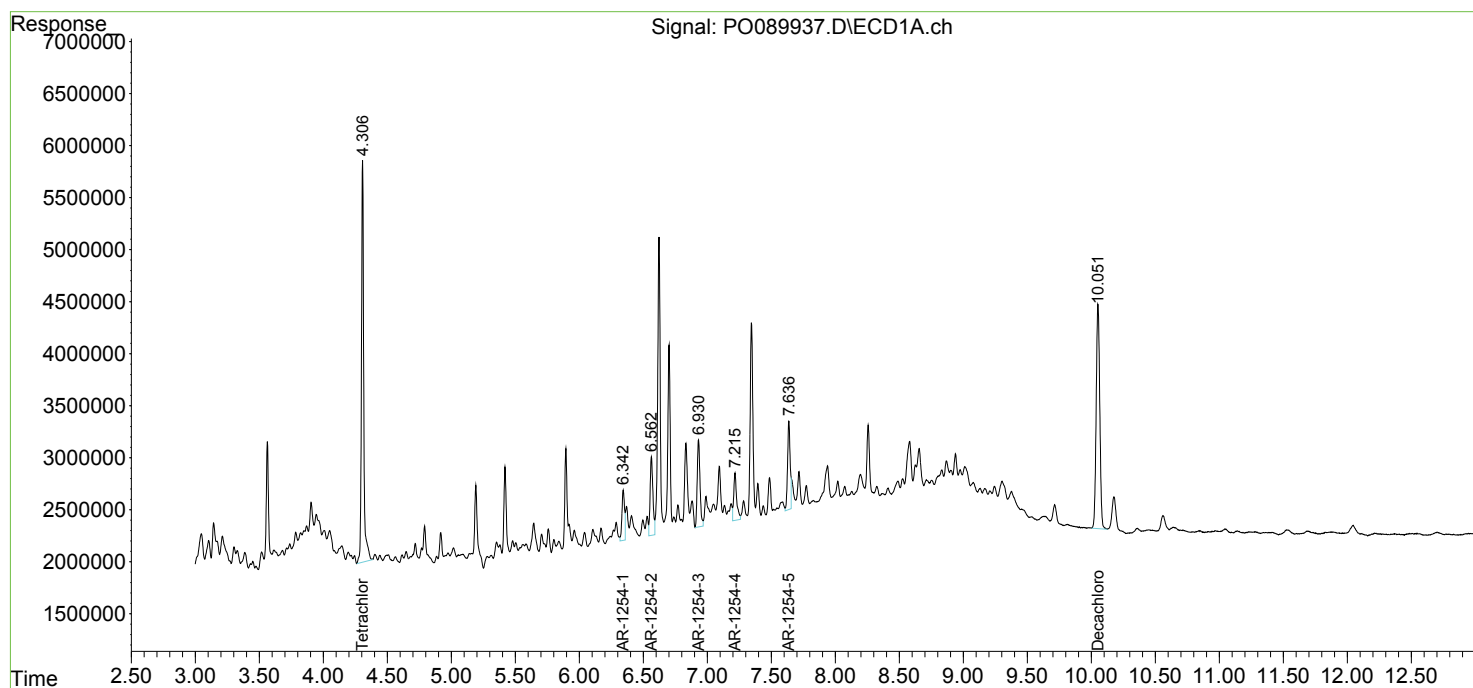

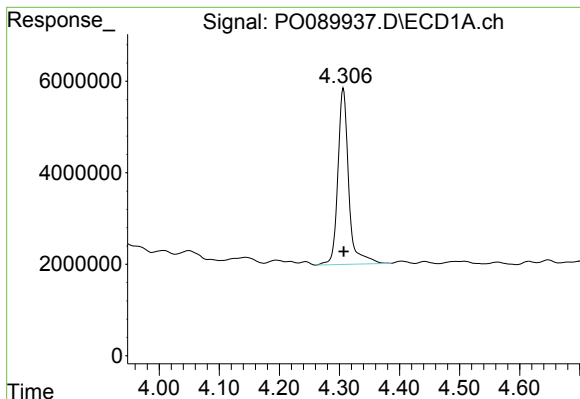


#1 Tetrachloro-m-xylene

R.T.: 4.307 min
Delta R.T.: 0.000 min
Response: 48231634
Conc: 15.16 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP2-1024


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/26/2022
Supervised By :Ankita Jodhani 10/27/2022

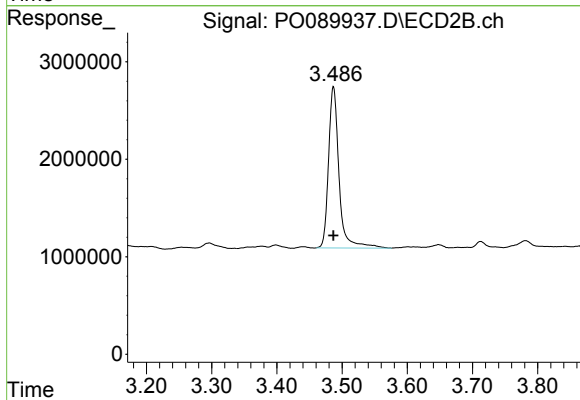


#1 Tetrachloro-m-xylene

R.T.: 3.487 min
Delta R.T.: 0.000 min
Response: 18514858
Conc: 18.50 ng/ml

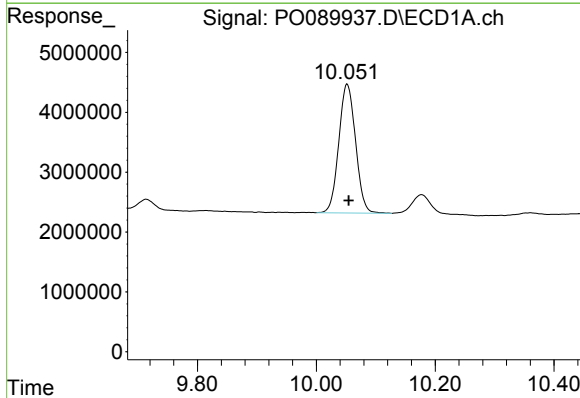


#2 Decachlorobiphenyl

R.T.: 10.052 min
Delta R.T.: -0.002 min
Response: 42167605
Conc: 17.62 ng/ml

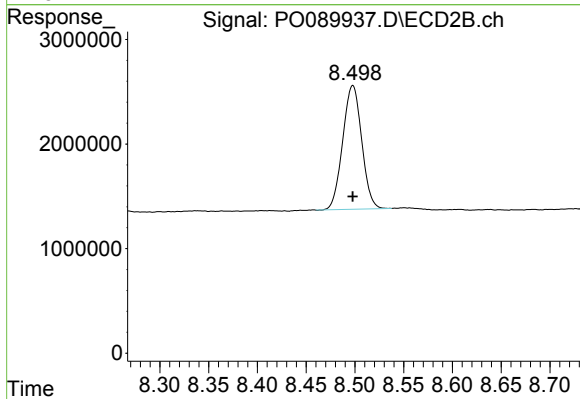

#2 Decachlorobiphenyl

R.T.: 8.498 min
Delta R.T.: 0.000 min
Response: 16030976
Conc: 17.64 ng/ml

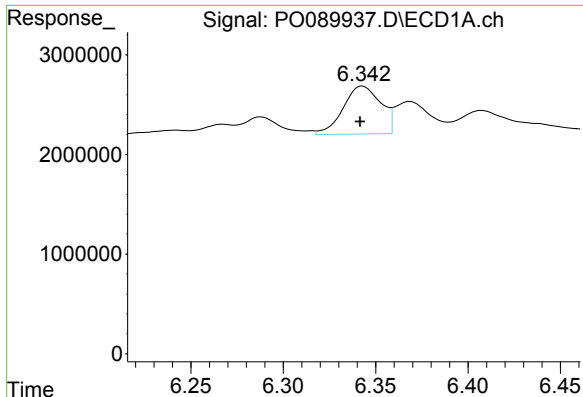


#26 AR-1254-1

R.T.: 6.343 min
Delta R.T.: 0.001 min
Response: 6822406
Conc: 59.39 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP2-1024


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/26/2022
Supervised By :Ankita Jodhani 10/27/2022

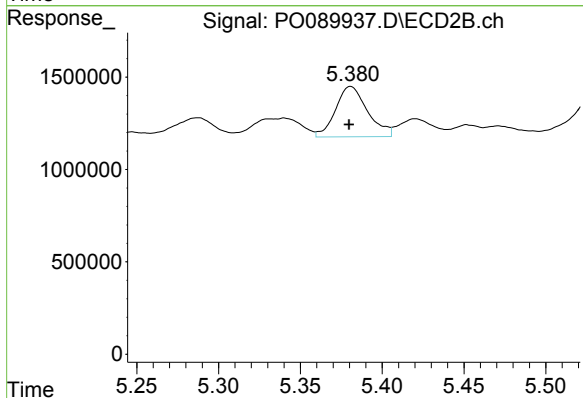


#26 AR-1254-1

R.T.: 5.381 min
Delta R.T.: 0.001 min
Response: 3712924
Conc: 64.87 ng/ml

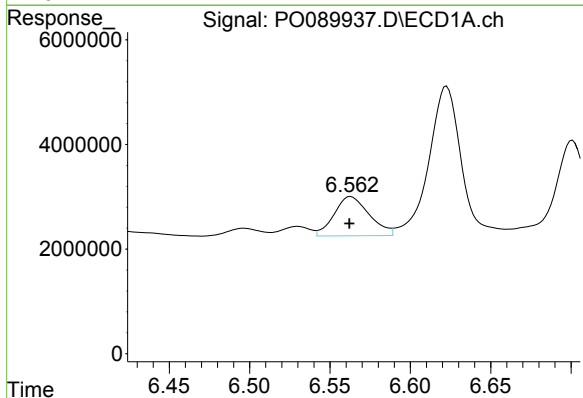


#27 AR-1254-2

R.T.: 6.563 min
Delta R.T.: 0.000 min
Response: 11449841
Conc: 66.47 ng/ml

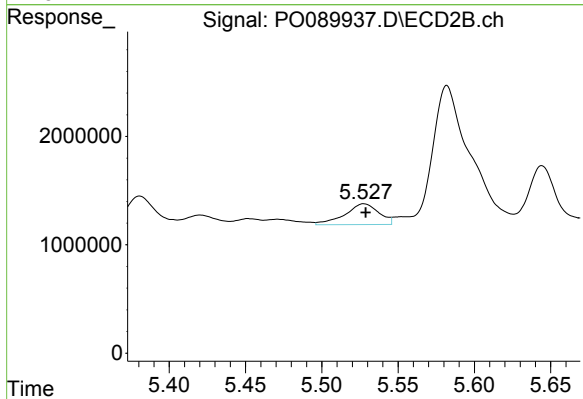

#27 AR-1254-2

R.T.: 5.528 min
Delta R.T.: -0.001 min
Response: 2977077
Conc: 58.21 ng/ml

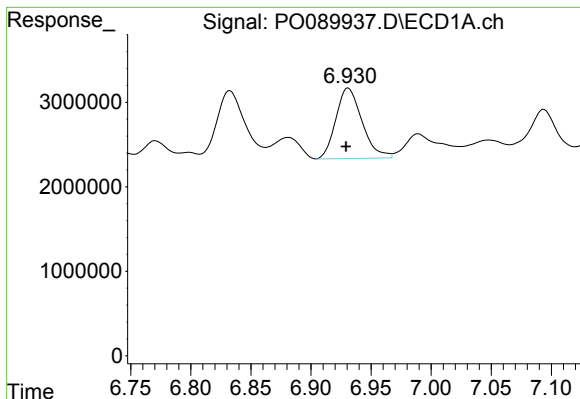


#28 AR-1254-3

R.T.: 6.931 min
Delta R.T.: 0.002 min
Response: 12635501
Conc: 72.95 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP2-1024


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/26/2022
Supervised By :Ankita Jodhani 10/27/2022

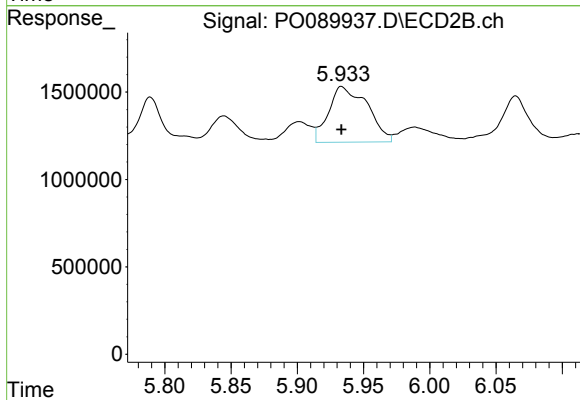


#28 AR-1254-3

R.T.: 5.933 min
Delta R.T.: 0.000 min
Response: 6488459
Conc: 82.28 ng/ml

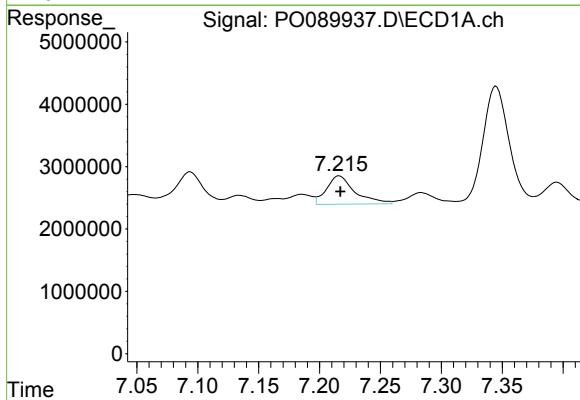


#29 AR-1254-4

R.T.: 7.216 min
Delta R.T.: 0.000 min
Response: 7382734
Conc: 58.24 ng/ml

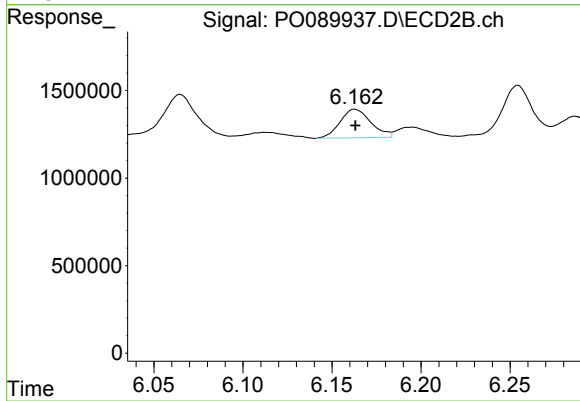

#29 AR-1254-4

R.T.: 6.163 min
Delta R.T.: 0.000 min
Response: 1977187
Conc: 41.49 ng/ml

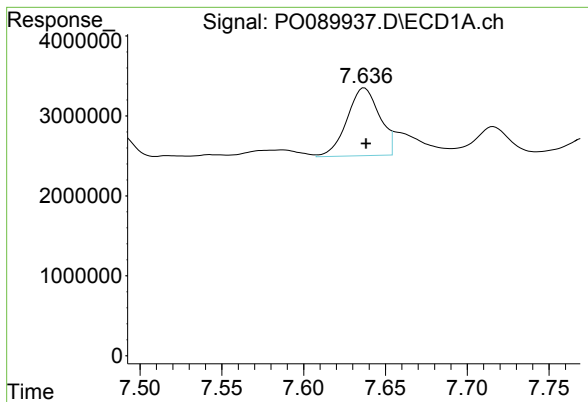


#30 AR-1254-5

R.T.: 7.636 min
Delta R.T.: -0.002 min
Response: 12084728
Conc: 86.78 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP2-1024

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/26/2022
Supervised By :Ankita Jodhani 10/27/2022

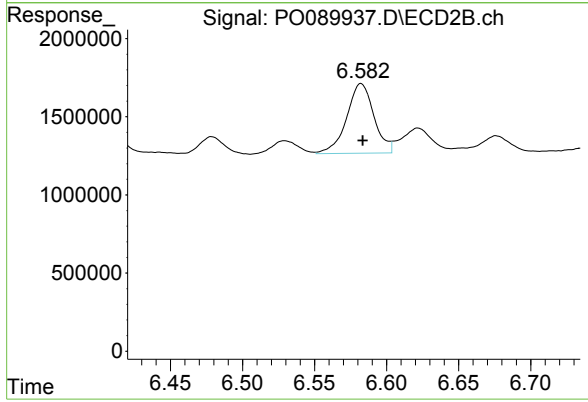

#30 AR-1254-5

R.T.: 6.582 min
Delta R.T.: -0.001 min
Response: 5877904
Conc: 83.18 ng/ml