

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102522\
 Data File : PO089941.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Oct 2022 21:45
 Operator : YP/AJ
 Sample : N5267-16
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TP6-1024

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/26/2022
 Supervised By :Ankita Jodhani 10/27/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 25 23:45:09 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102422.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Oct 25 02:35:13 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.307	3.487	40585642	16765634	12.754	16.753 #
2) SA Decachlor...	10.053	8.497	48211659	19296424	20.143	21.237
Target Compounds						
31) L7 AR-1260-1	7.094	6.064	6002668	2593070	44.221	46.905
32) L7 AR-1260-2	7.353	6.253	7694139	3065540	48.888	47.703
33) L7 AR-1260-3	7.715	6.407	4758776	2688312	44.301	44.534
34) L7 AR-1260-4	7.939	6.881	5927275	1913922	48.099m	40.166
35) L7 AR-1260-5	8.257	7.125	10875918	5063311	46.503	47.021

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102522\
Data File : P0089941.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Oct 2022 21:45
Operator : YP/AJ
Sample : N5267-16
Misc :
ALS Vial : 39 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
TP6-1024


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/26/2022
Supervised By :Ankita Jodhani 10/27/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 25 23:45:09 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102422.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Oct 25 02:35:13 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

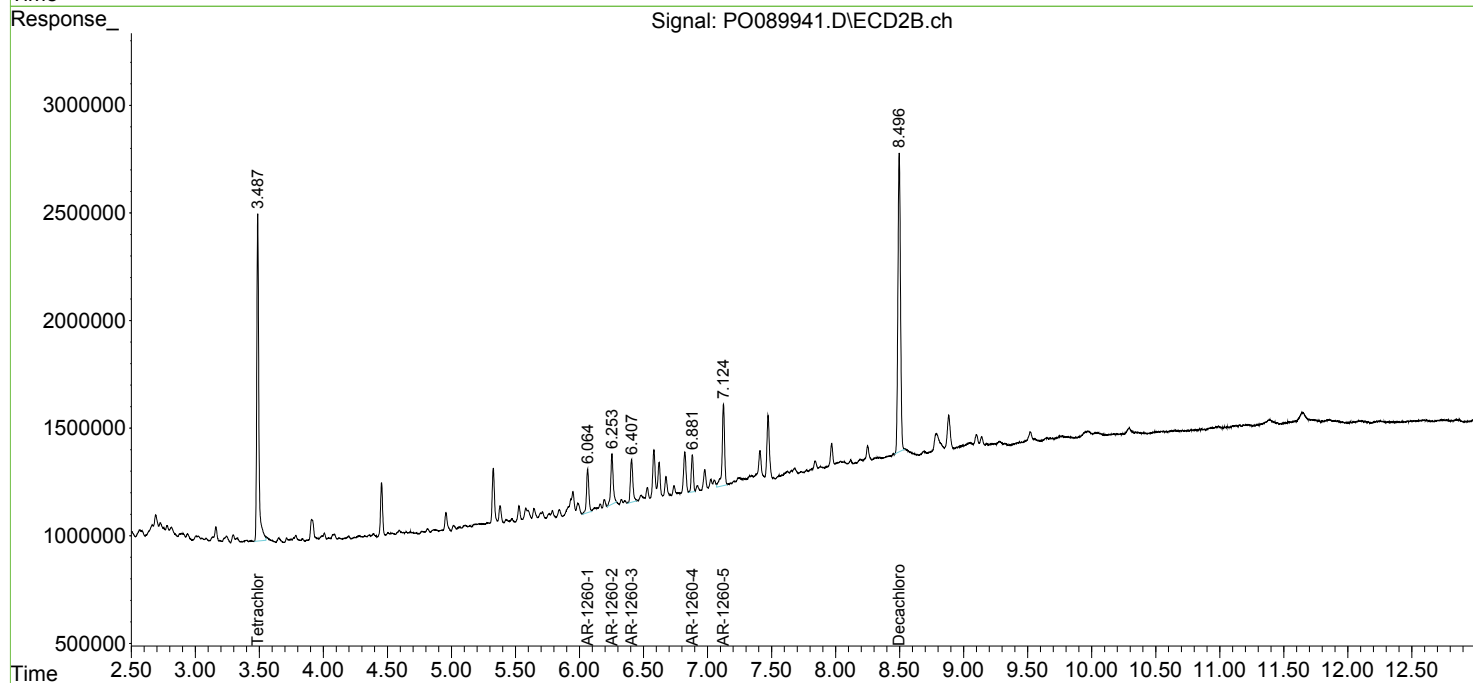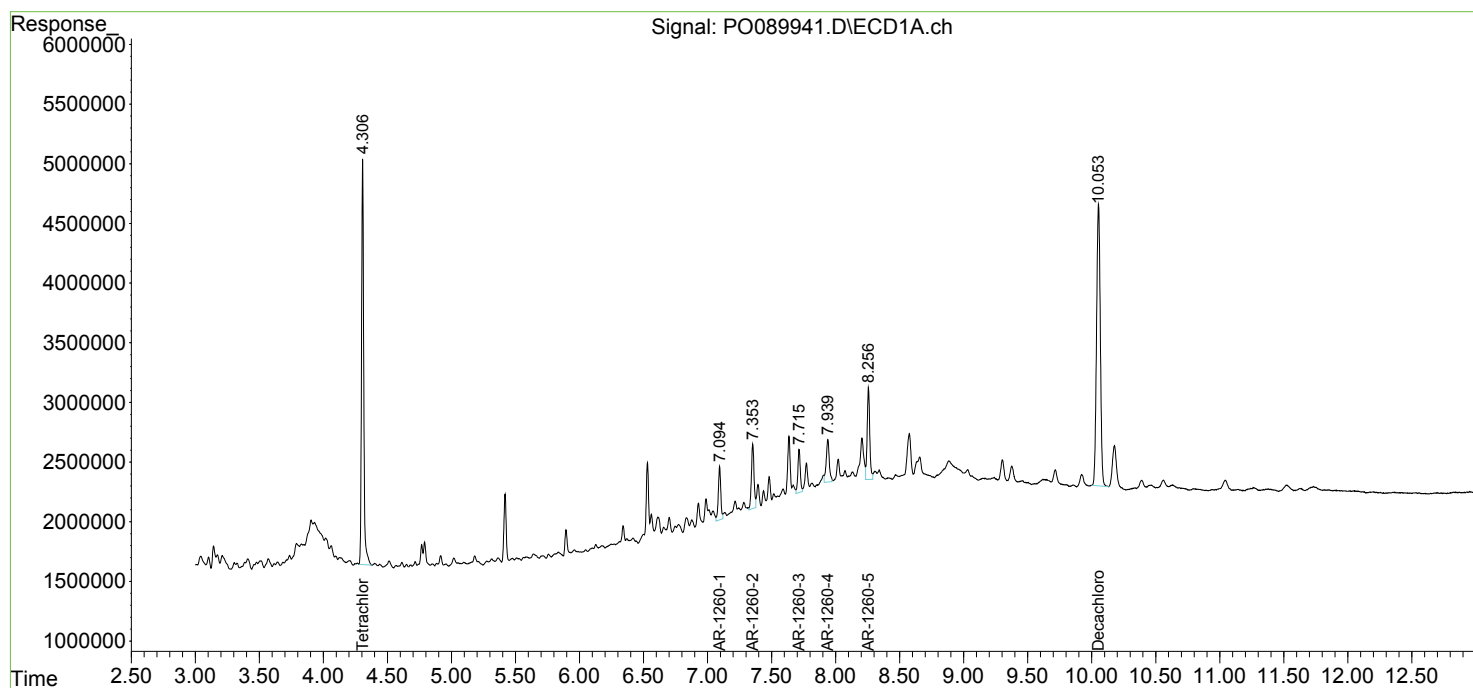

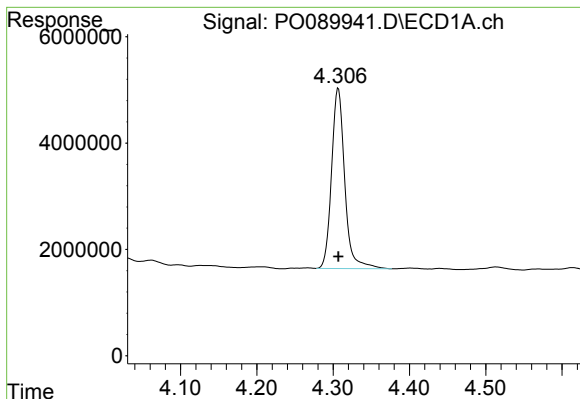


#1 Tetrachloro-m-xylene

R.T.: 4.307 min
Delta R.T.: 0.000 min
Response: 40585642
Conc: 12.75 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP6-1024


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/26/2022
Supervised By :Ankita Jodhani 10/27/2022

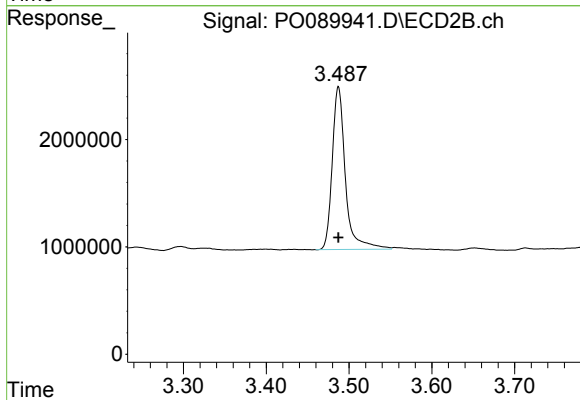


#1 Tetrachloro-m-xylene

R.T.: 3.487 min
Delta R.T.: 0.000 min
Response: 16765634
Conc: 16.75 ng/ml

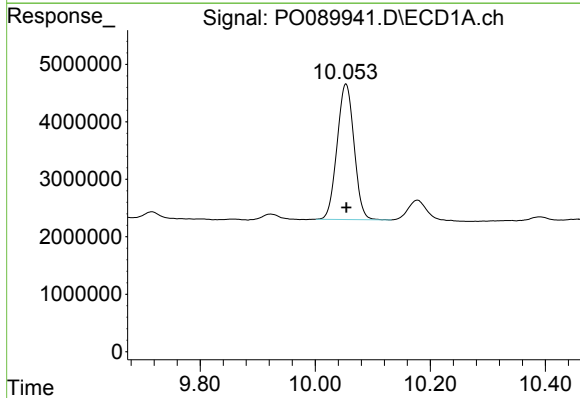


#2 Decachlorobiphenyl

R.T.: 10.053 min
Delta R.T.: -0.001 min
Response: 48211659
Conc: 20.14 ng/ml

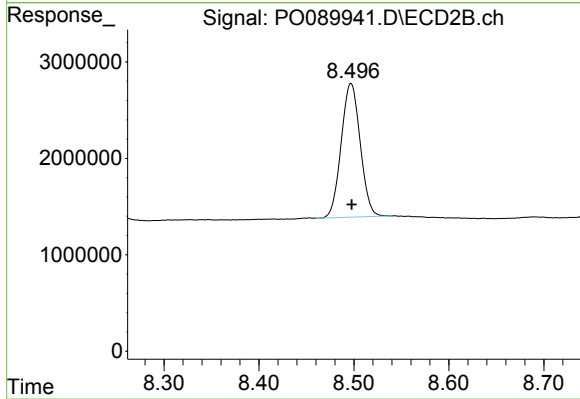

#2 Decachlorobiphenyl

R.T.: 8.497 min
Delta R.T.: 0.000 min
Response: 19296424
Conc: 21.24 ng/ml

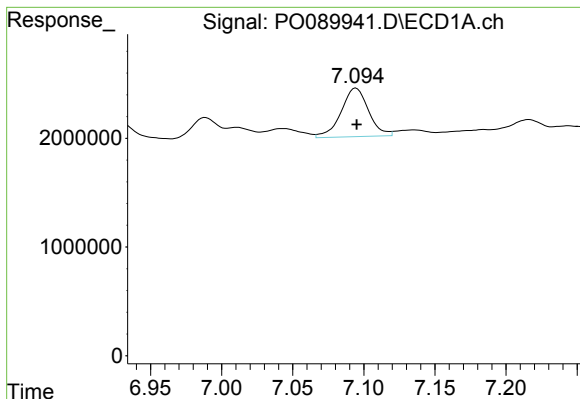


#31 AR-1260-1

R.T.: 7.094 min
Delta R.T.: 0.000 min
Response: 6002668
Conc: 44.22 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP6-1024


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/26/2022
Supervised By :Ankita Jodhani 10/27/2022

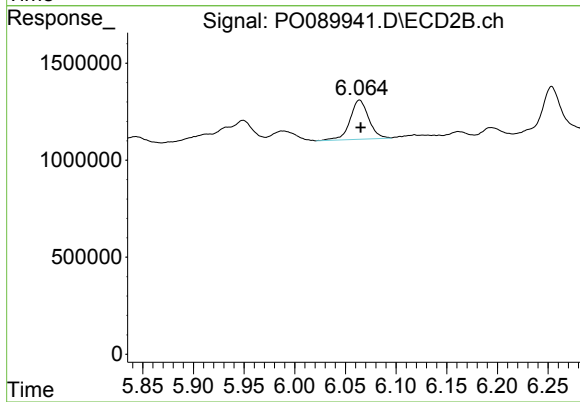


#31 AR-1260-1

R.T.: 6.064 min
Delta R.T.: -0.001 min
Response: 2593070
Conc: 46.91 ng/ml

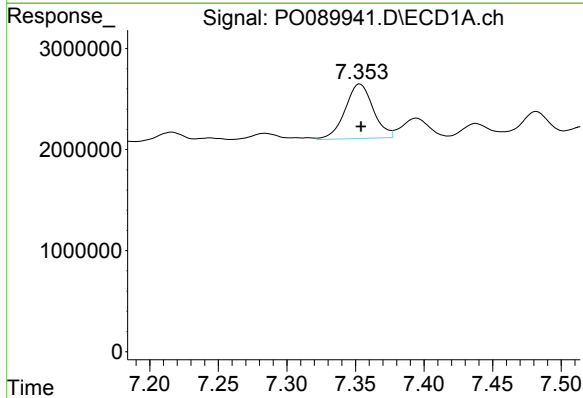


#32 AR-1260-2

R.T.: 7.353 min
Delta R.T.: 0.000 min
Response: 7694139
Conc: 48.89 ng/ml

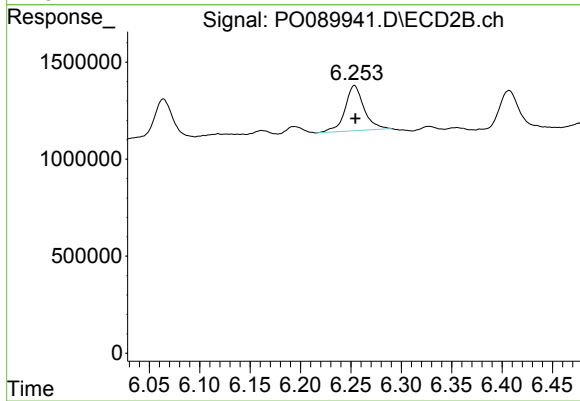

#32 AR-1260-2

R.T.: 6.253 min
Delta R.T.: 0.000 min
Response: 3065540
Conc: 47.70 ng/ml

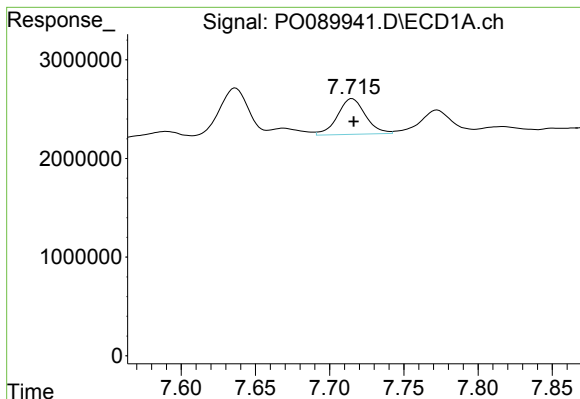


#33 AR-1260-3

R.T.: 7.715 min
Delta R.T.: 0.000 min
Response: 4758776
Conc: 44.30 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP6-1024


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/26/2022
Supervised By :Ankita Jodhani 10/27/2022

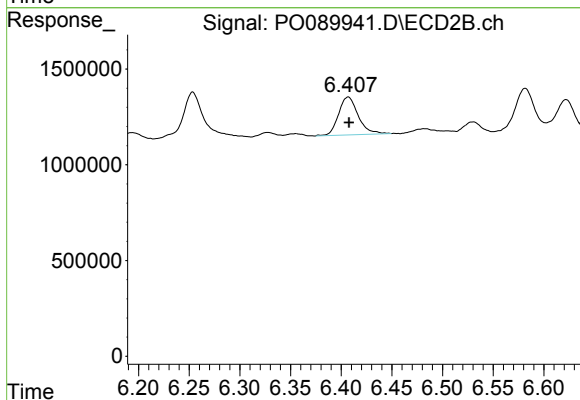


#33 AR-1260-3

R.T.: 6.407 min
Delta R.T.: 0.000 min
Response: 2688312
Conc: 44.53 ng/ml

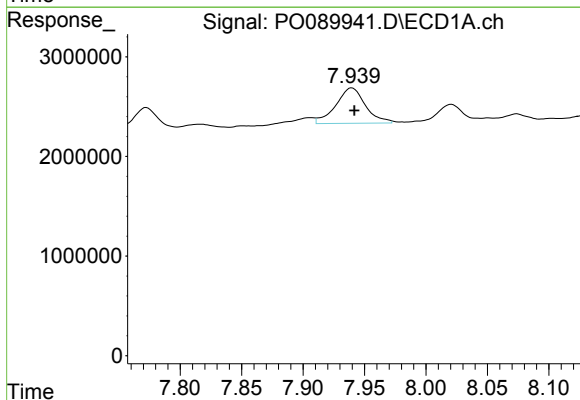


#34 AR-1260-4

R.T.: 7.939 min
Delta R.T.: -0.003 min
Response: 5927275
Conc: 48.10 ng/ml m

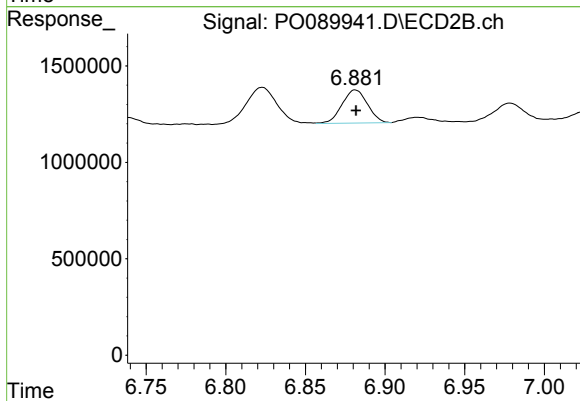

#34 AR-1260-4

R.T.: 6.881 min
Delta R.T.: 0.000 min
Response: 1913922
Conc: 40.17 ng/ml

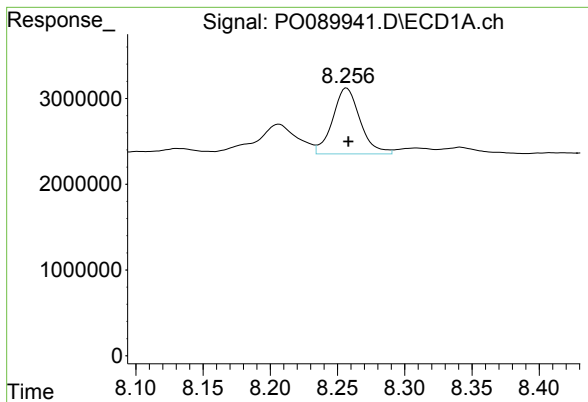


#35 AR-1260-5

R.T.: 8.257 min
Delta R.T.: -0.001 min
Response: 10875918
Conc: 46.50 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP6-1024

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/26/2022
Supervised By :Ankita Jodhani 10/27/2022

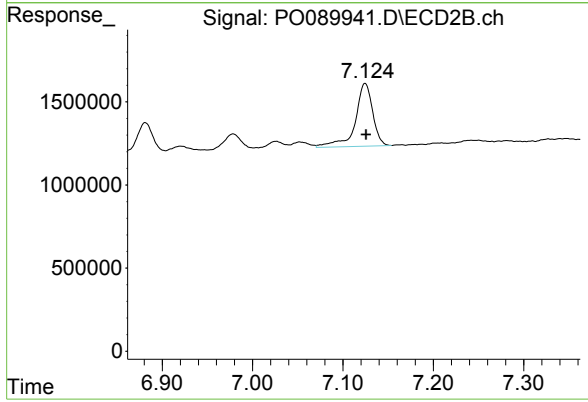

#35 AR-1260-5

R.T.: 7.125 min
Delta R.T.: -0.001 min
Response: 5063311
Conc: 47.02 ng/ml