

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102523\
 Data File : PO098924.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Oct 2023 16:52
 Operator : YP/AJ
 Sample : 05040-01
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 M-4(50FT)(0-5)

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/26/2023
 Supervised By :Ankita Jodhani 10/26/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 25 17:56:39 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102523.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 25 06:04:36 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.477	3.632	41121045	12836418	20.811m	17.836
2) SA Decachlor...	10.280	8.630	22745978	9747133	20.078	18.167

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102523\
Data File : PO098924.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Oct 2023 16:52
Operator : YP/AJ
Sample : 05040-01
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
M-4(50FT)(0-5)


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/26/2023
Supervised By :Ankita Jodhani 10/26/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 25 17:56:39 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102523.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 25 06:04:36 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

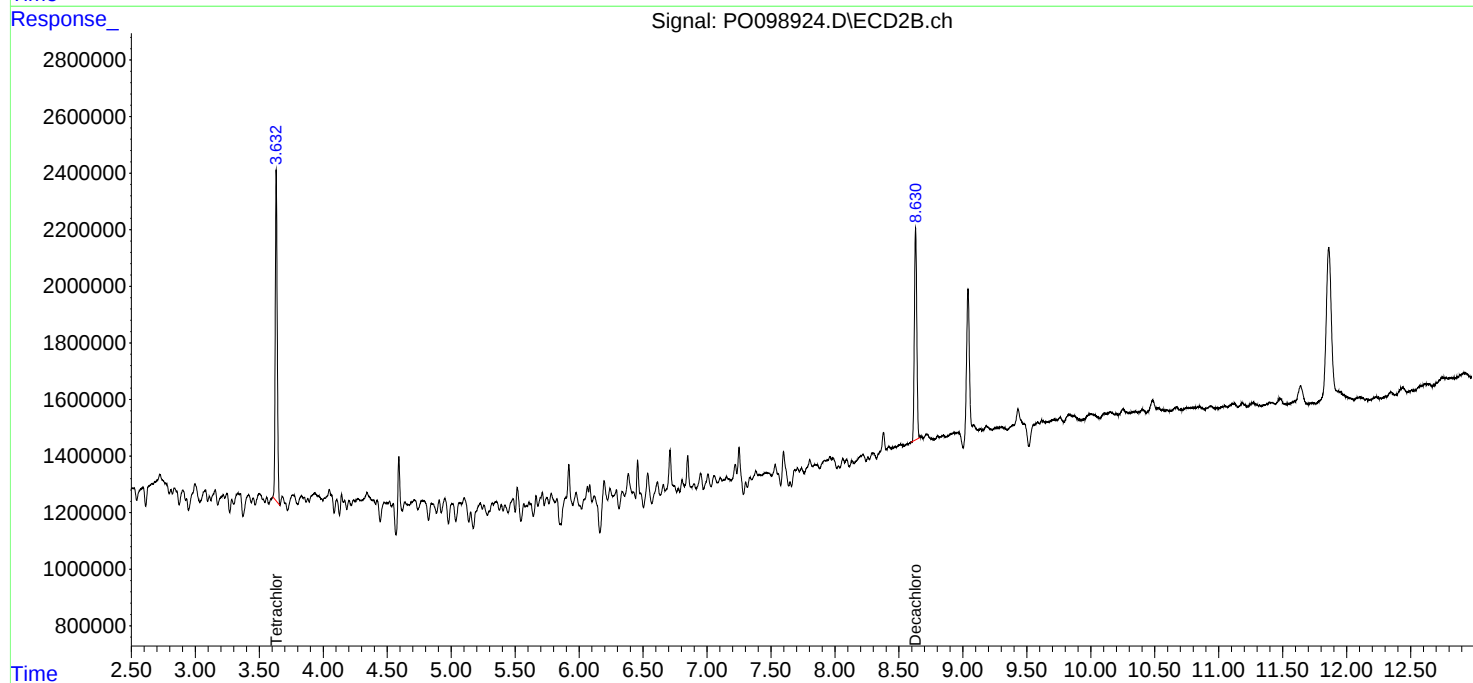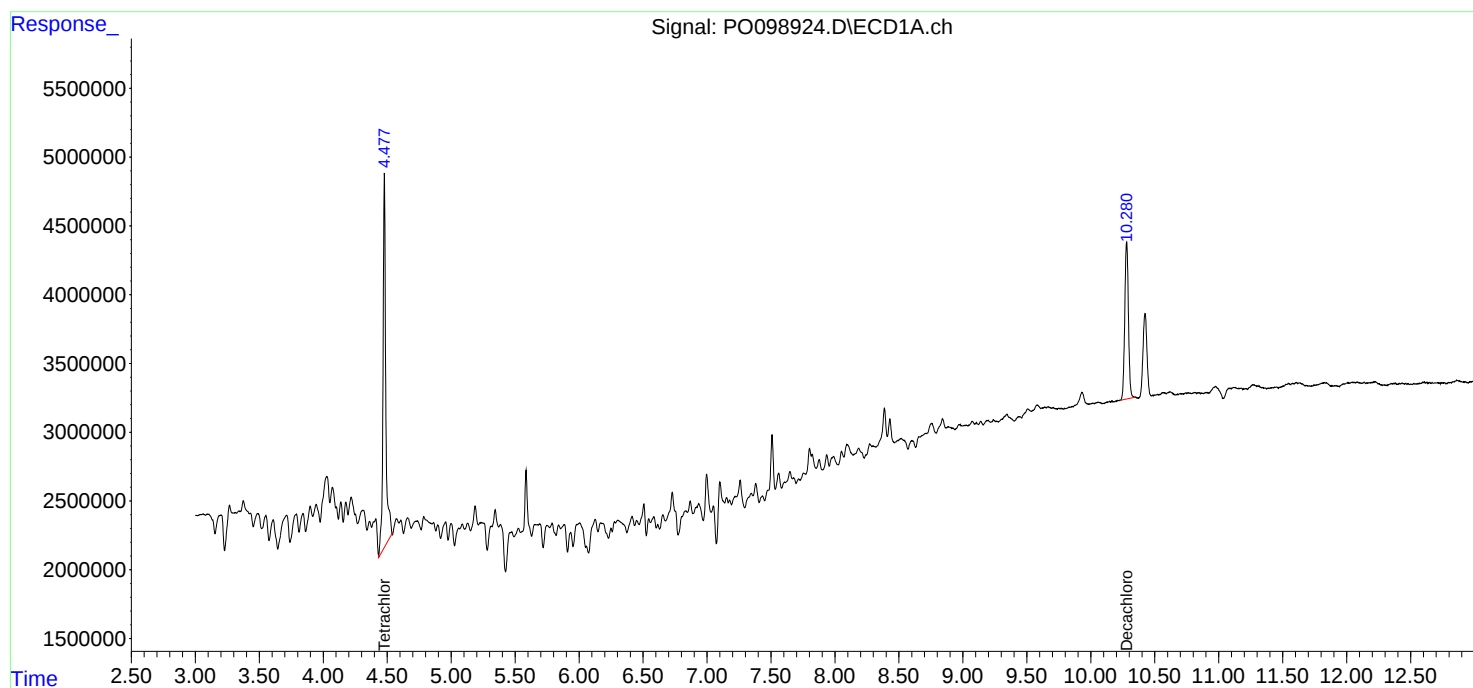

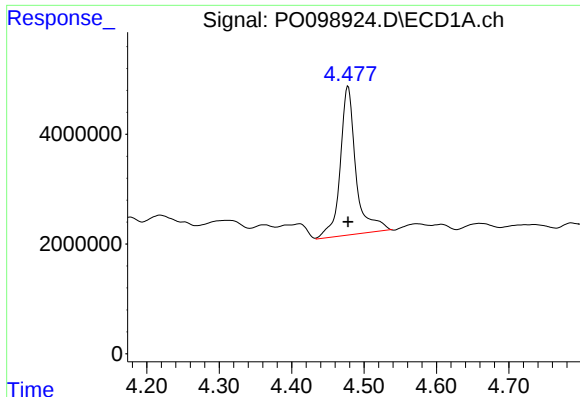


#1 Tetrachloro-m-xylene

R.T.: 4.477 min
Delta R.T.: 0.000 min
Response: 41121045
Conc: 20.81 ng/ml

Instrument :
ECD_O
ClientSampleId :
M-4(50FT)(0-5)


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/26/2023
Supervised By :Ankita Jodhani 10/26/2023

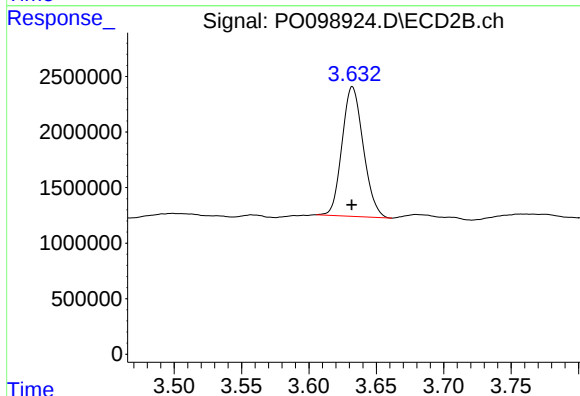


#1 Tetrachloro-m-xylene

R.T.: 3.632 min
Delta R.T.: 0.000 min
Response: 12836418
Conc: 17.84 ng/ml

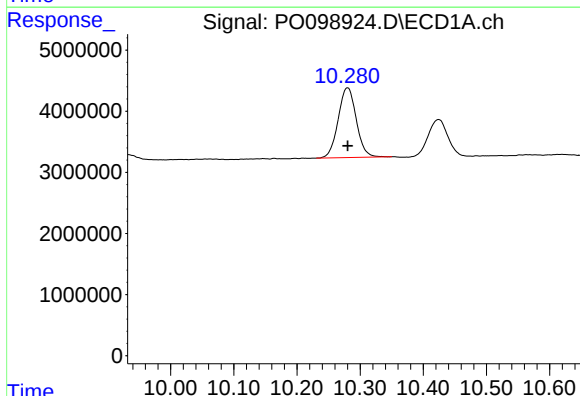

#2 Decachlorobiphenyl

R.T.: 10.280 min
Delta R.T.: 0.000 min
Response: 22745978
Conc: 20.08 ng/ml

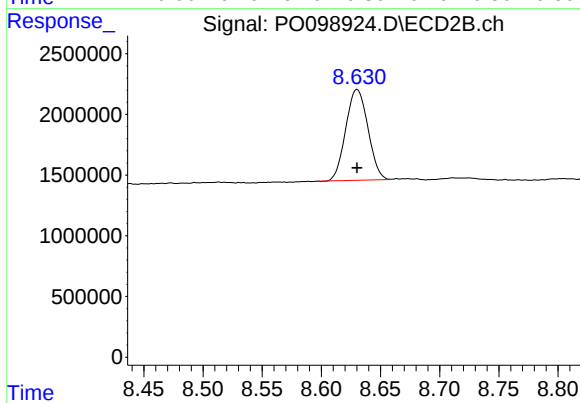

#2 Decachlorobiphenyl

R.T.: 8.630 min
Delta R.T.: 0.000 min
Response: 9747133
Conc: 18.17 ng/ml