

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0102524\
 Data File : P0107389.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Oct 2024 17:55
 Operator : YP/AJ
 Sample : P4531-01
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 OR-03-102424

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/28/2024
 Supervised By :Ankita Jodhani 10/28/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 26 00:02:50 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 16 04:53:16 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.371	3.644	169.5E6	79646201	18.595m	24.746m#
2) SA Decachlor...	10.062	8.638	52309576	47597080	21.321	17.361

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102524\
Data File : PO107389.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Oct 2024 17:55
Operator : YP/AJ
Sample : P4531-01
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
OR-03-102424


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/28/2024
Supervised By :Ankita Jodhani 10/28/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 26 00:02:50 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 16 04:53:16 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

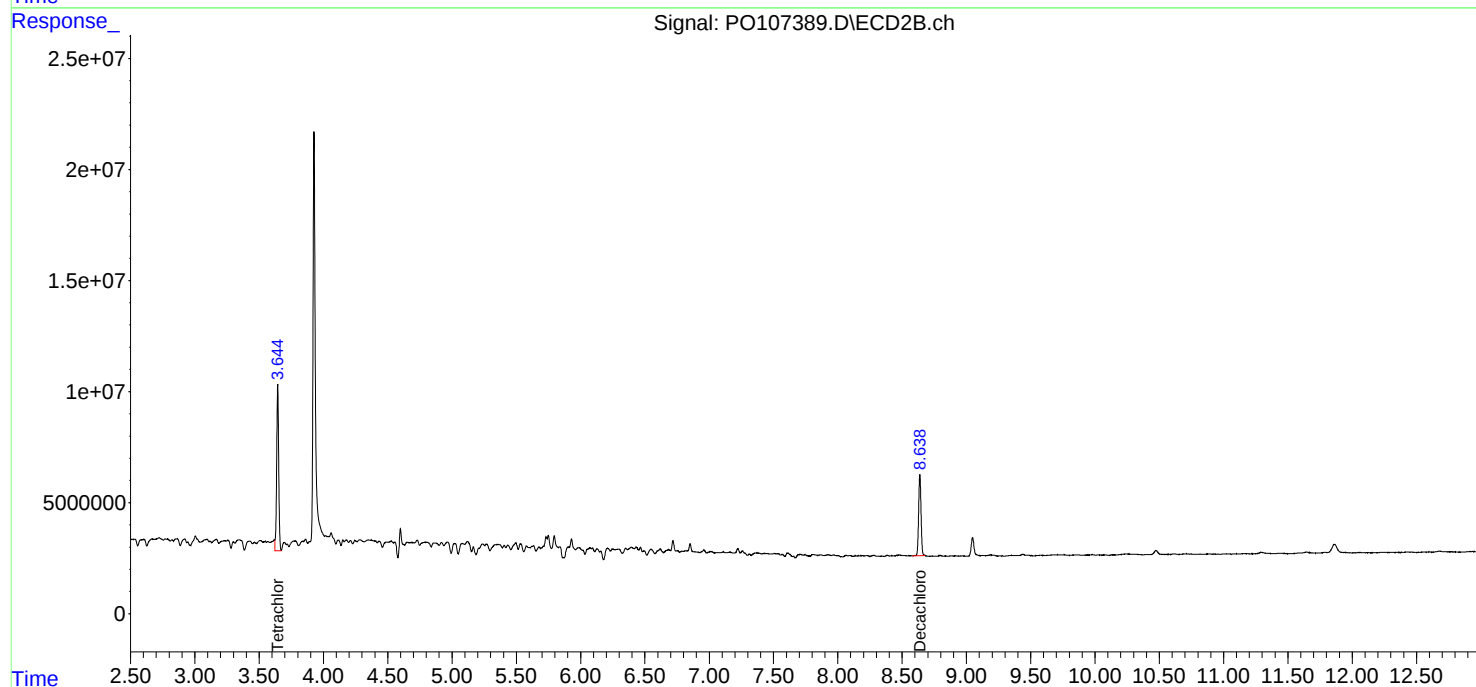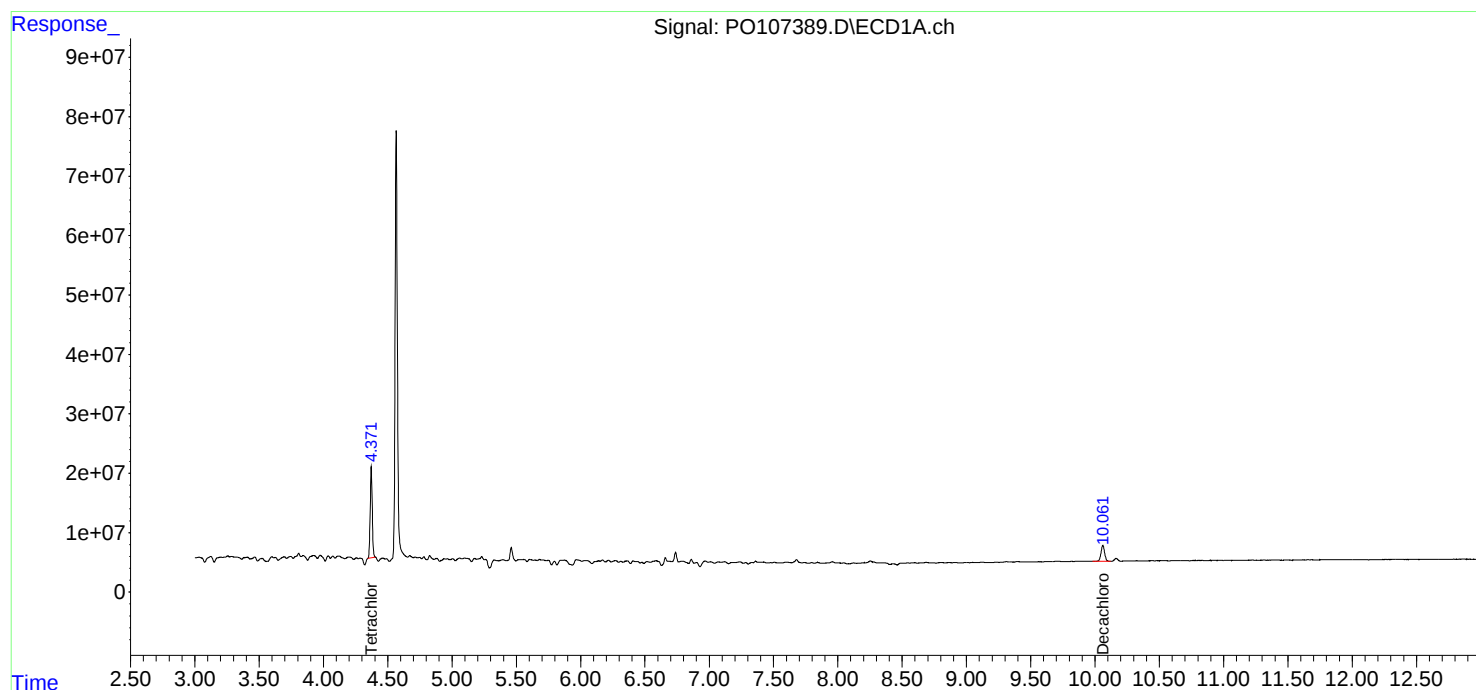

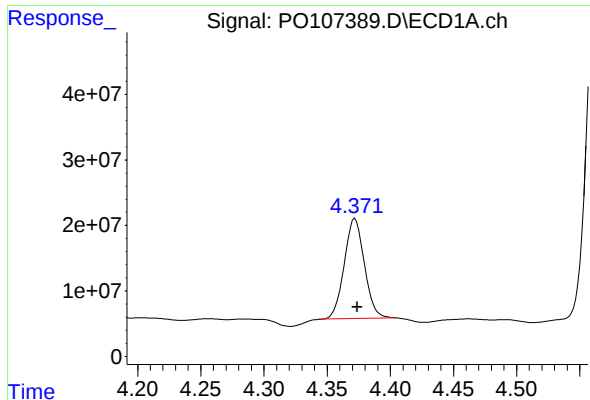


#1 Tetrachloro-m-xylene

R.T.: 4.371 min
Delta R.T.: -0.003 min
Response: 169470264
Conc: 18.59 ng/ml

Instrument :
ECD_O
ClientSampleId :
OR-03-102424


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/28/2024
Supervised By :Ankita Jodhani 10/28/2024

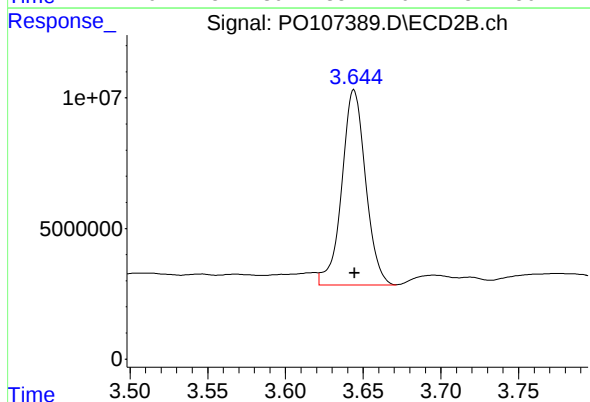


#1 Tetrachloro-m-xylene

R.T.: 3.644 min
Delta R.T.: 0.000 min
Response: 79646201
Conc: 24.75 ng/ml

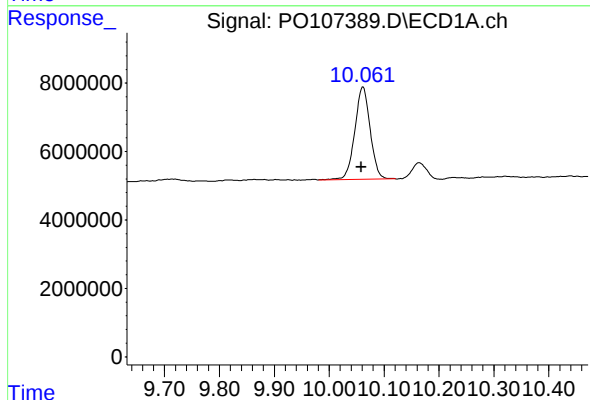

#2 Decachlorobiphenyl

R.T.: 10.062 min
Delta R.T.: 0.003 min
Response: 52309576
Conc: 21.32 ng/ml

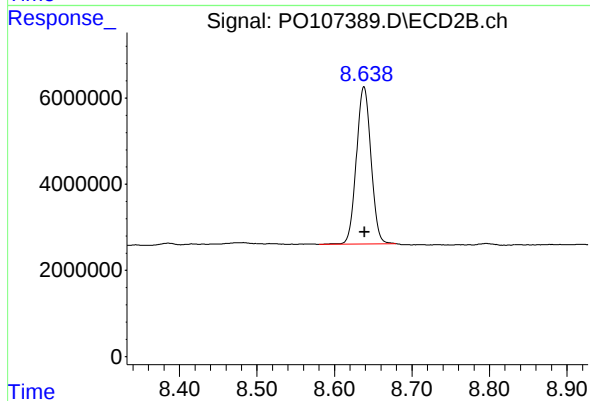

#2 Decachlorobiphenyl

R.T.: 8.638 min
Delta R.T.: 0.000 min
Response: 47597080
Conc: 17.36 ng/ml