

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0102524\
 Data File : P0107403.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Oct 2024 22:37
 Operator : YP/AJ
 Sample : P4512-01
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 3140

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/28/2024
 Supervised By :Ankita Jodhani 10/28/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 26 00:11:32 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 16 04:53:16 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.372	3.645	131.7E6	54313955	14.455m	16.876m
2) SA Decachlor...	10.065	8.639	50105281	47984000	20.423	17.502m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102524\
Data File : PO107403.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Oct 2024 22:37
Operator : YP/AJ
Sample : P4512-01
Misc :
ALS Vial : 25 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
3140


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/28/2024
Supervised By :Ankita Jodhani 10/28/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 26 00:11:32 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 16 04:53:16 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

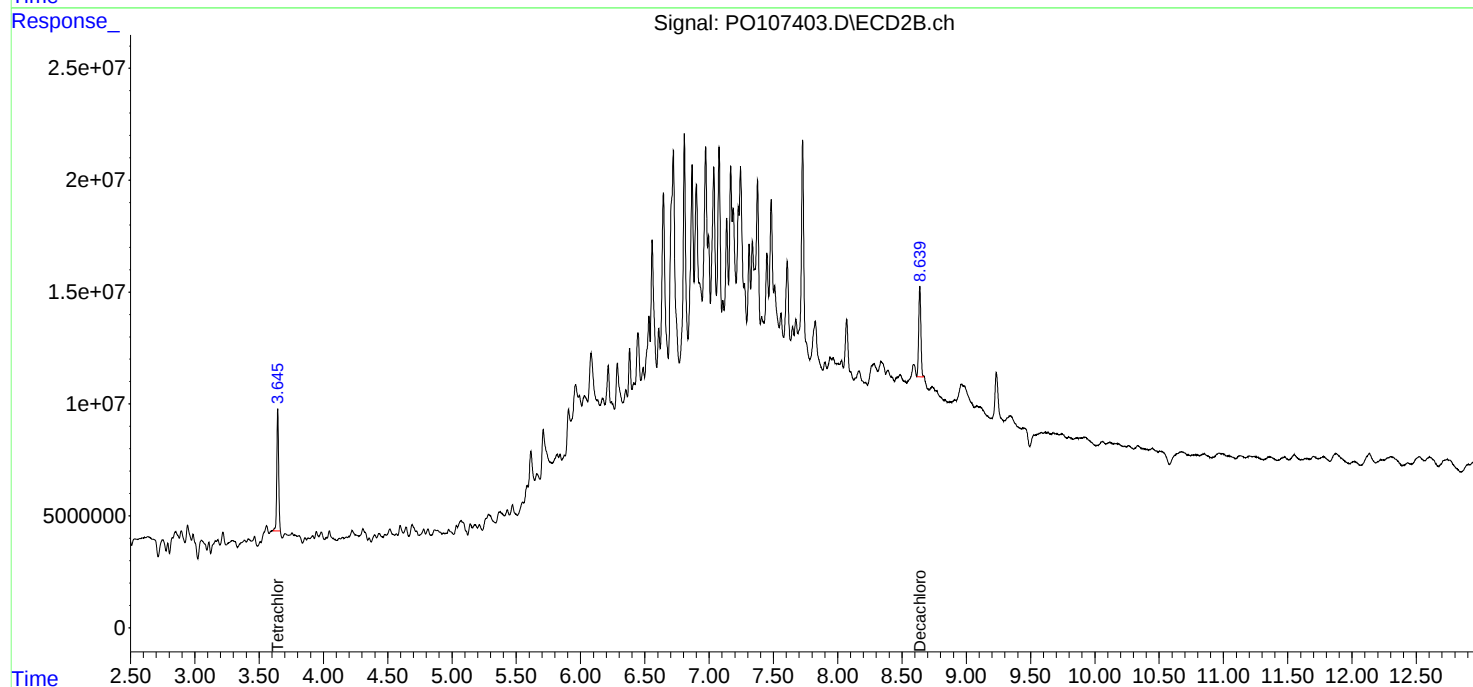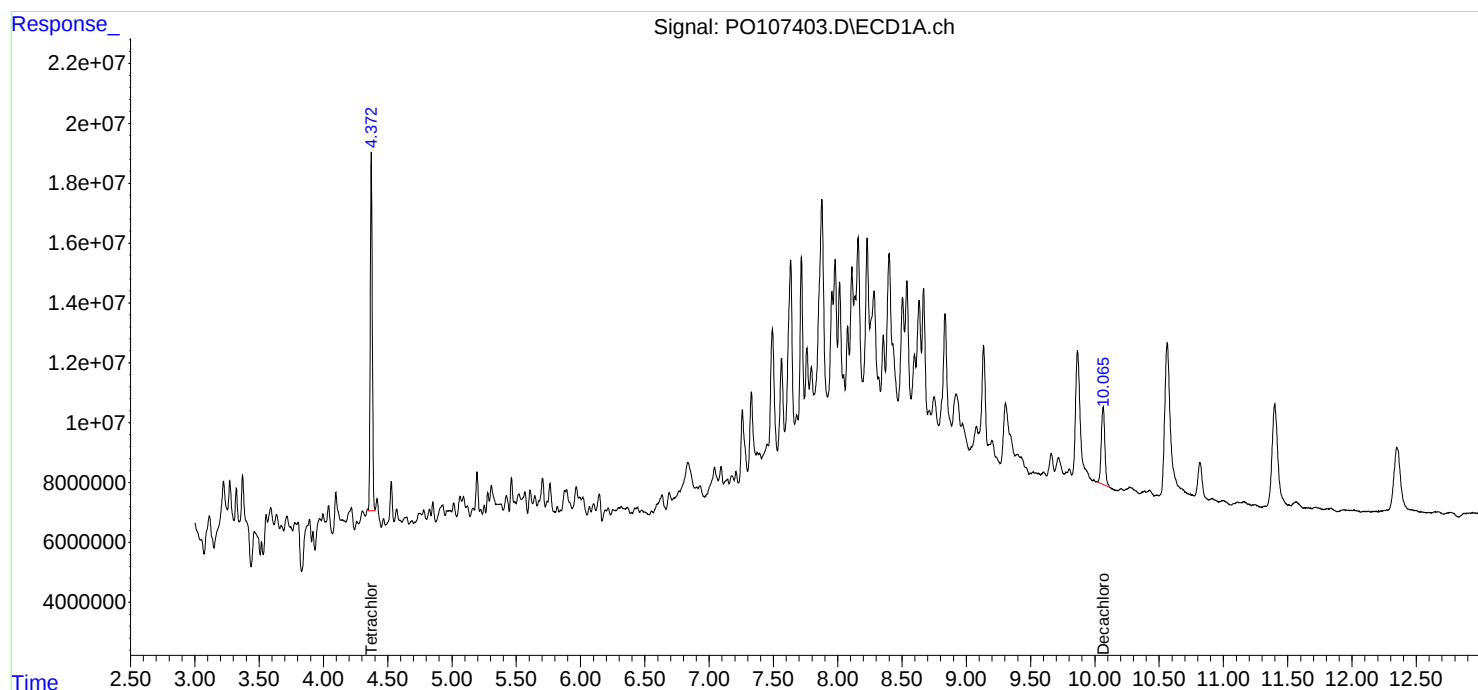

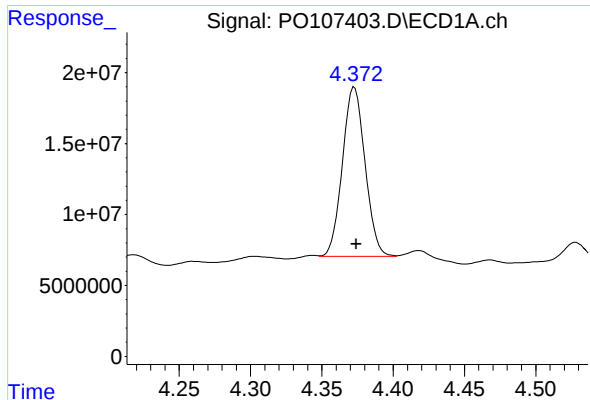


#1 Tetrachloro-m-xylene

R.T.: 4.372 min
Delta R.T.: -0.002 min
Response: 131740748
Conc: 14.45 ng/ml

Instrument :
ECD_O
ClientSampleId :
3140


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/28/2024
Supervised By :Ankita Jodhani 10/28/2024

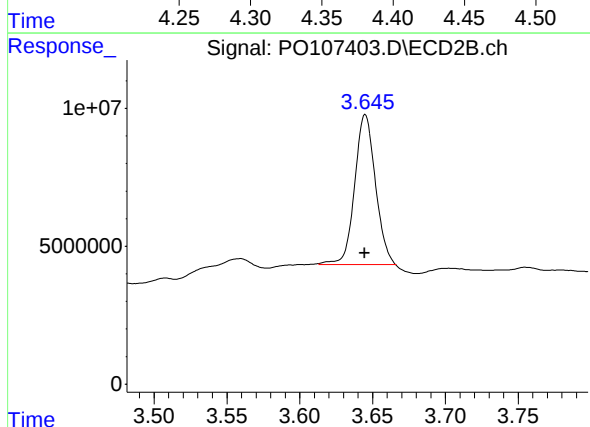


#1 Tetrachloro-m-xylene

R.T.: 3.645 min
Delta R.T.: 0.000 min
Response: 54313955
Conc: 16.88 ng/ml

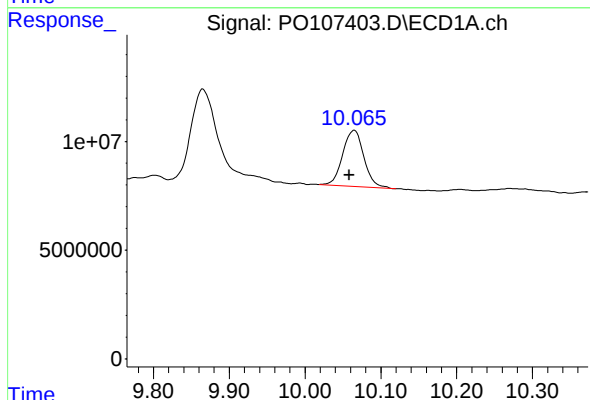

#2 Decachlorobiphenyl

R.T.: 10.065 min
Delta R.T.: 0.006 min
Response: 50105281
Conc: 20.42 ng/ml

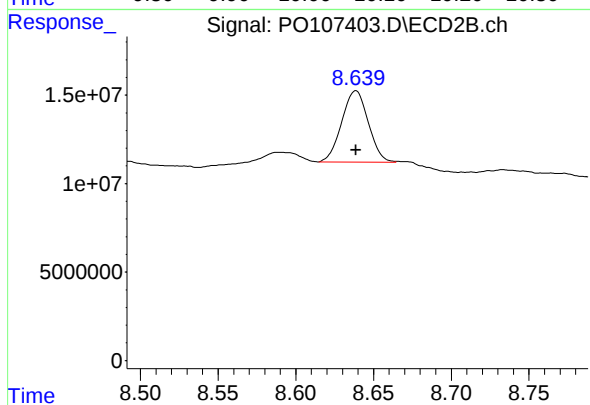

#2 Decachlorobiphenyl

R.T.: 8.639 min
Delta R.T.: 0.000 min
Response: 47984000
Conc: 17.50 ng/ml