

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0102524\
 Data File : P0107404.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Oct 2024 22:55
 Operator : YP/AJ
 Sample : P4512-02
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 3149

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/28/2024
 Supervised By :Ankita Jodhani 10/28/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 26 00:12:16 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 16 04:53:16 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.372	3.644	112.3E6	43206792	12.321	13.425m
2) SA Decachlor...	10.063	8.639	22919782	12105189	9.342	4.415m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102524\
Data File : PO107404.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Oct 2024 22:55
Operator : YP/AJ
Sample : P4512-02
Misc :
ALS Vial : 26 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
3149


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/28/2024
Supervised By :Ankita Jodhani 10/28/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 26 00:12:16 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 16 04:53:16 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

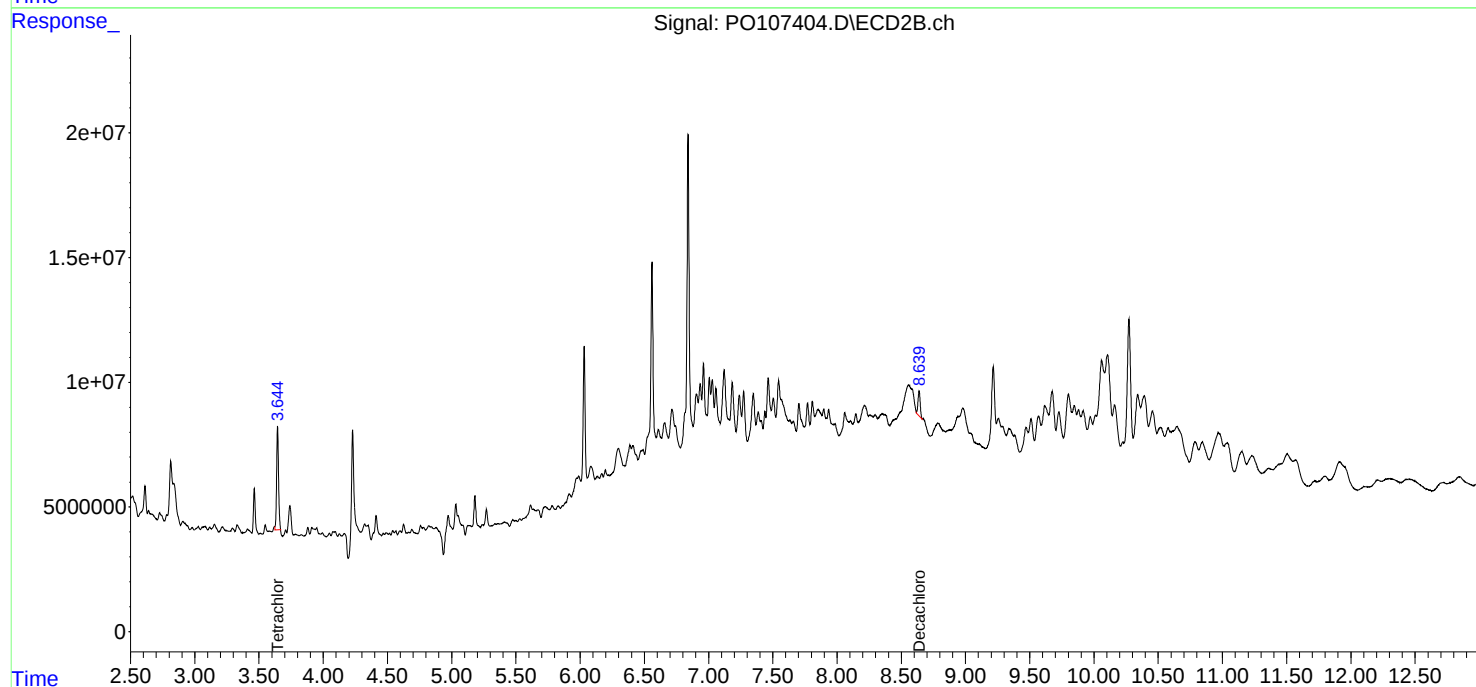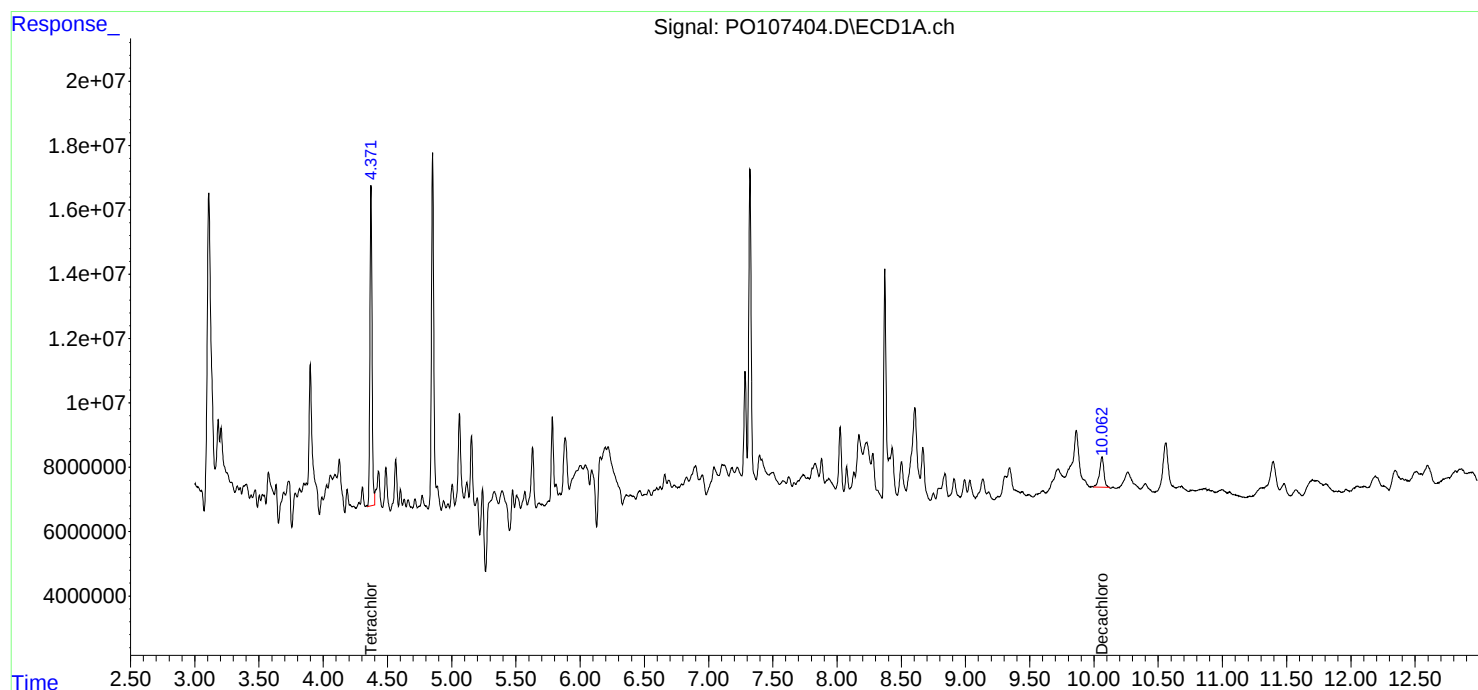

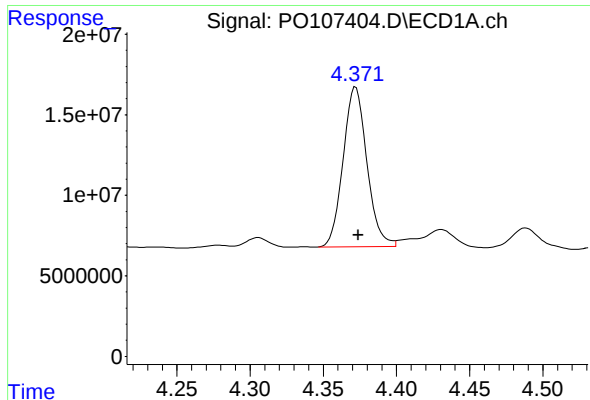


#1 Tetrachloro-m-xylene

R.T.: 4.372 min
Delta R.T.: -0.002 min
Response: 112289901
Conc: 12.32 ng/ml

Instrument :
ECD_O
ClientSampleId :
3149


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/28/2024
Supervised By :Ankita Jodhani 10/28/2024

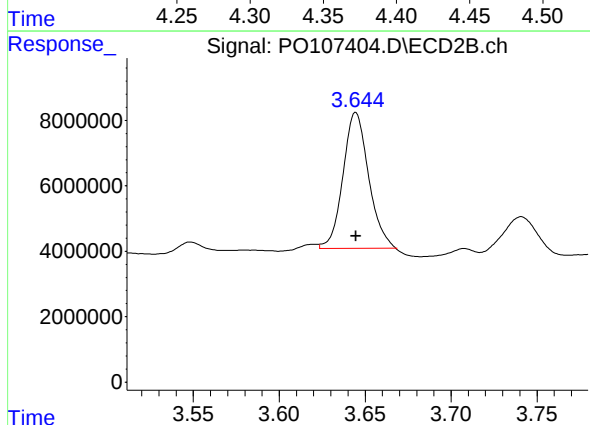


#1 Tetrachloro-m-xylene

R.T.: 3.644 min
Delta R.T.: 0.000 min
Response: 43206792
Conc: 13.42 ng/ml

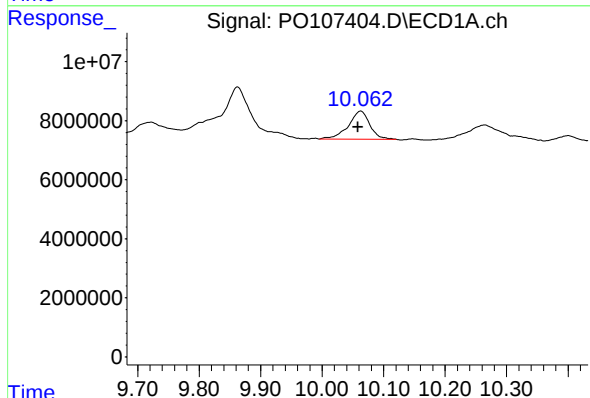

#2 Decachlorobiphenyl

R.T.: 10.063 min
Delta R.T.: 0.004 min
Response: 22919782
Conc: 9.34 ng/ml

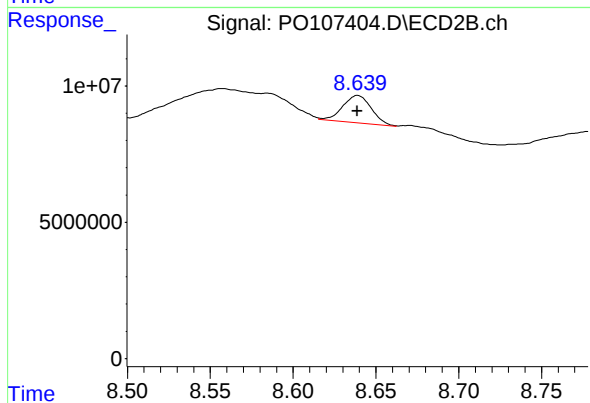

#2 Decachlorobiphenyl

R.T.: 8.639 min
Delta R.T.: 0.000 min
Response: 12105189
Conc: 4.42 ng/ml