

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102618\
 Data File : PO050660.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 27 Oct 2018 9:59
 Operator : SM/SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 29 01:03:30 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101818.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Oct 19 02:02:26 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.355	3.350	8322817	4713768	27.892	23.976
2)	SA Decachlor...	10.019	8.099	7157109	5255214	32.984	27.494
Target Compounds							
20)	L4 AR-1242-5	0.000	5.194	0	48536	N.D.	8.700 #
25)	L5 AR-1248-5	0.000	5.194	0	48536	N.D.	6.138 #
26)	L6 AR-1254-1	0.000	5.194	0	48536	N.D.	3.348 #
27)	L6 AR-1254-2	0.000	5.256	0	27547	N.D.	2.168 #
29)	L6 AR-1254-4	0.000	5.940	0	151995	N.D.	13.052 #
32)	L7 AR-1260-2	0.000	5.940	0	151995	N.D.	8.216 #
45)	L9 AR-1268-5	0.000	7.919	0	245250	N.D.	3.235 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102618\
Data File : PO050660.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 27 Oct 2018 9:59
Operator : SM/SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 29 01:03:30 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101818.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Oct 19 02:02:26 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

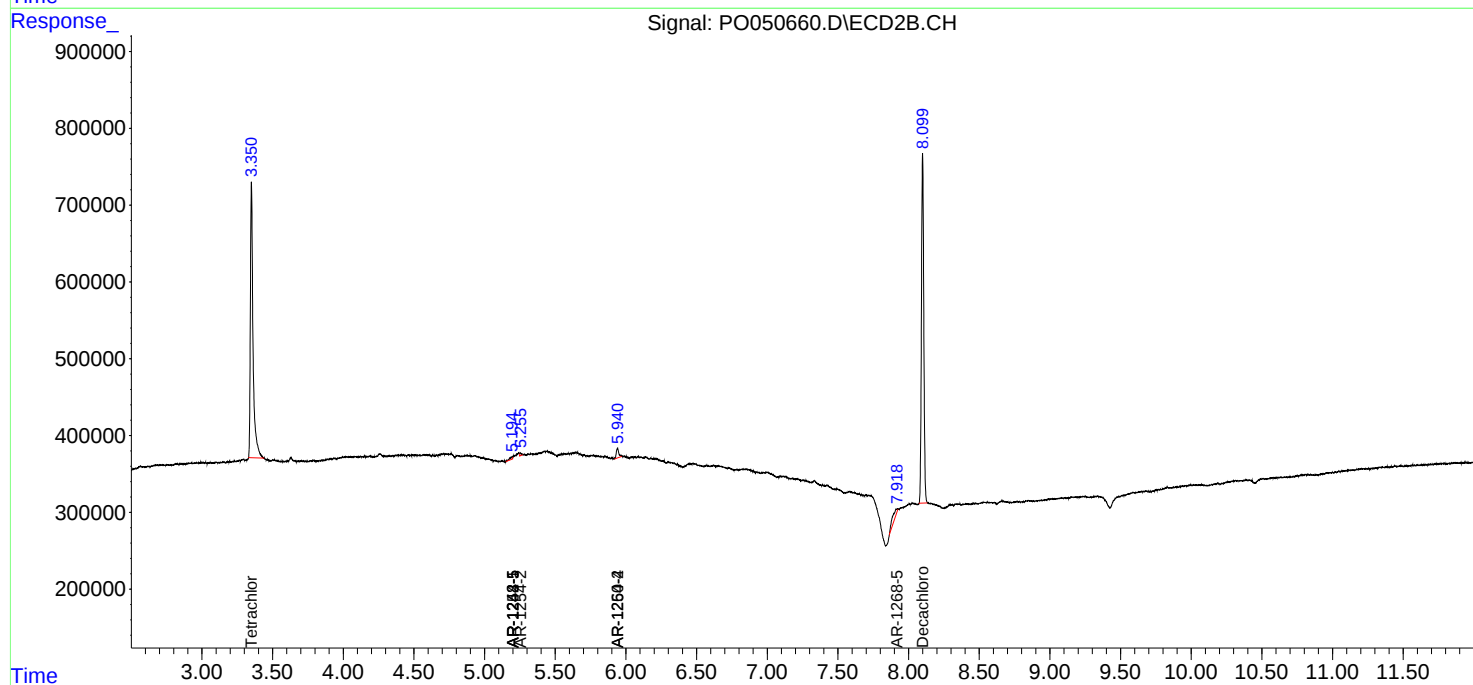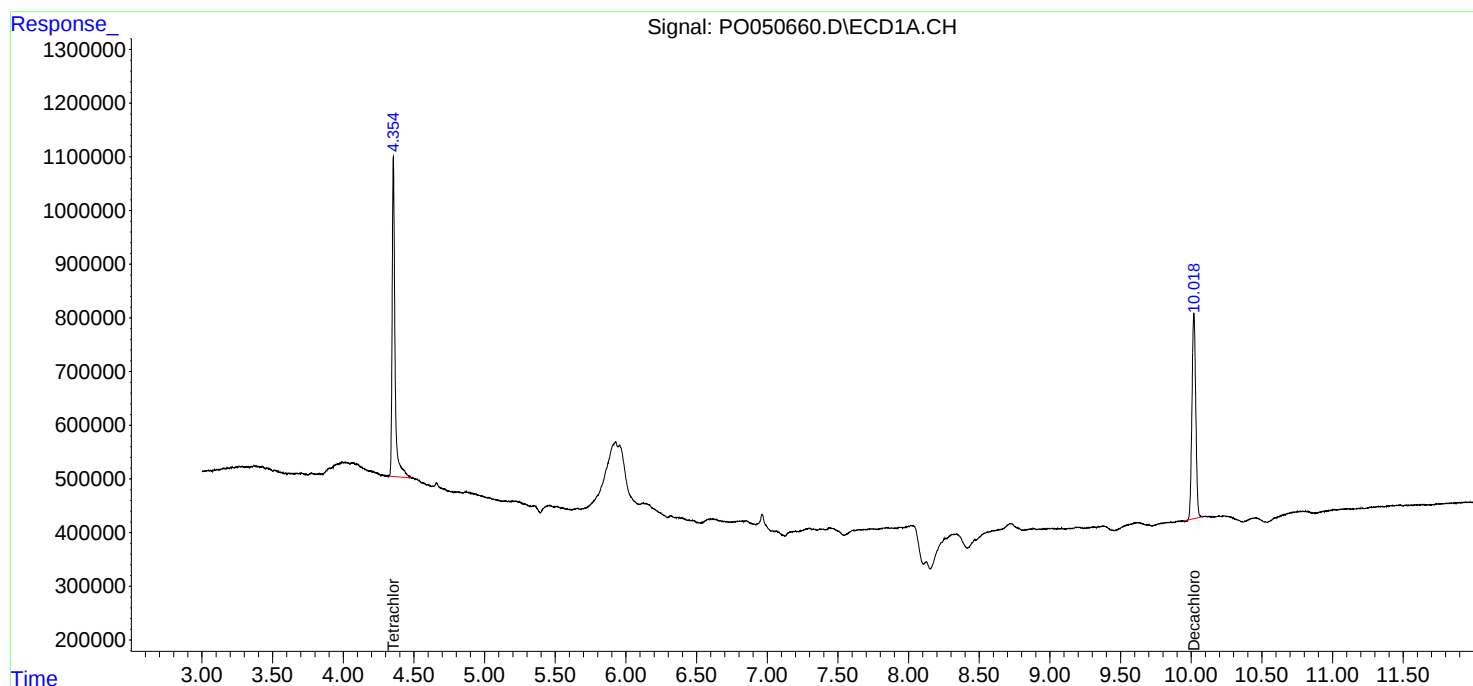


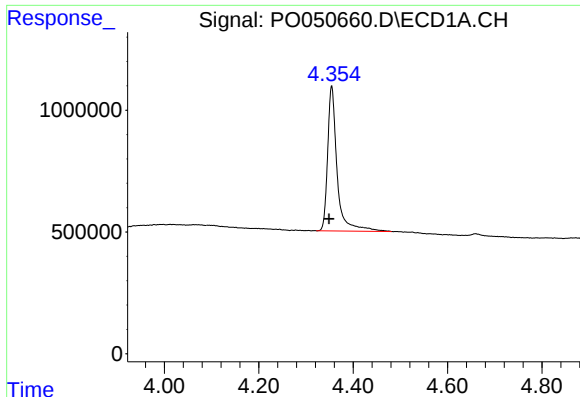

#1 Tetrachloro-m-xylene


R.T.: 4.355 min
Delta R.T.: 0.006 min
Response: 8322817
Conc: 27.89 ng/ml

Instrument :
ECD_O
ClientSampleId :

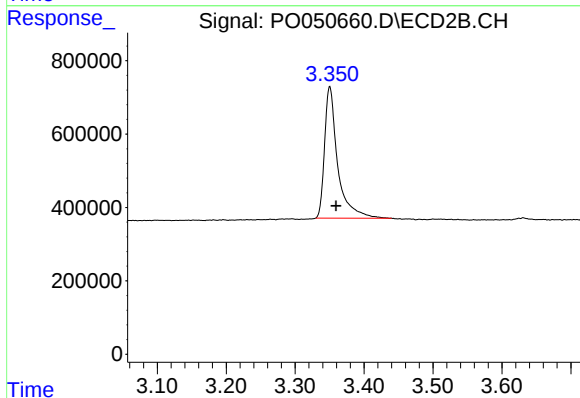


#1 Tetrachloro-m-xylene

R.T.: 3.350 min
Delta R.T.: -0.009 min
Response: 4713768
Conc: 23.98 ng/ml

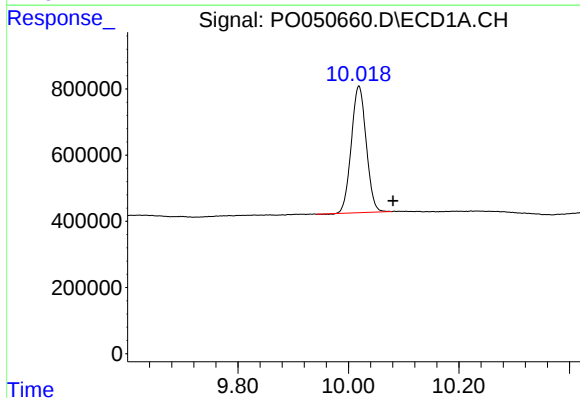


#2 Decachlorobiphenyl

R.T.: 10.019 min
Delta R.T.: -0.062 min
Response: 7157109
Conc: 32.98 ng/ml

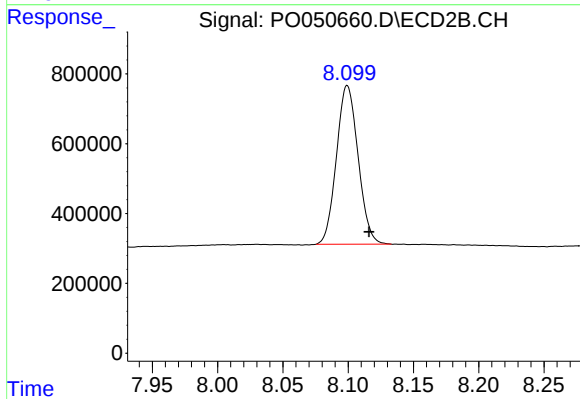

#2 Decachlorobiphenyl


R.T.: 8.099 min
Delta R.T.: -0.017 min
Response: 5255214
Conc: 27.49 ng/ml

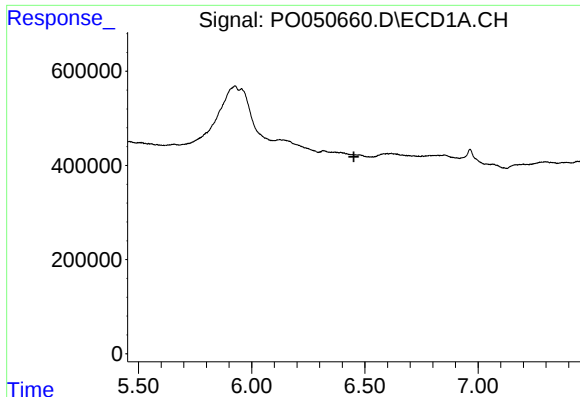

#20 AR-1242-5


R.T.: 0.000 min
Exp R.T.: 6.451 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

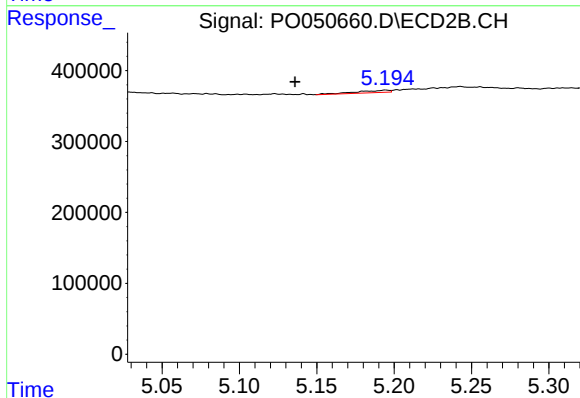


#20 AR-1242-5

R.T.: 5.194 min
Delta R.T.: 0.058 min
Response: 48536
Conc: 8.70 ng/ml

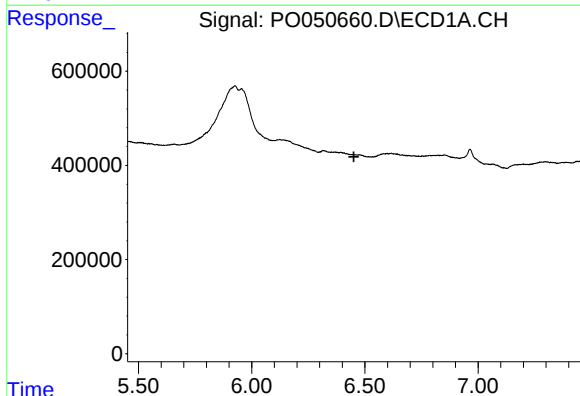


#25 AR-1248-5

R.T.: 0.000 min
Exp R.T.: 6.451 min
Response: 0
Conc: N.D.

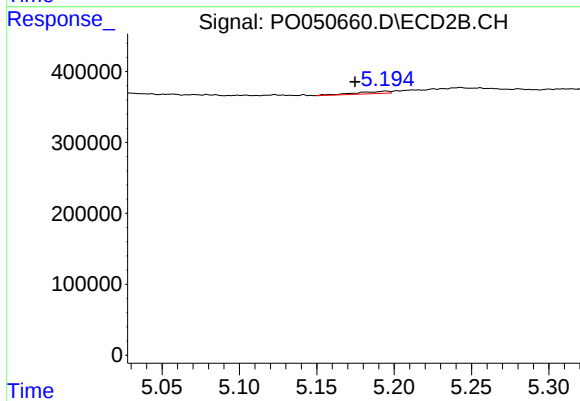

#25 AR-1248-5


R.T.: 5.194 min
Delta R.T.: 0.020 min
Response: 48536
Conc: 6.14 ng/ml

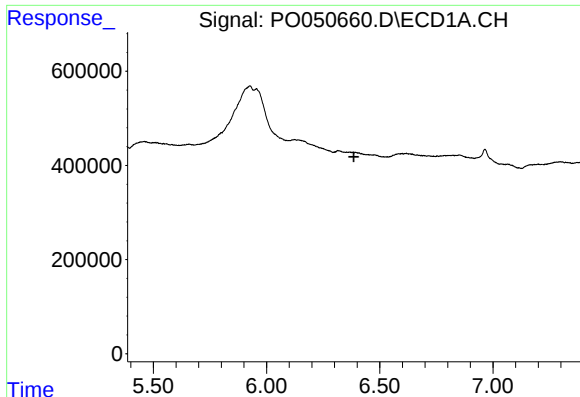

#26 AR-1254-1


R.T.: 0.000 min
Exp R.T. : 6.386 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

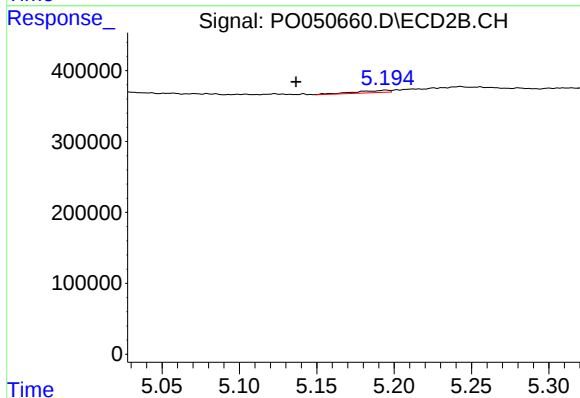


#26 AR-1254-1

R.T.: 5.194 min
Delta R.T.: 0.058 min
Response: 48536
Conc: 3.35 ng/ml

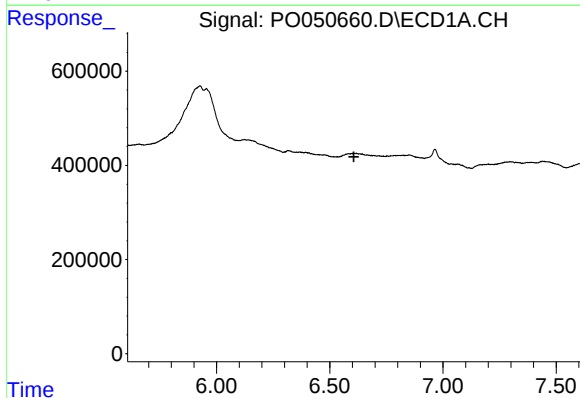


#27 AR-1254-2

R.T.: 0.000 min
Exp R.T. : 6.606 min
Response: 0
Conc: N.D.

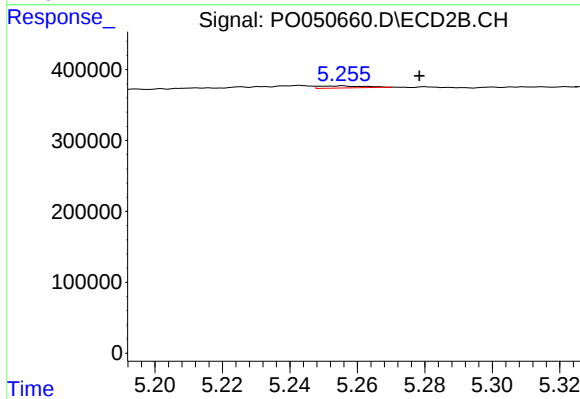

#27 AR-1254-2


R.T.: 5.256 min
Delta R.T.: -0.023 min
Response: 27547
Conc: 2.17 ng/ml

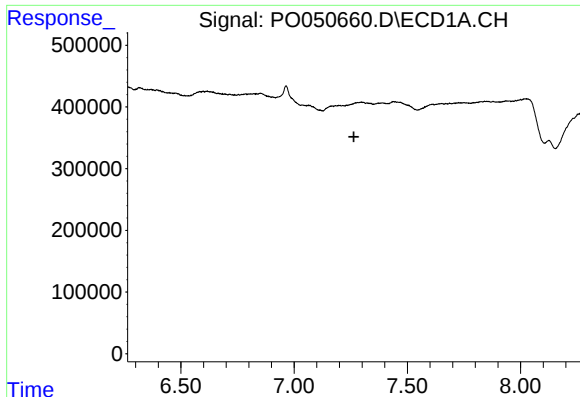

#29 AR-1254-4


R.T.: 0.000 min
Exp R.T. : 7.264 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

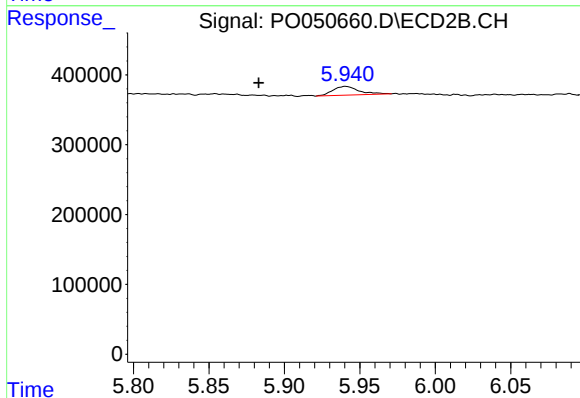


#29 AR-1254-4

R.T.: 5.940 min
Delta R.T.: 0.058 min
Response: 151995
Conc: 13.05 ng/ml

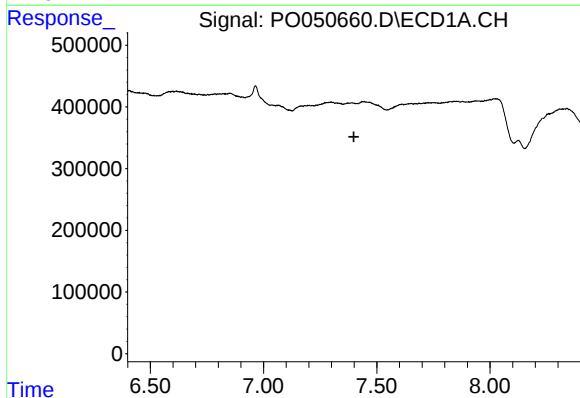


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 7.399 min
Response: 0
Conc: N.D.

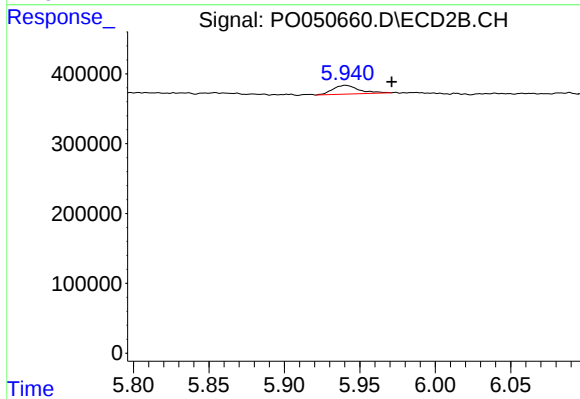

#32 AR-1260-2


R.T.: 5.940 min
Delta R.T.: -0.031 min
Response: 151995
Conc: 8.22 ng/ml

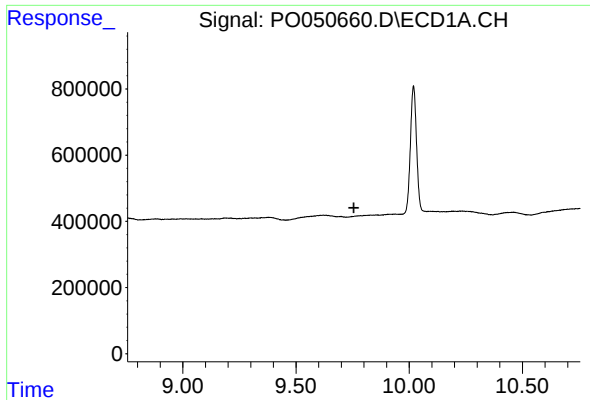

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T.: 9.756 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

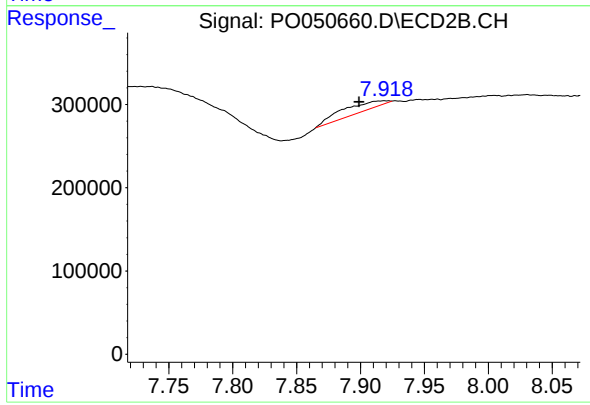

#45 AR-1268-5

R.T.: 7.919 min
Delta R.T.: 0.020 min
Response: 245250
Conc: 3.24 ng/ml