

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0102618\
 Data File : P0050610.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 26 Oct 2018 18:11
 Operator : SM/SJ
 Sample : J5650-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 102218-SIDI-E-U-M

Manual Integrations
 APPROVED

Sohil
 10/30/2018 9:33:08 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 26 22:55:22 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101818.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Oct 19 02:02:26 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.359	3.352	5825610	3760575	19.523	19.128m
2) SA Decachlor...	10.021	8.100	4864410	4386471	22.418m	22.949

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102618\
Data File : PO050610.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 26 Oct 2018 18:11
Operator : SM/SJ
Sample : J5650-01
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
102218-SIDI-E-U-M


Manual Integrations
APPROVED

Sohil
10/30/2018 9:33:08 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 26 22:55:22 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101818.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Oct 19 02:02:26 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

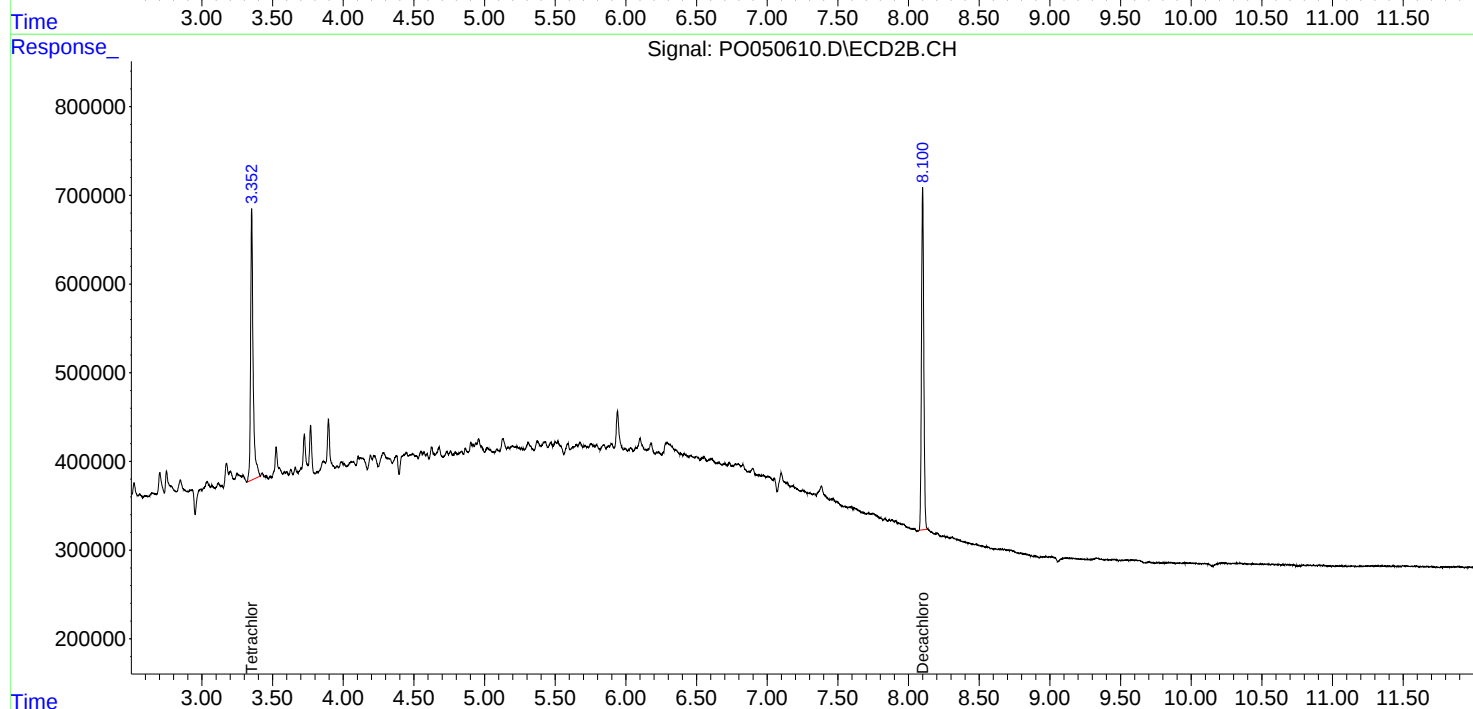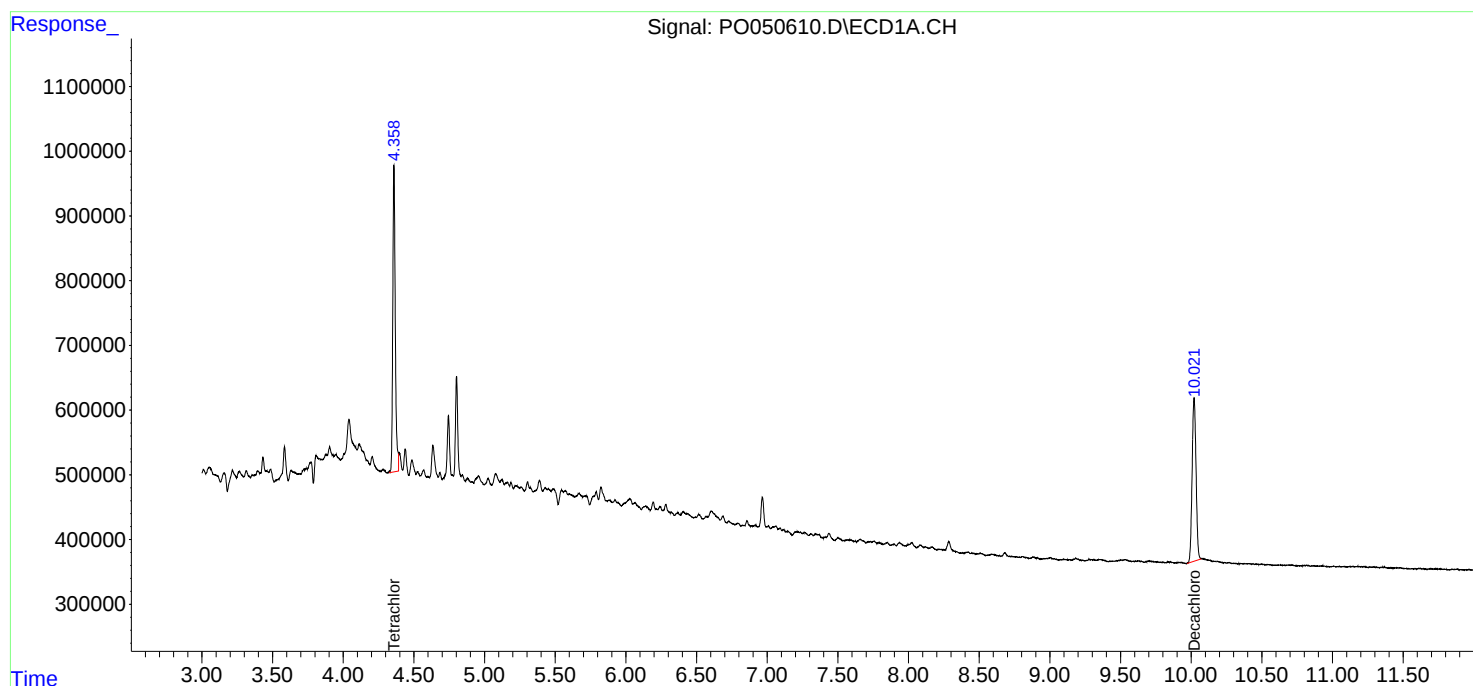

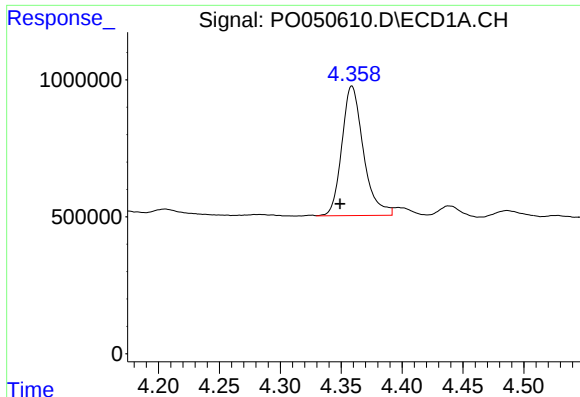


#1 Tetrachloro-m-xylene

R.T.: 4.359 min
Delta R.T.: 0.010 min
Response: 5825610
Conc: 19.52 ng/ml

Instrument :
ECD_O
ClientSampleId :
102218-SIDI-E-U-M


Manual Integrations
APPROVED

Sohil
10/30/2018 9:33:08 AM

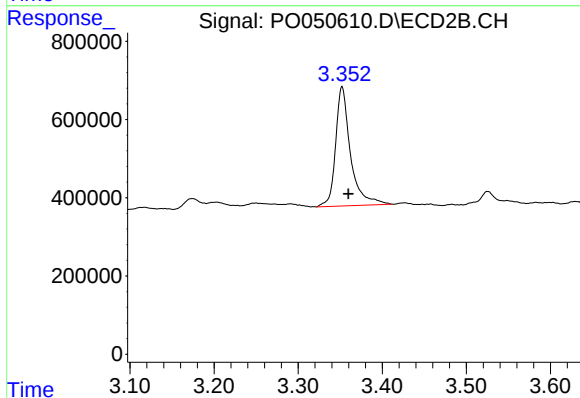


#1 Tetrachloro-m-xylene

R.T.: 3.352 min
Delta R.T.: -0.008 min
Response: 3760575
Conc: 19.13 ng/ml m

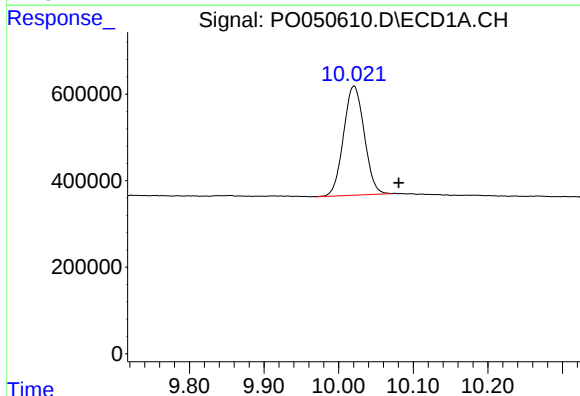

#2 Decachlorobiphenyl

R.T.: 10.021 min
Delta R.T.: -0.060 min
Response: 4864410
Conc: 22.42 ng/ml m

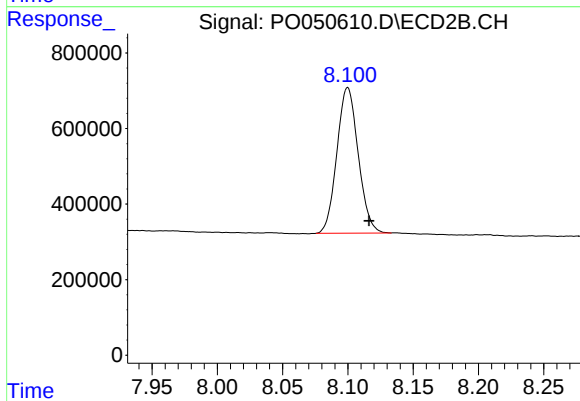

#2 Decachlorobiphenyl

R.T.: 8.100 min
Delta R.T.: -0.016 min
Response: 4386471
Conc: 22.95 ng/ml