

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0102618\
 Data File : P0050636.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 27 Oct 2018 1:49
 Operator : SM/SJ
 Sample : J5662-14
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 102318-TIPC-F-D-S

Manual Integrations
 APPROVED

Sohil
 10/30/2018 9:33:48 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 27 02:22:42 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101818.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Oct 19 02:02:26 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.356	3.350	6343795	3464365	21.260m	17.621m
2) SA Decachlor...	10.018	8.100	5203839	4613145	23.982	24.134

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102618\
Data File : PO050636.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 27 Oct 2018 1:49
Operator : SM/SJ
Sample : J5662-14
Misc :
ALS Vial : 37 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
102318-TIPC-F-D-S


Manual Integrations
APPROVED

Sohil
10/30/2018 9:33:48 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 27 02:22:42 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101818.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Oct 19 02:02:26 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

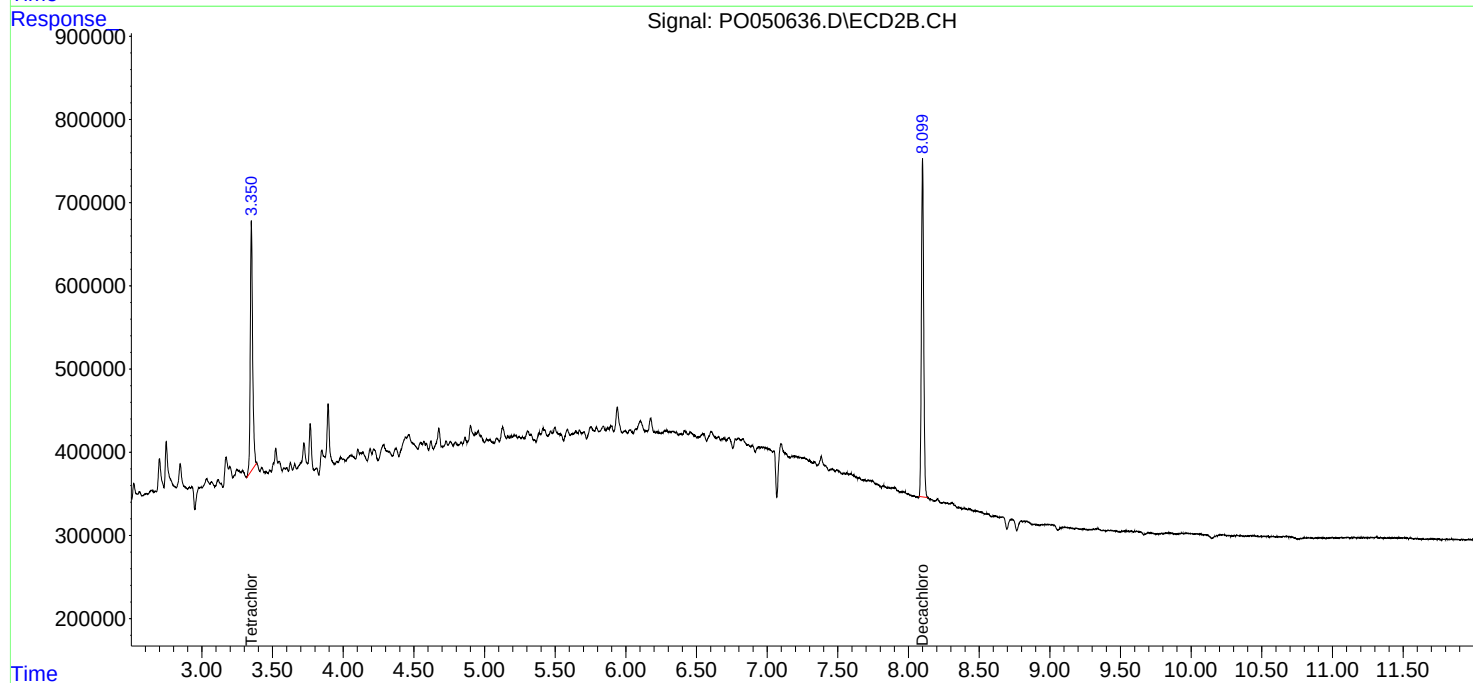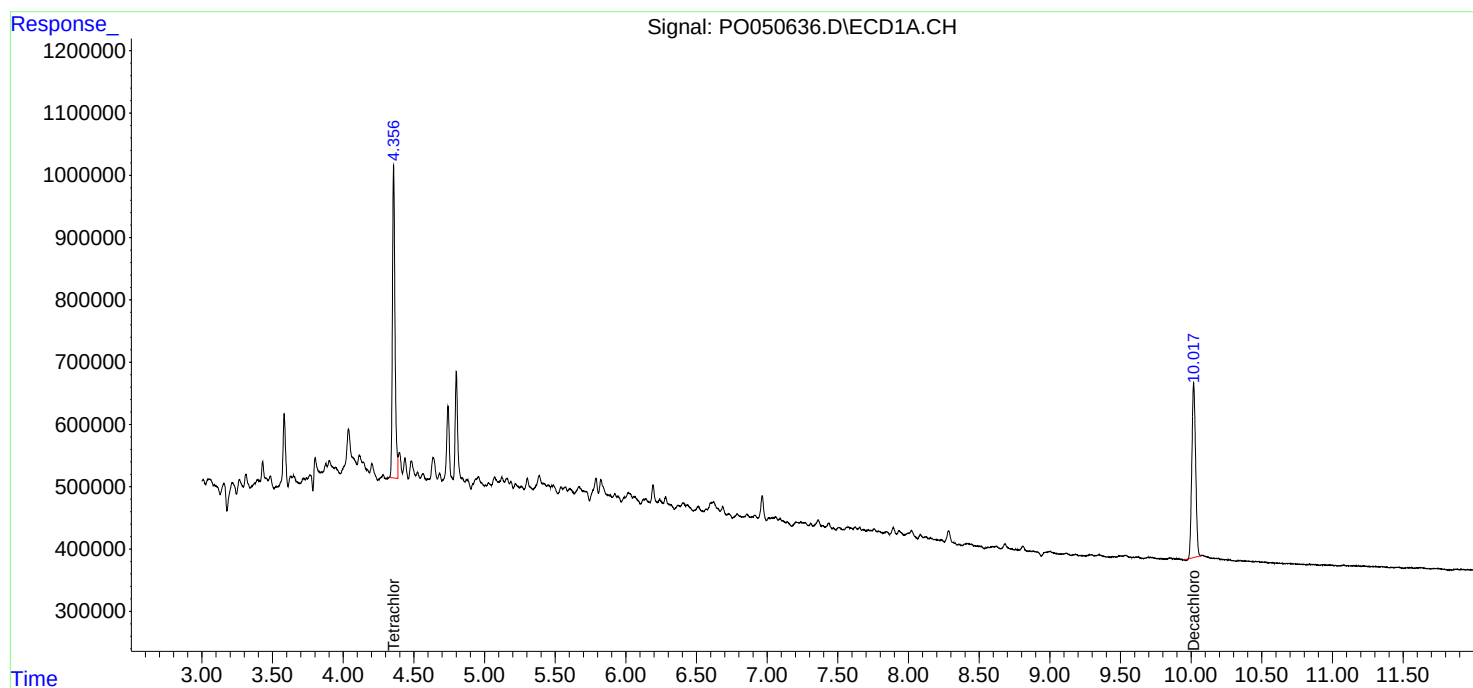

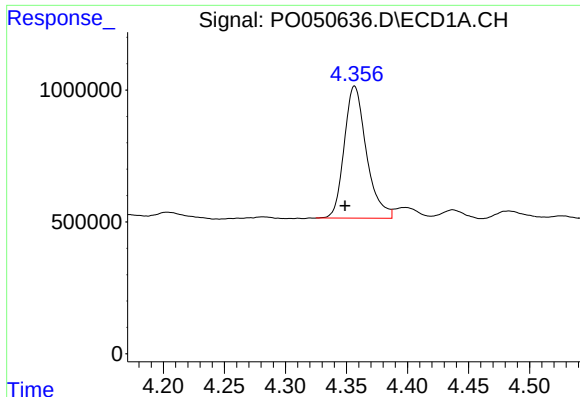


#1 Tetrachloro-m-xylene

R.T.: 4.356 min
Delta R.T.: 0.007 min
Response: 6343795
Conc: 21.26 ng/ml m

Instrument :
ECD_O
ClientSampleId :
102318-TIPC-F-D-S


Manual Integrations
APPROVED

Sohil
10/30/2018 9:33:48 AM

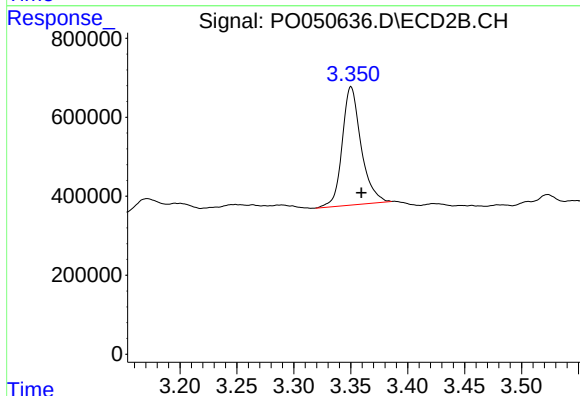


#1 Tetrachloro-m-xylene

R.T.: 3.350 min
Delta R.T.: -0.010 min
Response: 3464365
Conc: 17.62 ng/ml m

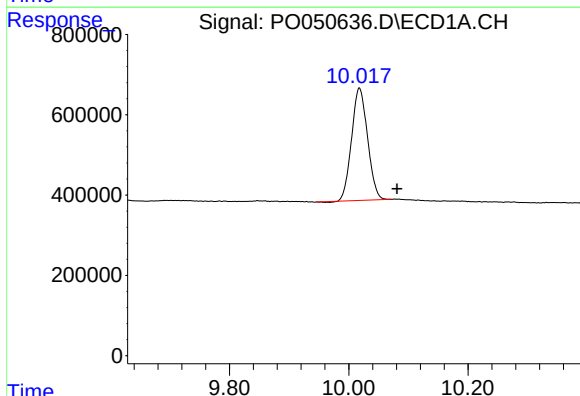

#2 Decachlorobiphenyl

R.T.: 10.018 min
Delta R.T.: -0.063 min
Response: 5203839
Conc: 23.98 ng/ml

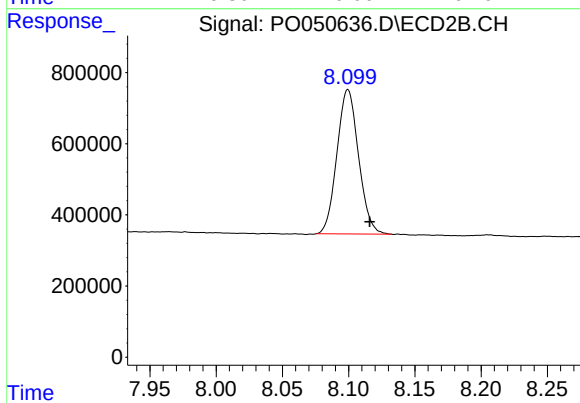

#2 Decachlorobiphenyl

R.T.: 8.100 min
Delta R.T.: -0.017 min
Response: 4613145
Conc: 24.13 ng/ml