

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102620\
 Data File : PO072779.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 26 Oct 2020 20:53
 Operator : DD\AJ
 Sample : AR1248ICC250
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1248ICC250

Manual Integrations
 APPROVED

Ankita
 10/27/2020 10:00:22 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 27 03:46:06 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102620.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Oct 27 03:44:22 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.949	4.021	1174079	950420	24.826	26.138
2) SA Decachlor...	10.984	9.313	1040953	1037741	26.211	28.049
Target Compounds						
21) L5 AR-1248-1	6.273	5.275	268188	253170	258.946	282.513
22) L5 AR-1248-2	6.568	5.539	337046	327947	256.162m	273.709
23) L5 AR-1248-3	6.787	5.583	383097	335586	252.780	270.472
24) L5 AR-1248-4	7.217	5.767	458206	399936	258.911	272.788
25) L5 AR-1248-5	7.257	6.188	436002	416489	255.767	278.703

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102620\
Data File : PO072779.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 26 Oct 2020 20:53
Operator : DD\AJ
Sample : AR1248ICC250
Misc :
ALS Vial : 18 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
AR1248ICC250


Manual Integrations
APPROVED

Ankita
10/27/2020 10:00:22 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 27 03:46:06 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102620.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Oct 27 03:44:22 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

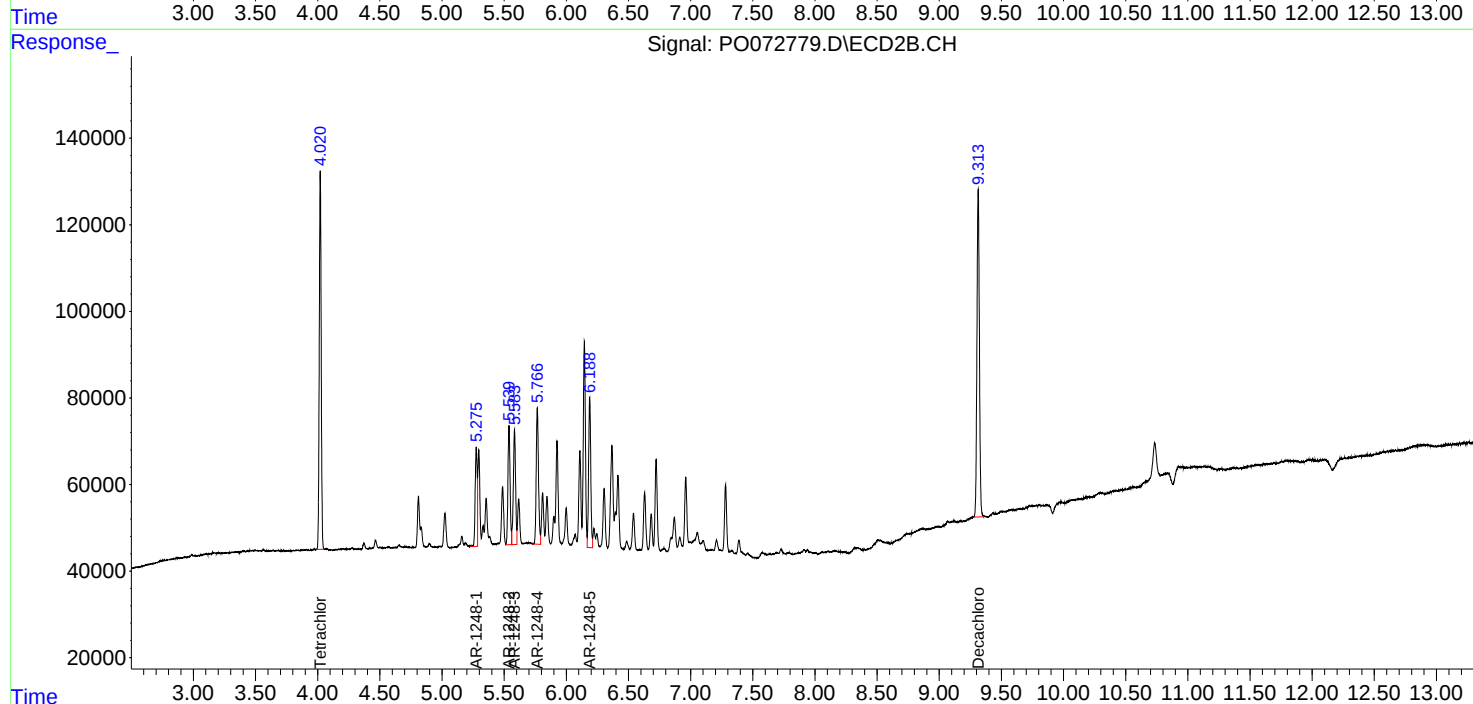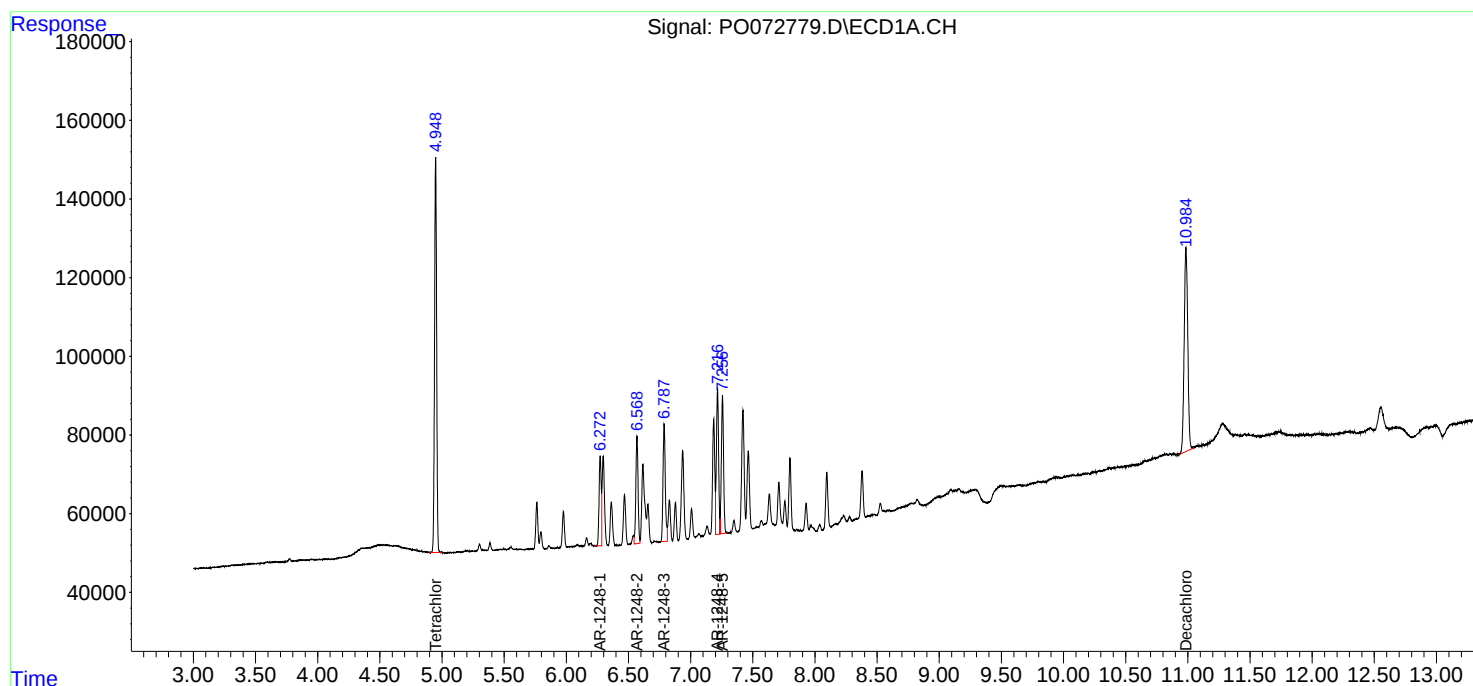

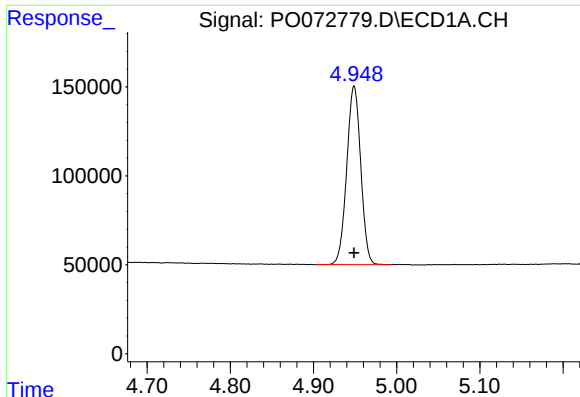


#1 Tetrachloro-m-xylene

R.T.: 4.949 min
Delta R.T.: 0.000 min
Response: 1174079
Conc: 24.83 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1248ICC250


Manual Integrations
APPROVED

Ankita
10/27/2020 10:00:22 AM

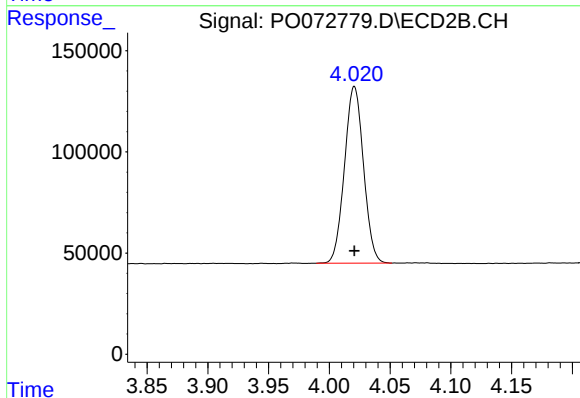


#1 Tetrachloro-m-xylene

R.T.: 4.021 min
Delta R.T.: 0.000 min
Response: 950420
Conc: 26.14 ng/ml

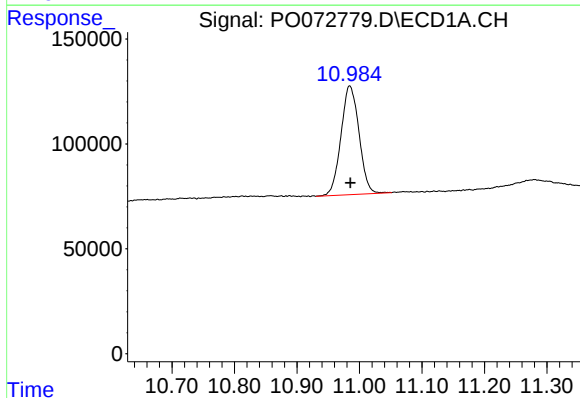


#2 Decachlorobiphenyl

R.T.: 10.984 min
Delta R.T.: -0.001 min
Response: 1040953
Conc: 26.21 ng/ml

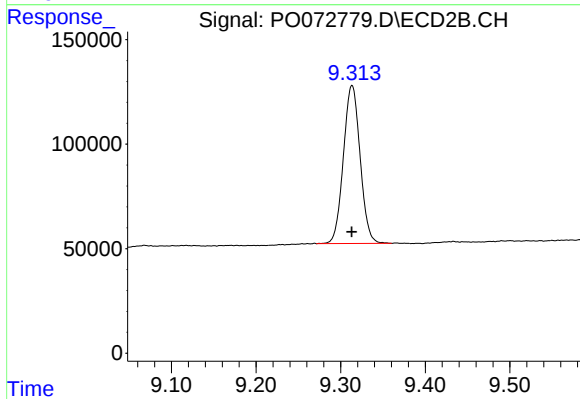

#2 Decachlorobiphenyl

R.T.: 9.313 min
Delta R.T.: 0.000 min
Response: 1037741
Conc: 28.05 ng/ml

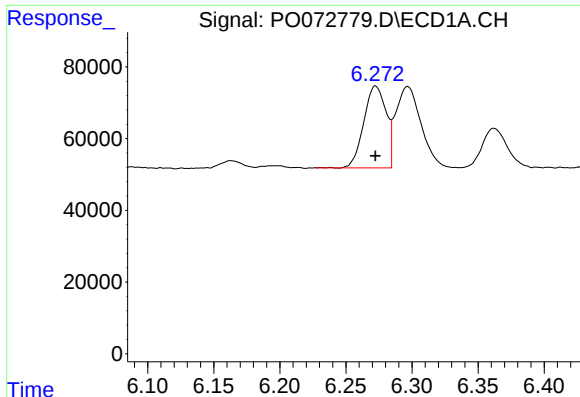


#21 AR-1248-1

R.T.: 6.273 min
Delta R.T.: 0.000 min
Response: 268188
Conc: 258.95 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1248ICC250


Manual Integrations
APPROVED

Ankita
10/27/2020 10:00:22 AM

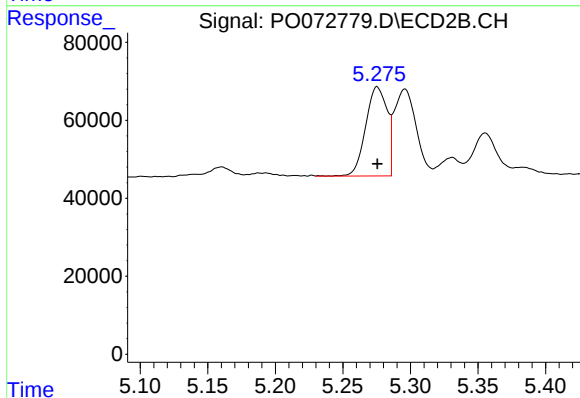


#21 AR-1248-1

R.T.: 5.275 min
Delta R.T.: 0.000 min
Response: 253170
Conc: 282.51 ng/ml

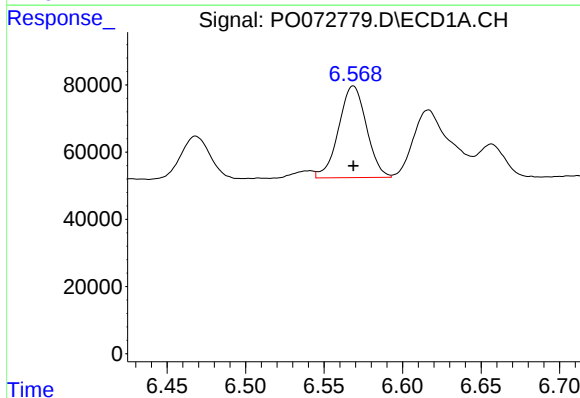


#22 AR-1248-2

R.T.: 6.568 min
Delta R.T.: 0.000 min
Response: 337046
Conc: 256.16 ng/ml m

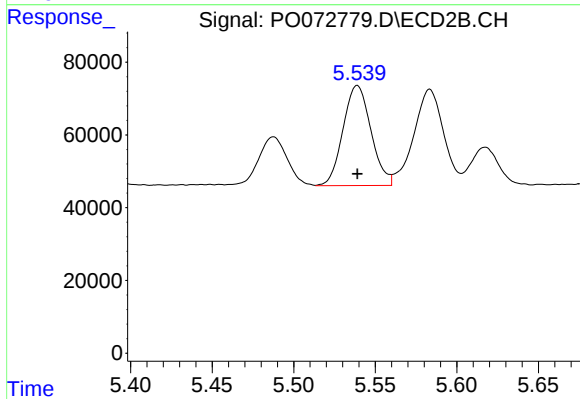

#22 AR-1248-2

R.T.: 5.539 min
Delta R.T.: 0.000 min
Response: 327947
Conc: 273.71 ng/ml

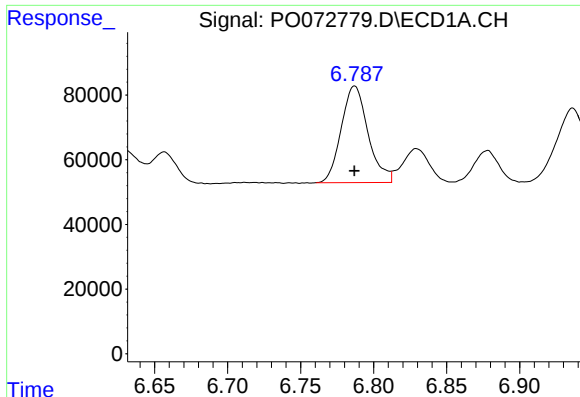


#23 AR-1248-3

R.T.: 6.787 min
Delta R.T.: 0.000 min
Response: 383097
Conc: 252.78 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1248ICC250


Manual Integrations
APPROVED

Ankita
10/27/2020 10:00:22 AM

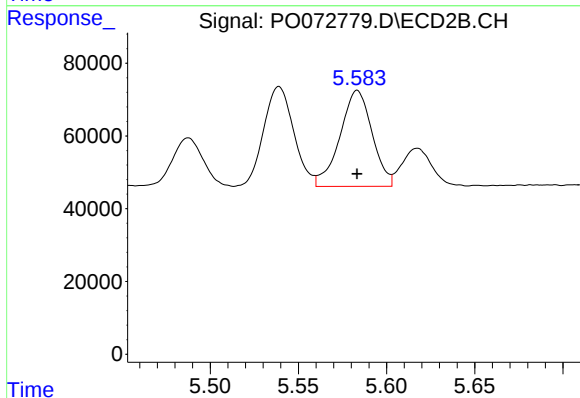


#23 AR-1248-3

R.T.: 5.583 min
Delta R.T.: 0.000 min
Response: 335586
Conc: 270.47 ng/ml

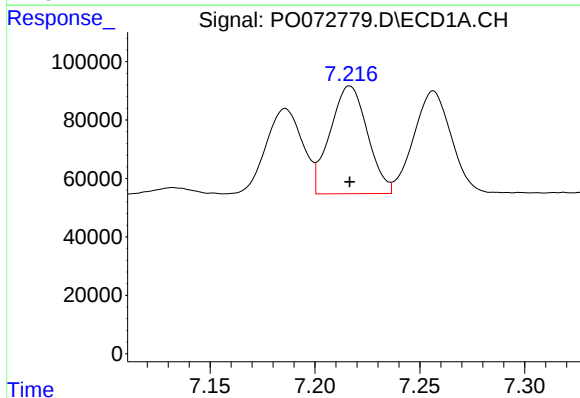


#24 AR-1248-4

R.T.: 7.217 min
Delta R.T.: 0.000 min
Response: 458206
Conc: 258.91 ng/ml

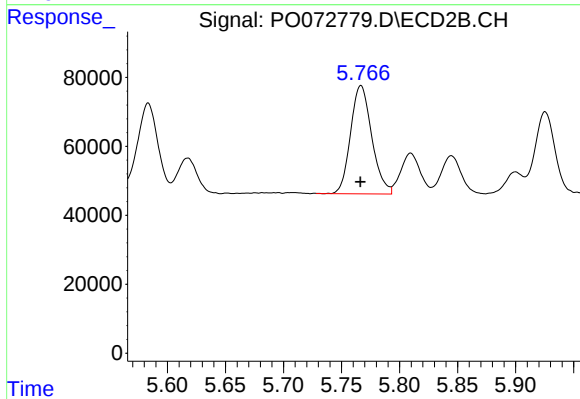

#24 AR-1248-4

R.T.: 5.767 min
Delta R.T.: 0.000 min
Response: 399936
Conc: 272.79 ng/ml

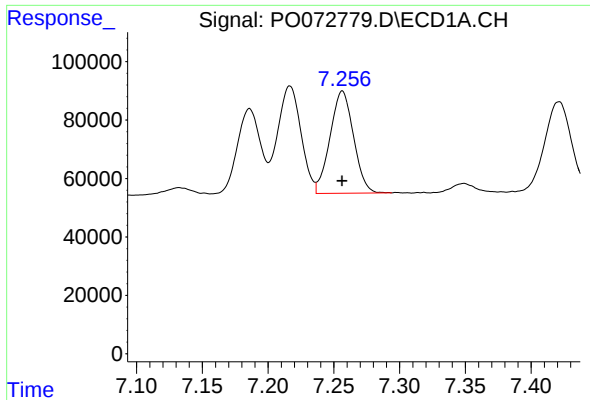


#25 AR-1248-5

R.T.: 7.257 min
Delta R.T.: 0.000 min
Response: 436002
Conc: 255.77 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1248ICC250

Manual Integrations
APPROVED

Ankita
10/27/2020 10:00:22 AM

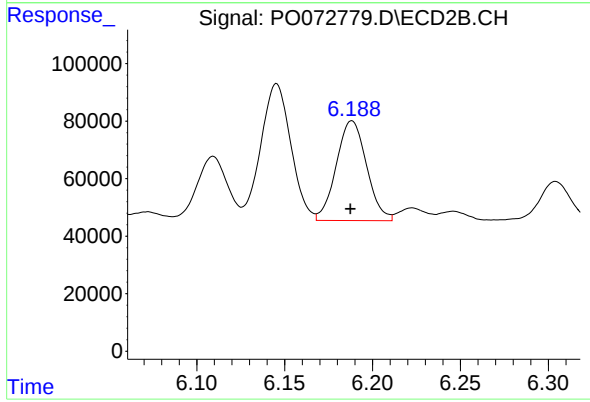

#25 AR-1248-5

R.T.: 6.188 min
Delta R.T.: 0.000 min
Response: 416489
Conc: 278.70 ng/ml