

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102621\
 Data File : PO082181.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 26 Oct 2021 17:36
 Operator : AJ\MA
 Sample : M4340-01
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TH-ES

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 27 02:31:23 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Oct 19 04:37:47 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.981	3.974	2123018	770398	26.274	26.111
2)	SA Decachlor...	11.105	9.303	1313915	587173	23.640	23.053

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102621\
Data File : PO082181.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 26 Oct 2021 17:36
Operator : AJ\MA
Sample : M4340-01
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TH-ES

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 27 02:31:23 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101821.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Oct 19 04:37:47 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

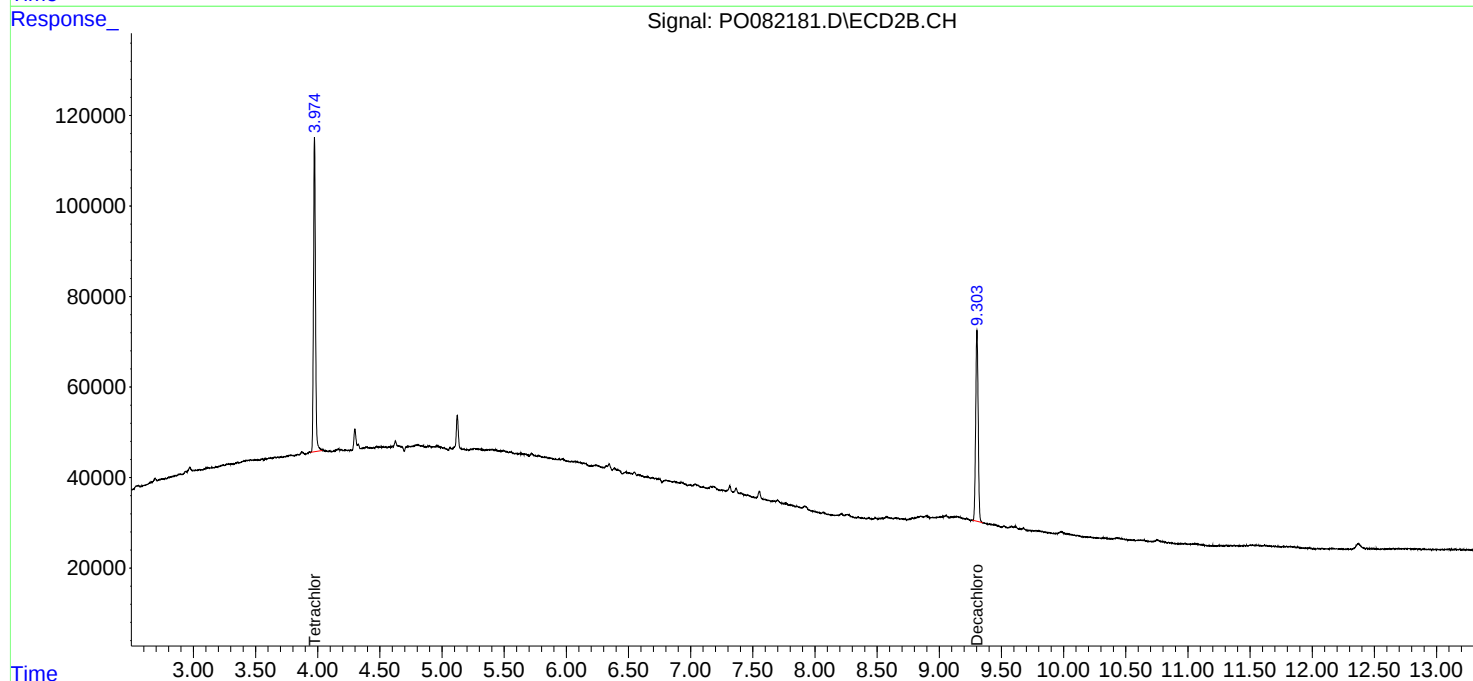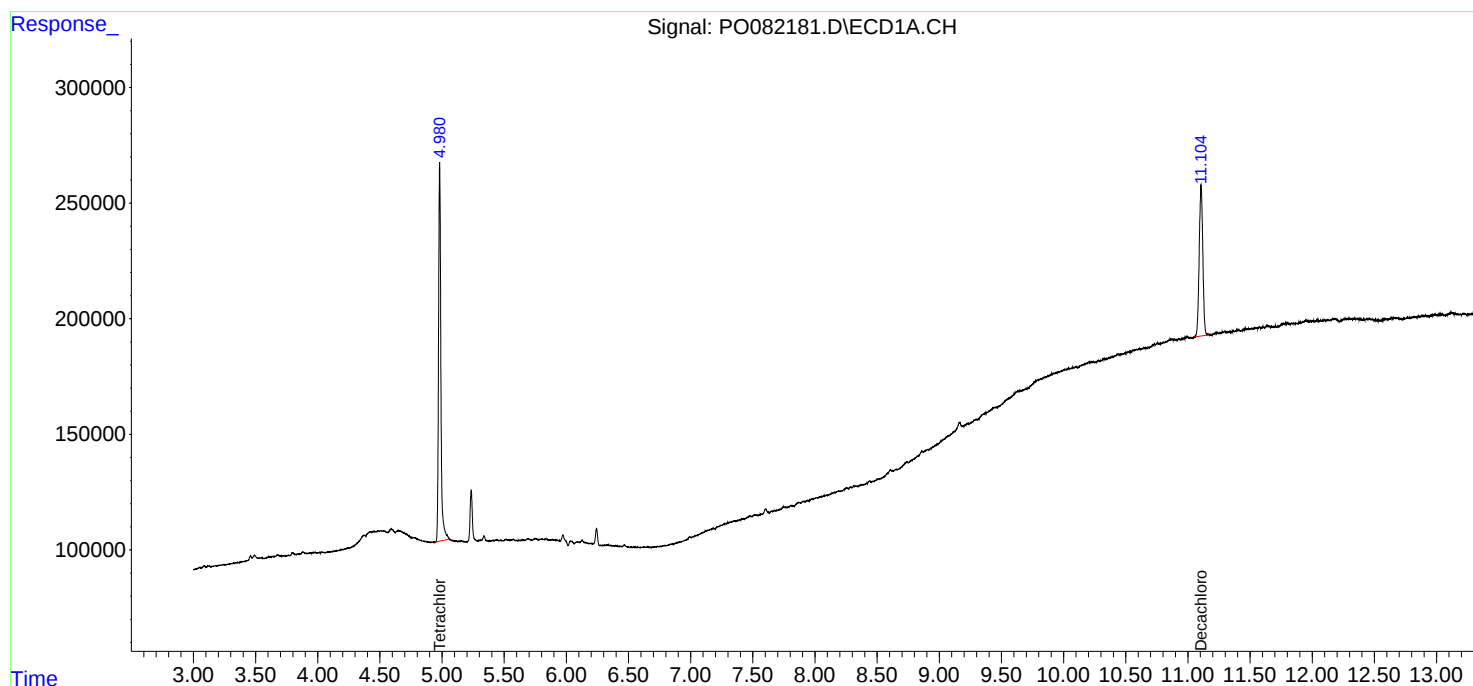


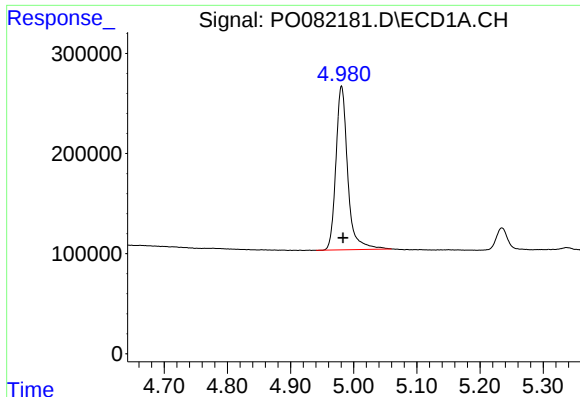

#1 Tetrachloro-m-xylene


R.T.: 4.981 min
Delta R.T.: -0.002 min
Response: 2123018
Conc: 26.27 ng/ml

Instrument :
ECD_O
ClientSampleId :
TH-ES

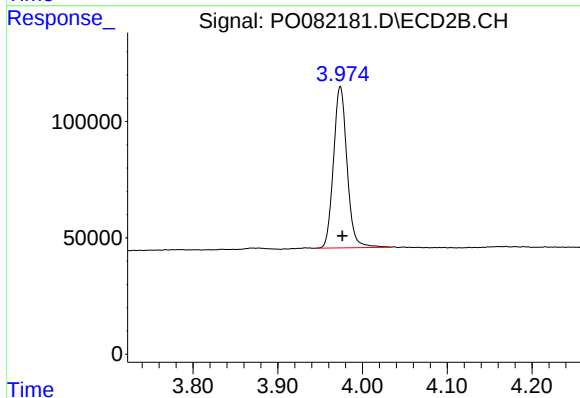


#1 Tetrachloro-m-xylene

R.T.: 3.974 min
Delta R.T.: -0.003 min
Response: 770398
Conc: 26.11 ng/ml

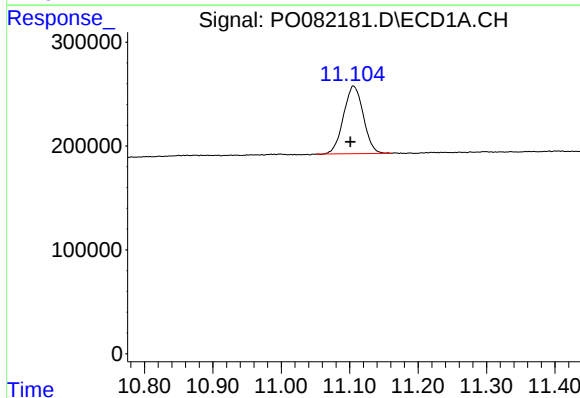

#2 Decachlorobiphenyl

R.T.: 11.105 min
Delta R.T.: 0.004 min
Response: 1313915
Conc: 23.64 ng/ml

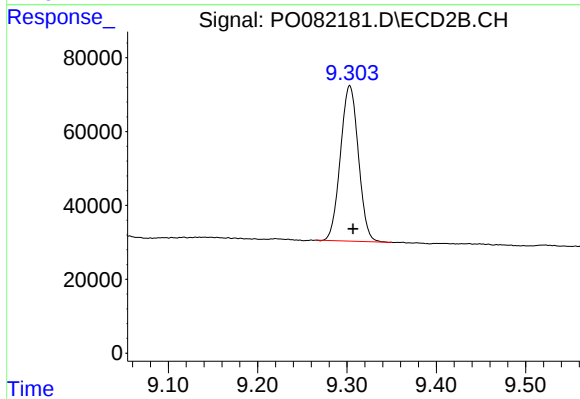

#2 Decachlorobiphenyl

R.T.: 9.303 min
Delta R.T.: -0.004 min
Response: 587173
Conc: 23.05 ng/ml