

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102621\
 Data File : PO082188.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 26 Oct 2021 19:36
 Operator : AJ\MA
 Sample : M4350-01
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CONCRETE-GRAB

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 27 02:33:00 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Oct 19 04:37:47 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.980	3.973	1615092	598415	19.988	20.282
2) SA Decachlor...	11.104	9.302	1092973	521546	19.665	20.477

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102621\
Data File : P0082188.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 26 Oct 2021 19:36
Operator : AJ\MA
Sample : M4350-01
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
CONCRETE-GRAB

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 27 02:33:00 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101821.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Oct 19 04:37:47 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

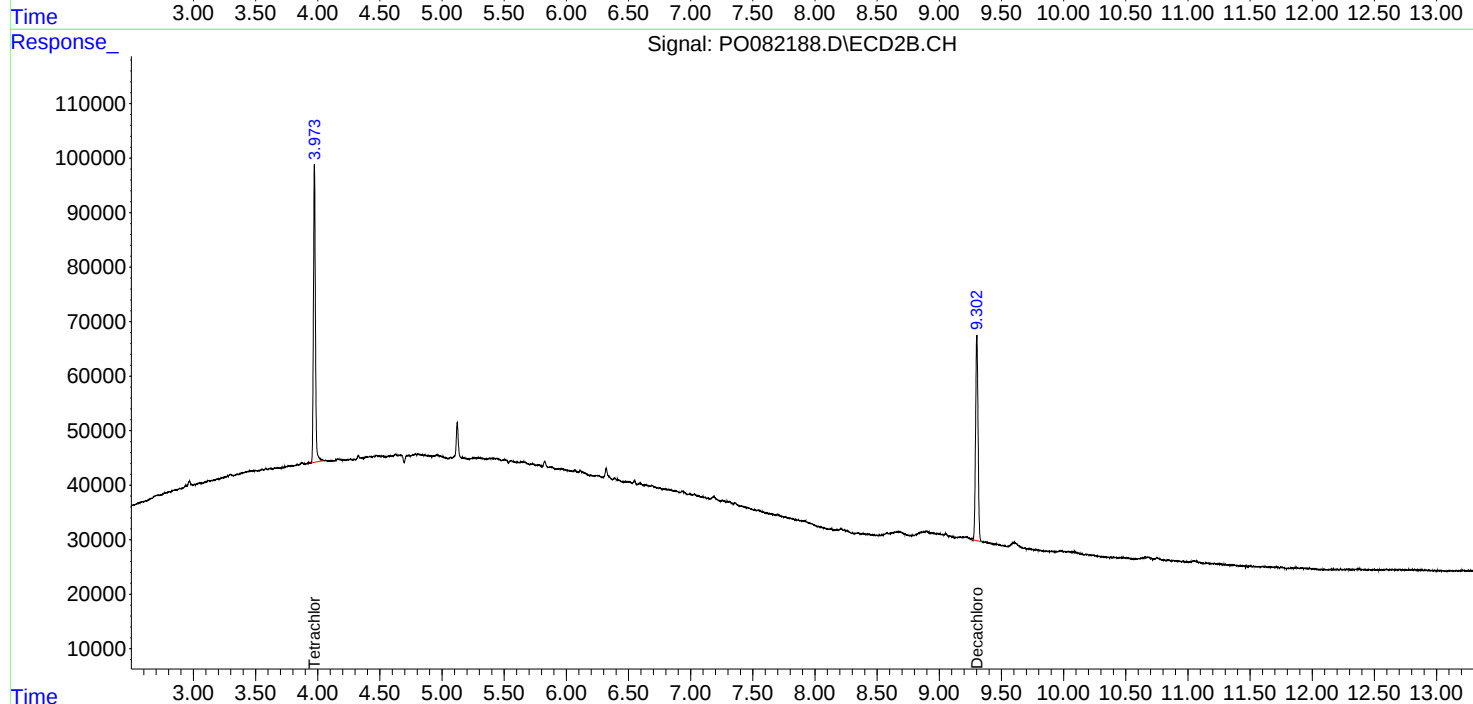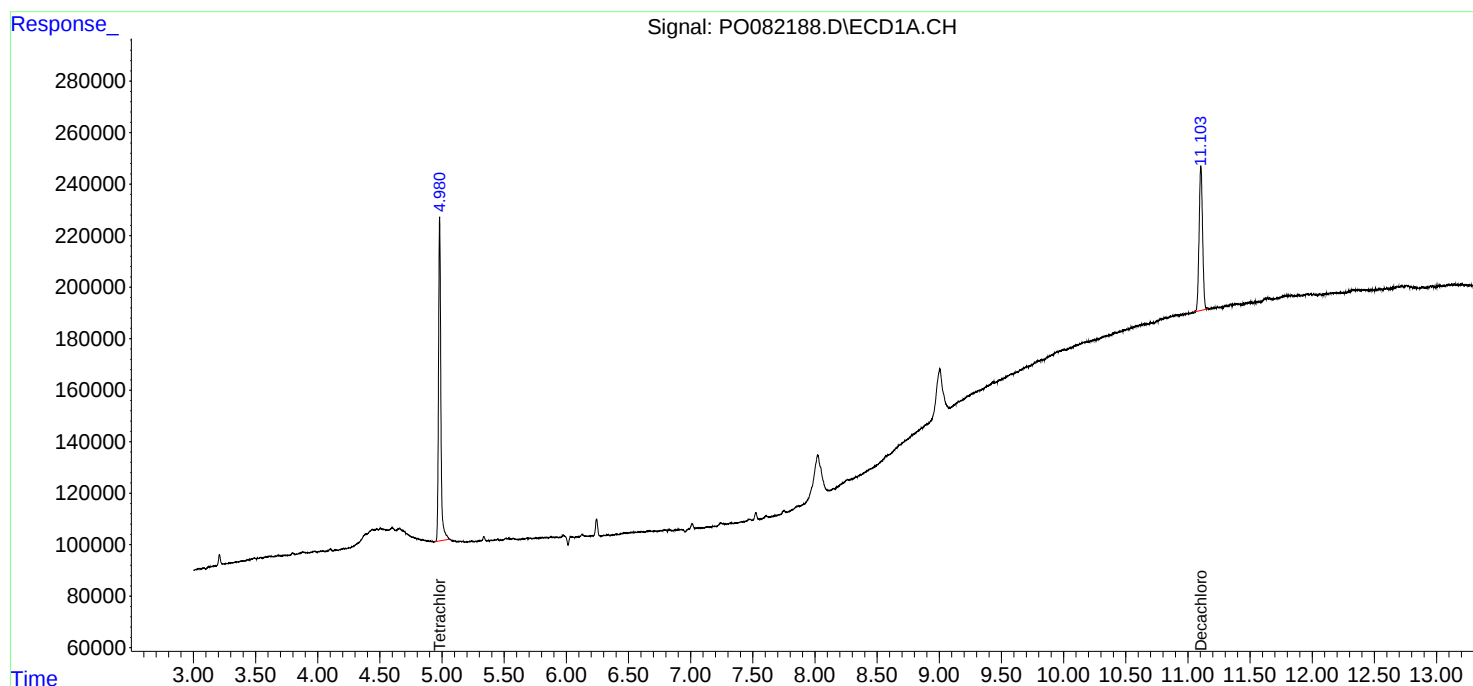


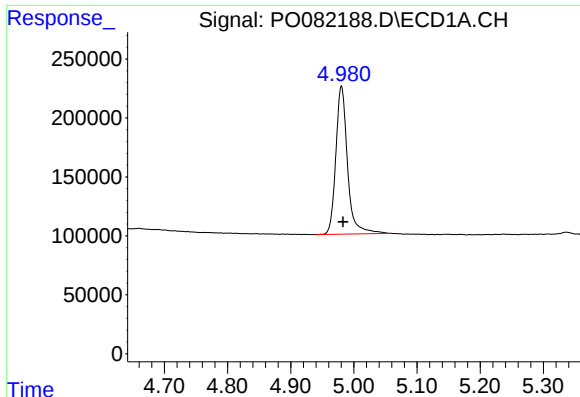

#1 Tetrachloro-m-xylene


R.T.: 4.980 min
Delta R.T.: -0.003 min
Response: 1615092
Conc: 19.99 ng/ml

Instrument :
ECD_O
ClientSampleId :
CONCRETE-GRAB

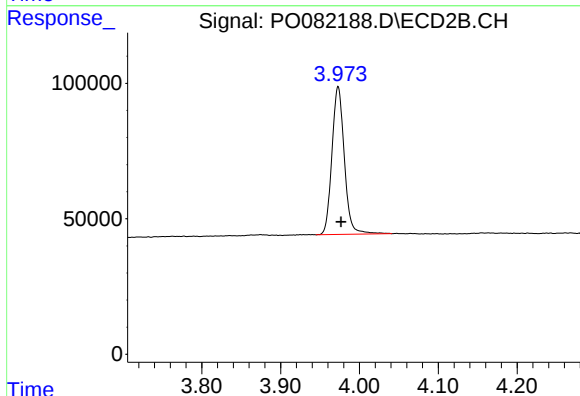


#1 Tetrachloro-m-xylene

R.T.: 3.973 min
Delta R.T.: -0.003 min
Response: 598415
Conc: 20.28 ng/ml

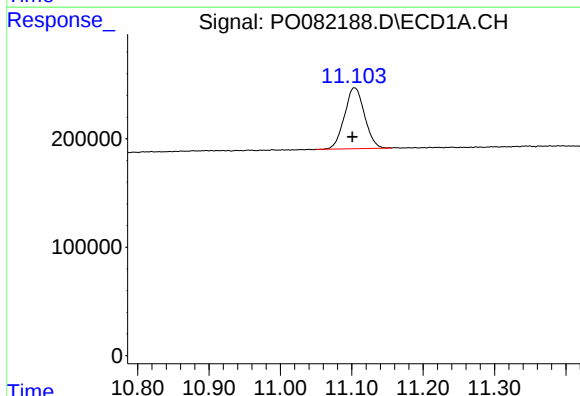

#2 Decachlorobiphenyl

R.T.: 11.104 min
Delta R.T.: 0.003 min
Response: 1092973
Conc: 19.67 ng/ml

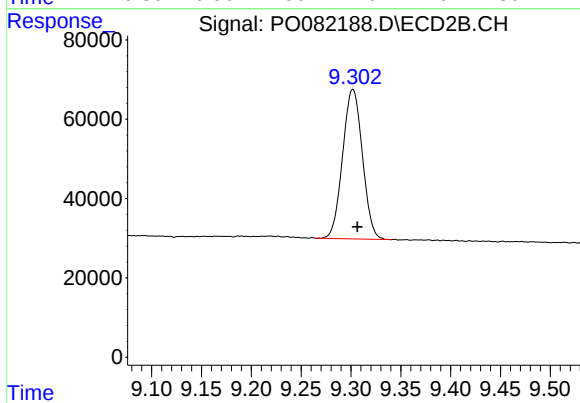

#2 Decachlorobiphenyl

R.T.: 9.302 min
Delta R.T.: -0.005 min
Response: 521546
Conc: 20.48 ng/ml