

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0102621\
 Data File : P0082199.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 26 Oct 2021 23:03
 Operator : AJ\MA
 Sample : M4358-10
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TH-GD

Manual Integrations
 APPROVED

mohammad
 10/27/2021 2:35:46 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 27 02:35:31 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Oct 19 04:37:47 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.979	3.973	2050412	748019	25.375m	25.353
2) SA Decachlor...	11.102	9.300	1367388	538066	24.603	21.125

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102621\
Data File : PO082199.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 26 Oct 2021 23:03
Operator : AJ\MA
Sample : M4358-10
Misc :
ALS Vial : 31 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
TH-GD


Manual Integrations
APPROVED

mohammad
10/27/2021 2:35:46 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 27 02:35:31 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101821.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Oct 19 04:37:47 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

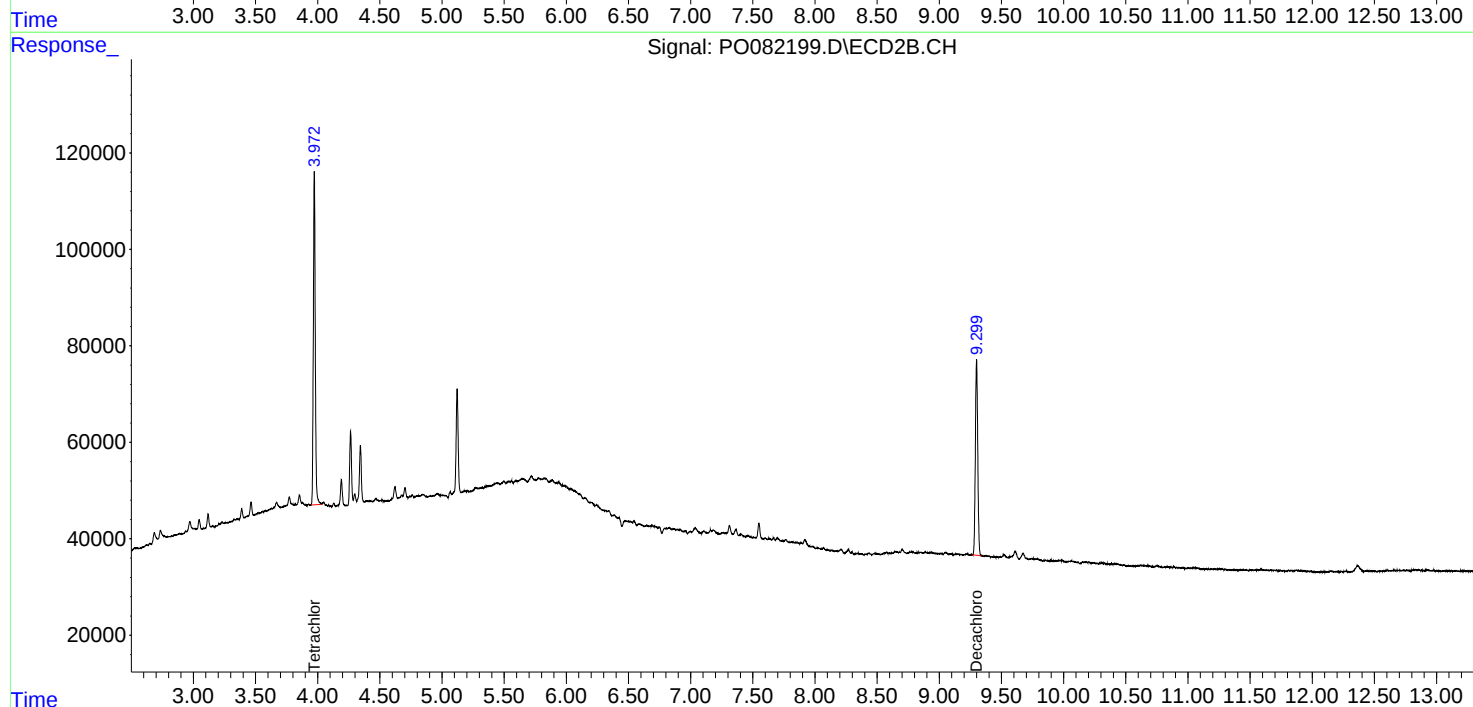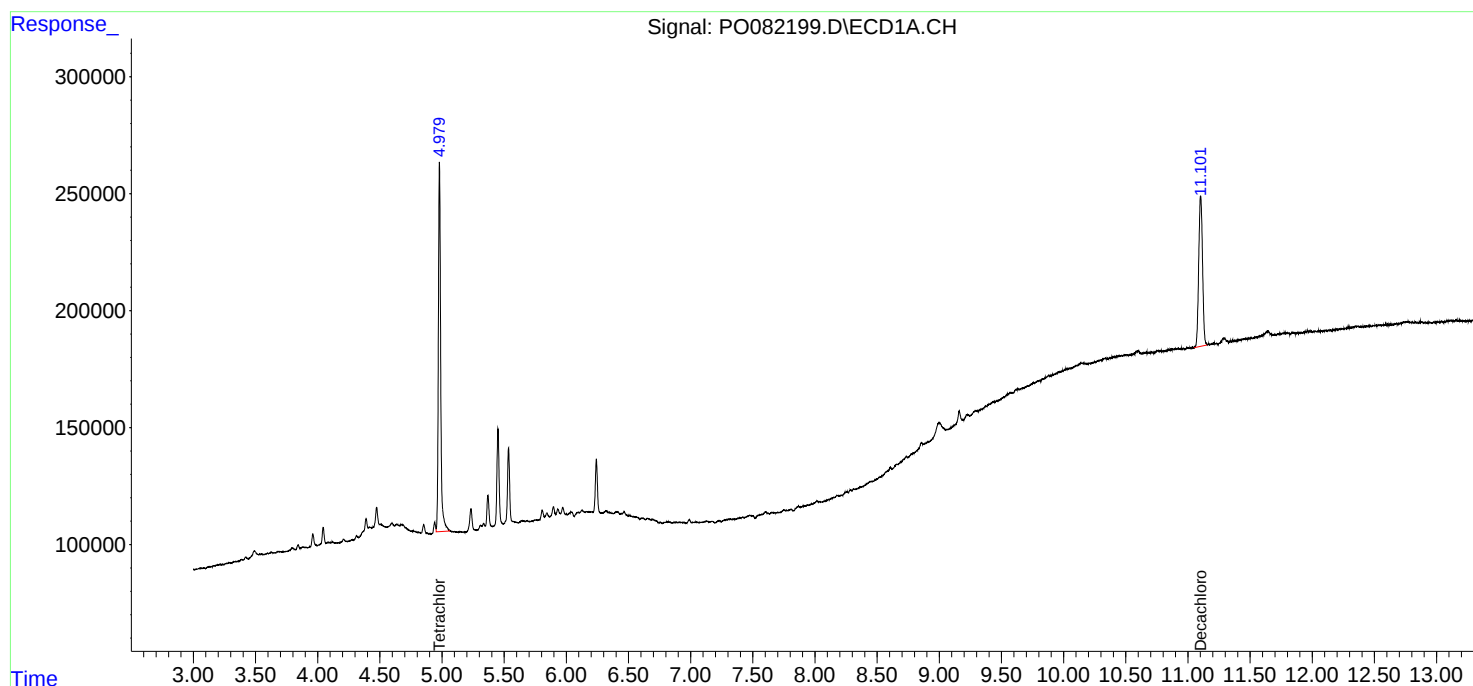

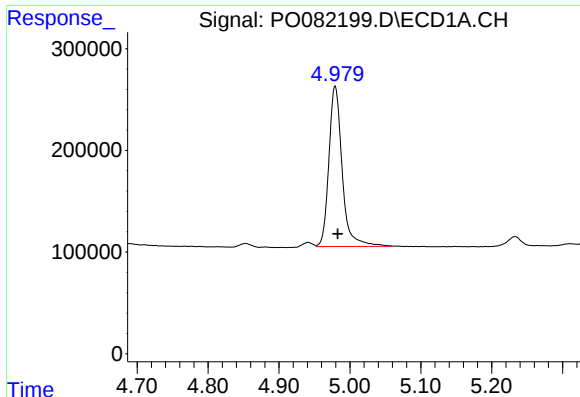


#1 Tetrachloro-m-xylene

R.T.: 4.979 min
Delta R.T.: -0.004 min
Response: 2050412
Conc: 25.38 ng/ml m

Instrument :
ECD_O
ClientSampleId :
TH-GD


Manual Integrations
APPROVED

mohammad
10/27/2021 2:35:46 PM

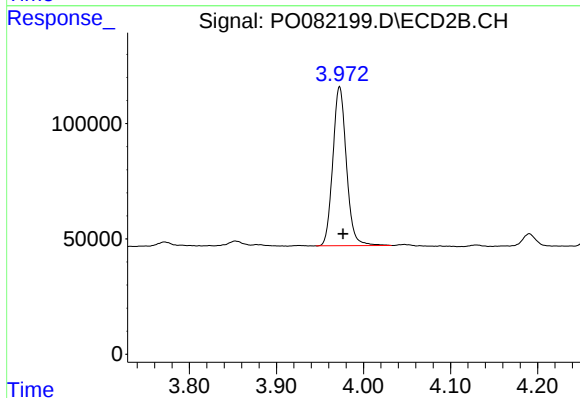


#1 Tetrachloro-m-xylene

R.T.: 3.973 min
Delta R.T.: -0.004 min
Response: 748019
Conc: 25.35 ng/ml

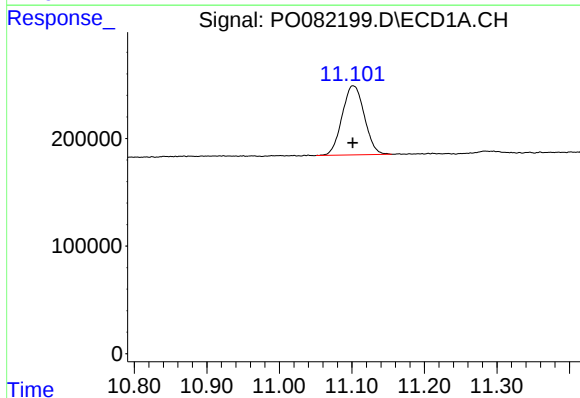

#2 Decachlorobiphenyl

R.T.: 11.102 min
Delta R.T.: 0.000 min
Response: 1367388
Conc: 24.60 ng/ml

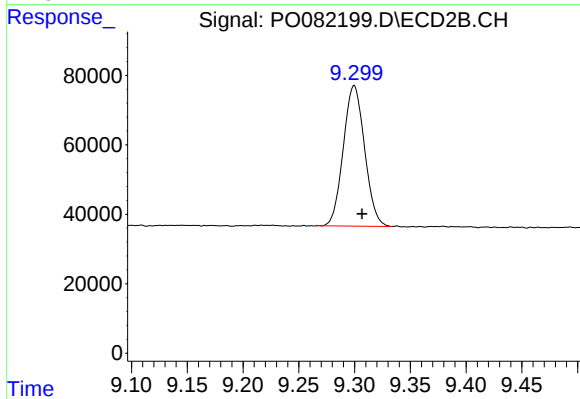

#2 Decachlorobiphenyl

R.T.: 9.300 min
Delta R.T.: -0.007 min
Response: 538066
Conc: 21.13 ng/ml