

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102621\
 Data File : PO082210.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 27 Oct 2021 2:31
 Operator : AJ\MA
 Sample : M4336-01
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MW-7

Manual Integrations
 APPROVED

mohammad
 10/27/2021 2:35:54 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 27 05:18:41 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Oct 19 04:37:47 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.982	3.975	1082627	448145	13.398	15.189
2) SA Decachlor...	11.105	9.299	334798	230823	6.024m	9.063m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\PO102621\
Data File : P0082210.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 27 Oct 2021 2:31
Operator : AJ\MA
Sample : M4336-01
Misc :
ALS Vial : 37 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
MW-7


Manual Integrations
APPROVED

mohammad
10/27/2021 2:35:54 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 27 05:18:41 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\PO101821.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Oct 19 04:37:47 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

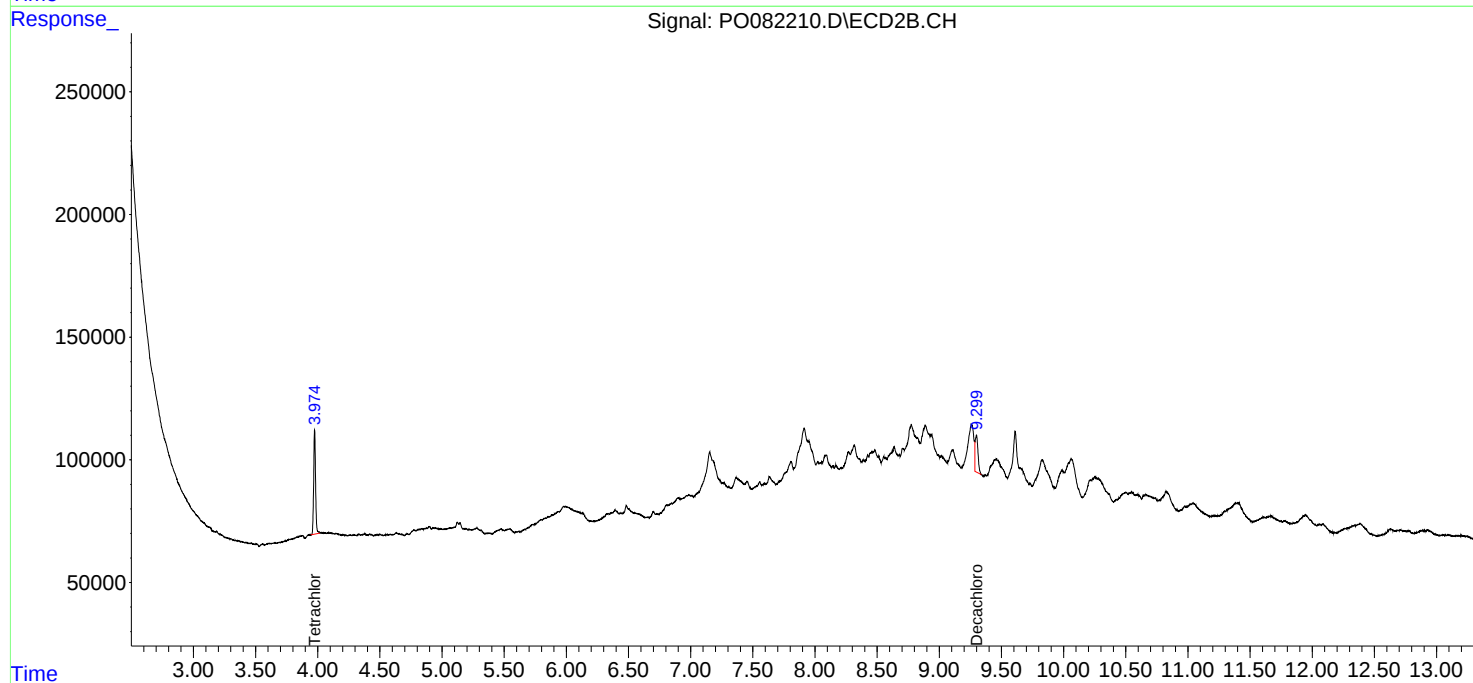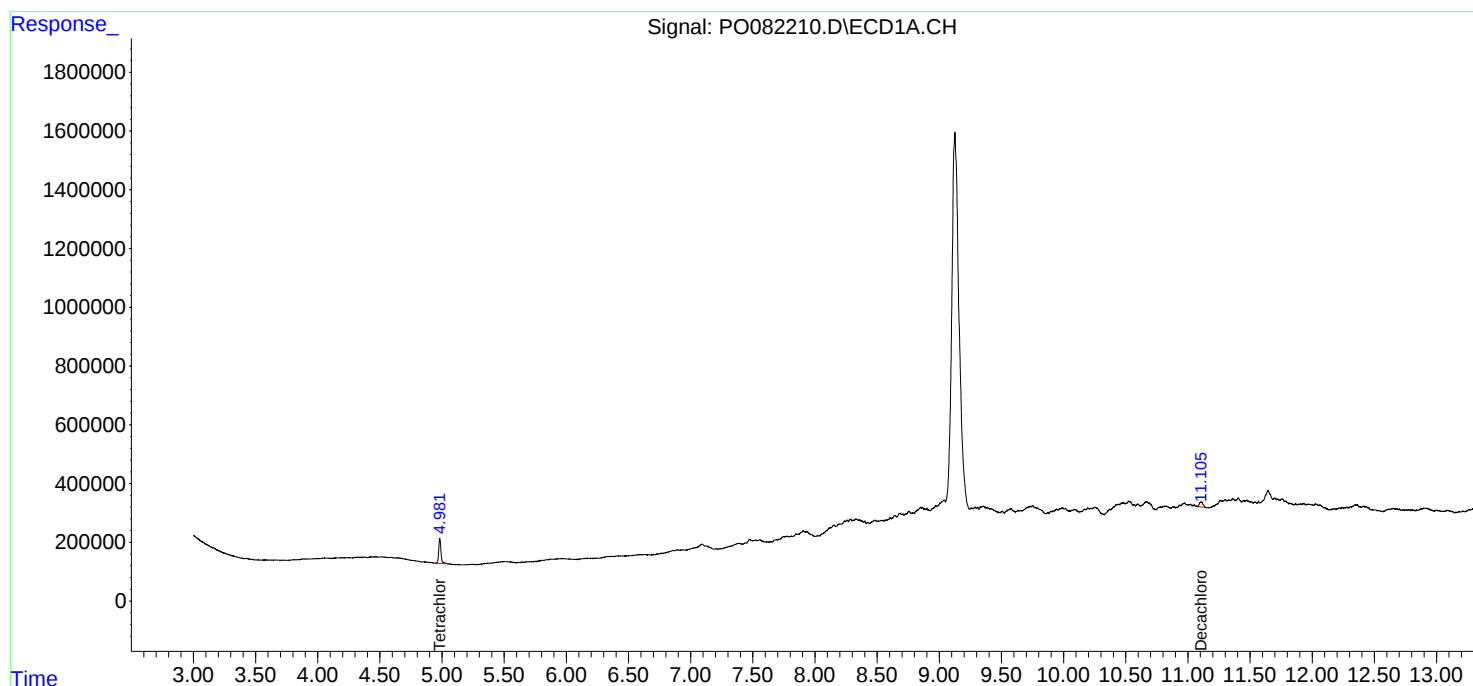

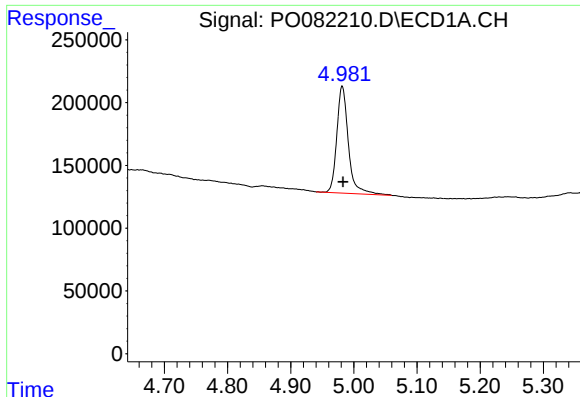


#1 Tetrachloro-m-xylene

R.T.: 4.982 min
Delta R.T.: -0.001 min
Response: 1082627
Conc: 13.40 ng/ml

Instrument :
ECD_O
ClientSampleId :
MW-7


Manual Integrations
APPROVED

mohammad
10/27/2021 2:35:54 PM

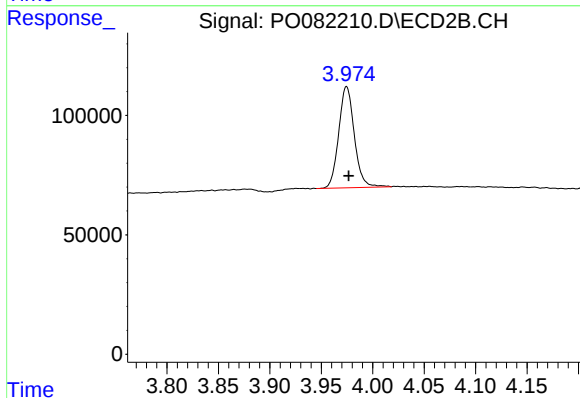


#1 Tetrachloro-m-xylene

R.T.: 3.975 min
Delta R.T.: -0.002 min
Response: 448145
Conc: 15.19 ng/ml

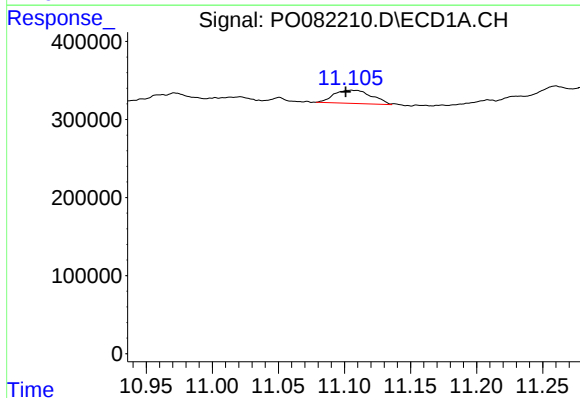

#2 Decachlorobiphenyl

R.T.: 11.105 min
Delta R.T.: 0.004 min
Response: 334798
Conc: 6.02 ng/ml m

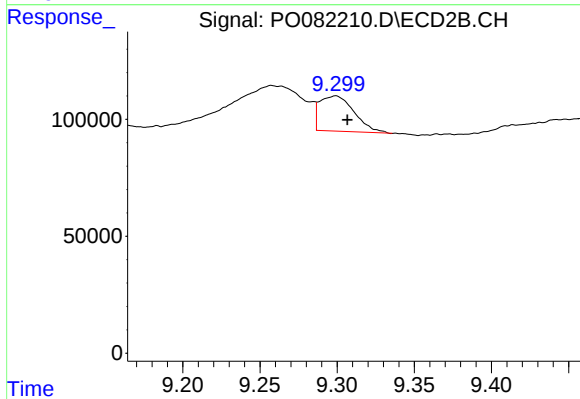

#2 Decachlorobiphenyl

R.T.: 9.299 min
Delta R.T.: -0.008 min
Response: 230823
Conc: 9.06 ng/ml m