

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102623\
 Data File : PO098962.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Oct 2023 10:04
 Operator : YP/AJ
 Sample : 04991-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 1021-1024

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/27/2023
 Supervised By :Ankita Jodhani 10/27/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 26 15:12:43 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102523.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 25 06:04:36 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.475	3.629	11318285	5236832	5.728m	7.277 #
2) SA Decachlor...	10.282	8.628	8462615	3671621	7.470	6.843m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102623\
Data File : PO098962.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Oct 2023 10:04
Operator : YP/AJ
Sample : 04991-01
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
1021-1024


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/27/2023
Supervised By :Ankita Jodhani 10/27/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 26 15:12:43 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102523.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 25 06:04:36 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

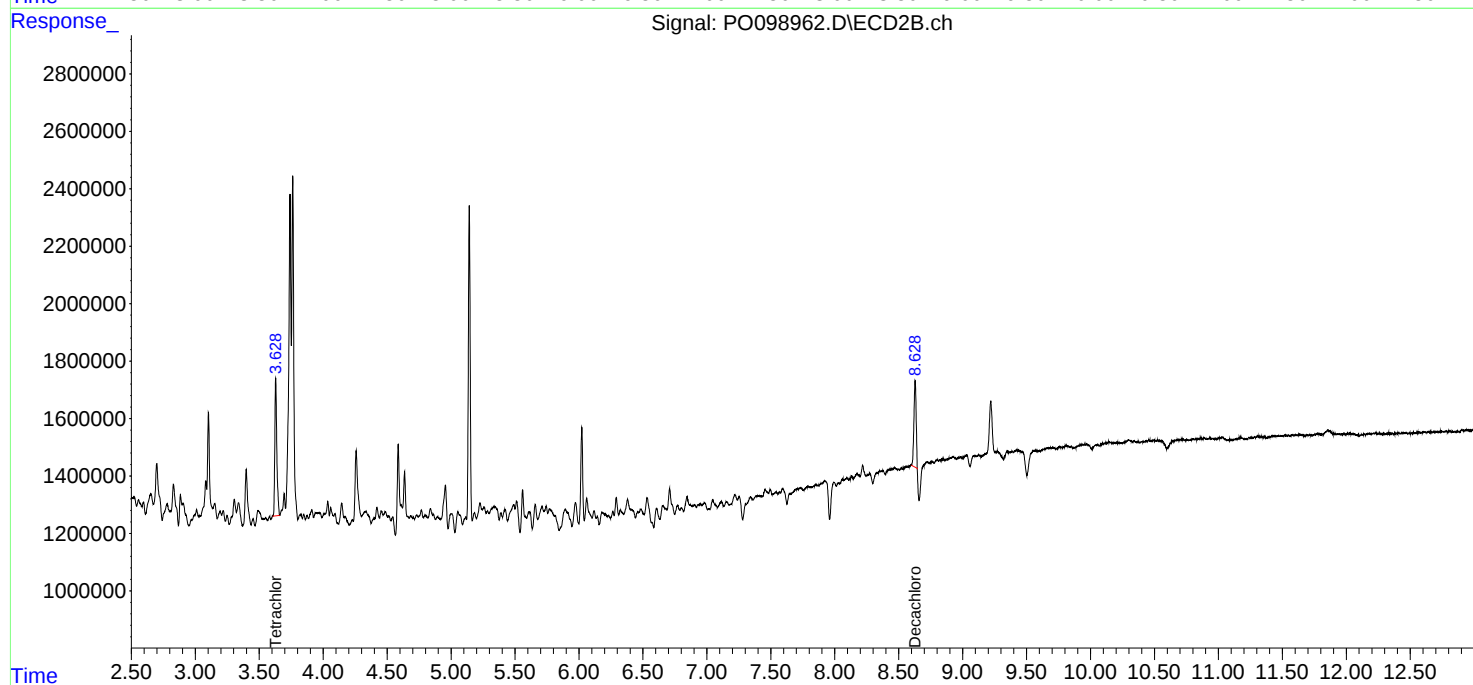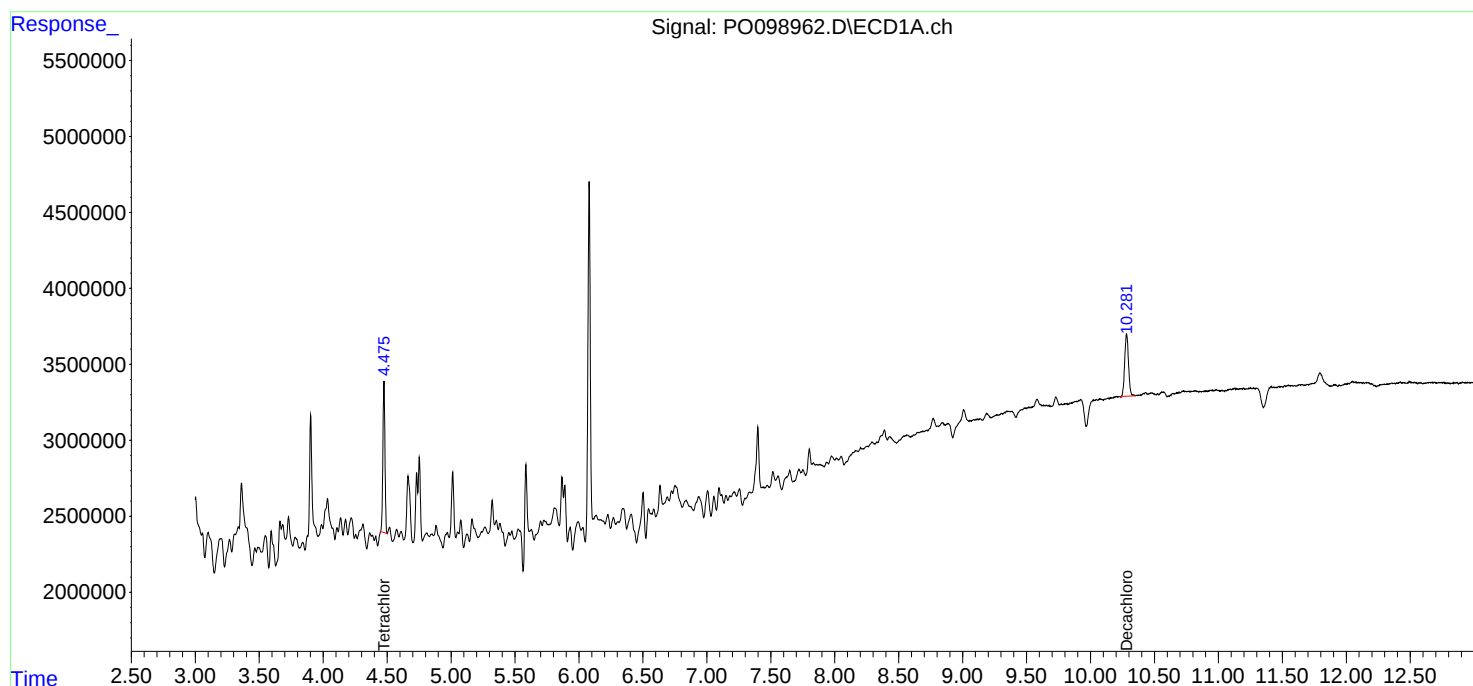

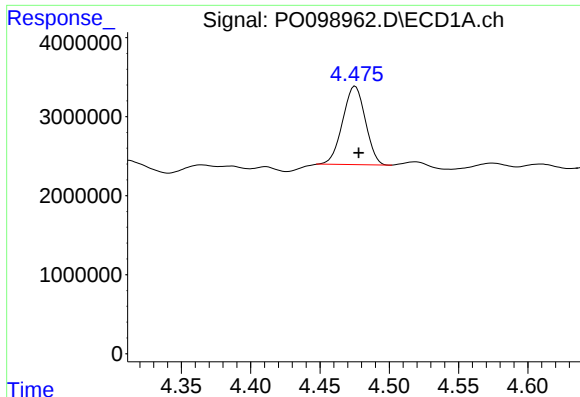


#1 Tetrachloro-m-xylene

R.T.: 4.475 min
Delta R.T.: -0.003 min
Response: 11318285
Conc: 5.73 ng/ml

Instrument :
ECD_O
ClientSampleId :
1021-1024


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/27/2023
Supervised By :Ankita Jodhani 10/27/2023

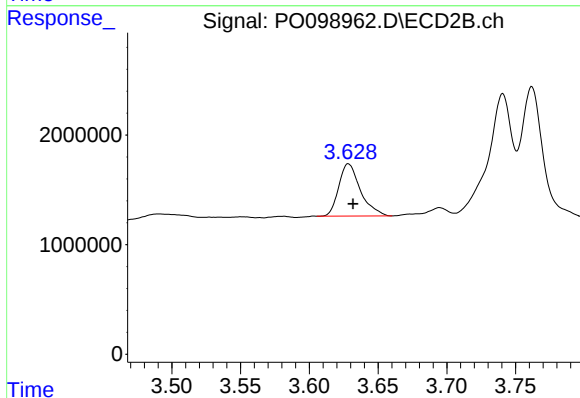


#1 Tetrachloro-m-xylene

R.T.: 3.629 min
Delta R.T.: -0.003 min
Response: 5236832
Conc: 7.28 ng/ml

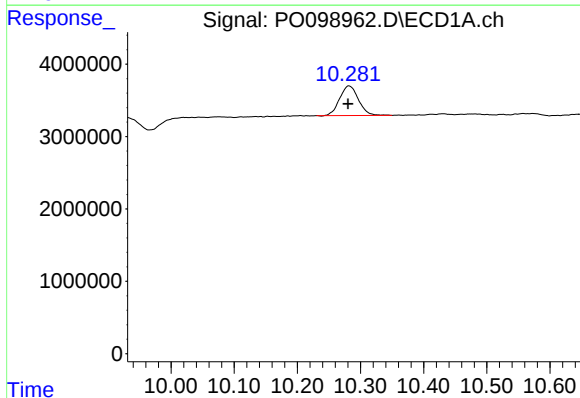

#2 Decachlorobiphenyl

R.T.: 10.282 min
Delta R.T.: 0.002 min
Response: 8462615
Conc: 7.47 ng/ml

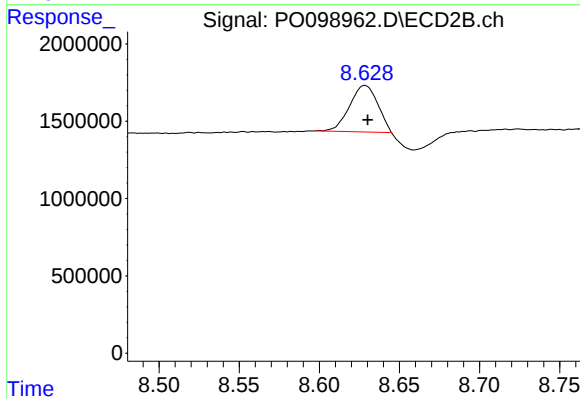

#2 Decachlorobiphenyl

R.T.: 8.628 min
Delta R.T.: -0.002 min
Response: 3671621
Conc: 6.84 ng/ml m