

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0102623\
 Data File : P0098964.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Oct 2023 10:55
 Operator : YP/AJ
 Sample : 05036-02RE
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 BUR-1282RE

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/27/2023
 Supervised By :Ankita Jodhani 10/27/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 26 15:14:10 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0102523.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 25 06:04:36 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.475	3.630	16935743	4779584	8.571m	6.641m
2) SA Decachlor...	10.273	8.626	5888666	2862568	5.198	5.335

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102623\
Data File : PO098964.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Oct 2023 10:55
Operator : YP/AJ
Sample : 05036-02RE
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
BUR-1282RE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/27/2023
Supervised By :Ankita Jodhani 10/27/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 26 15:14:10 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102523.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 25 06:04:36 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

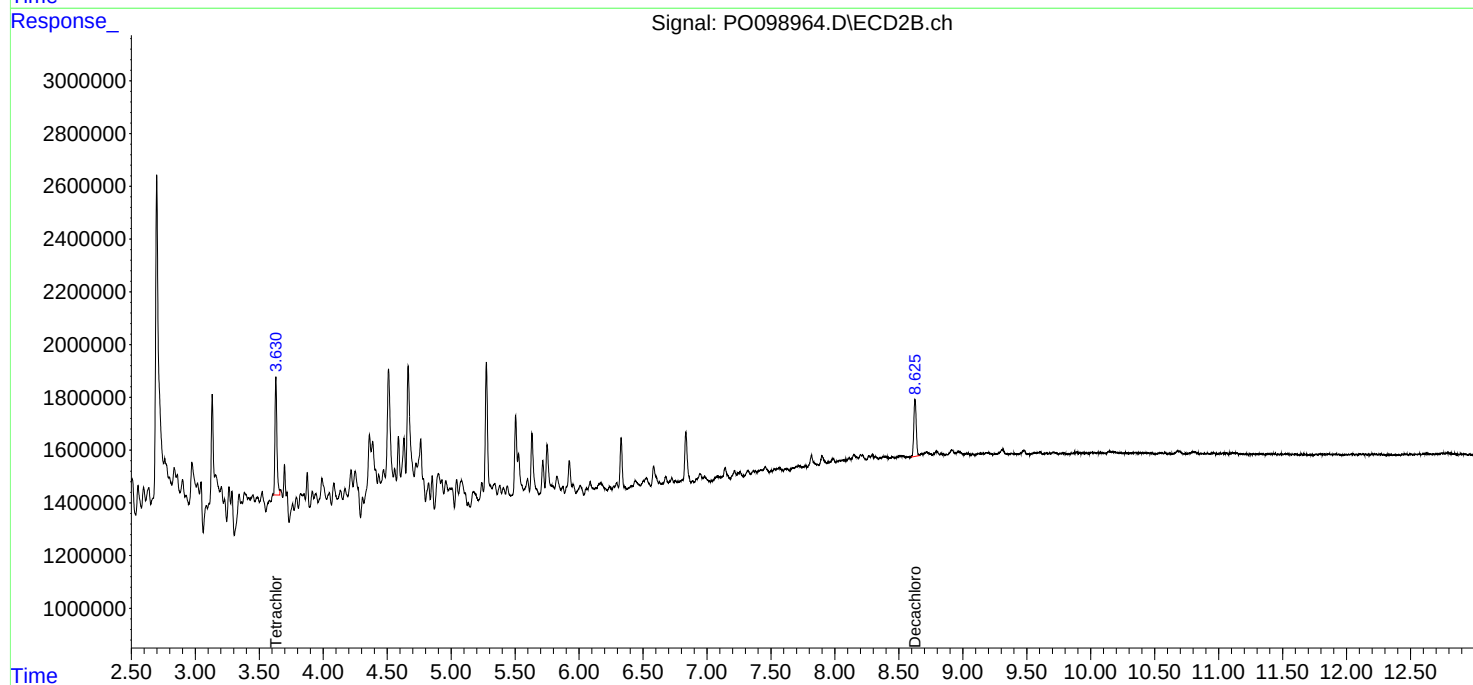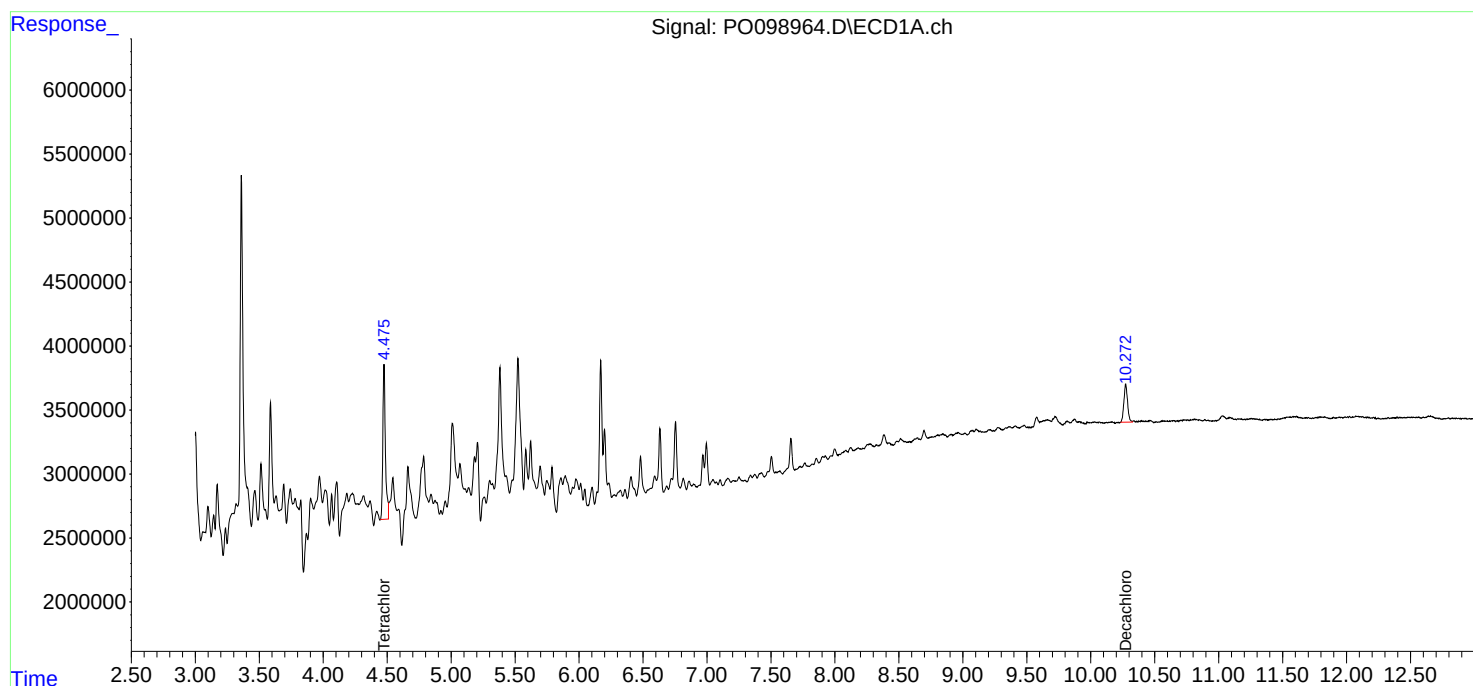

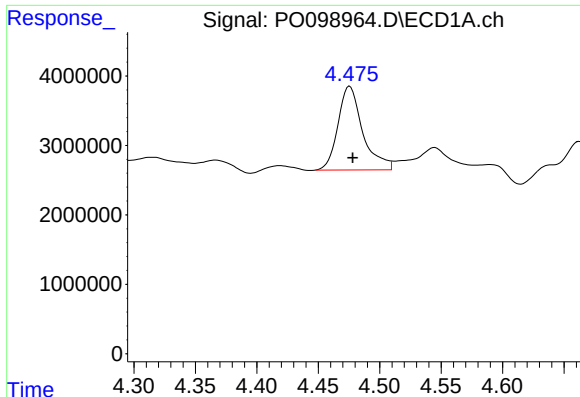


#1 Tetrachloro-m-xylene

R.T.: 4.475 min
Delta R.T.: -0.003 min
Response: 16935743
Conc: 8.57 ng/ml

Instrument :
ECD_O
ClientSampleId :
BUR-1282RE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/27/2023
Supervised By :Ankita Jodhani 10/27/2023

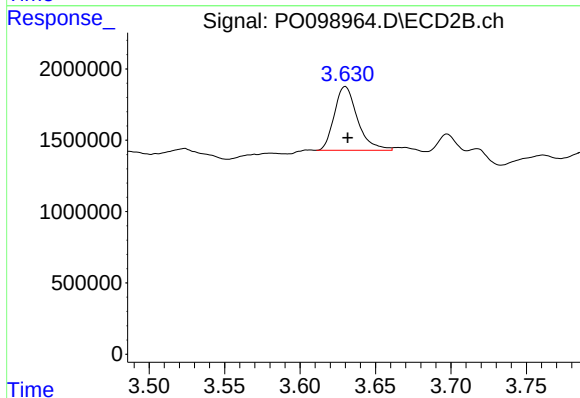


#1 Tetrachloro-m-xylene

R.T.: 3.630 min
Delta R.T.: -0.002 min
Response: 4779584
Conc: 6.64 ng/ml m

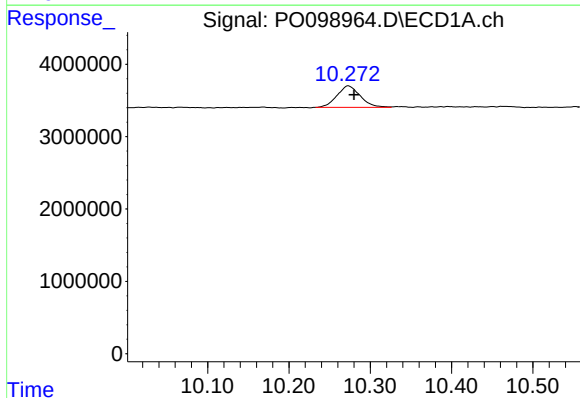

#2 Decachlorobiphenyl

R.T.: 10.273 min
Delta R.T.: -0.007 min
Response: 5888666
Conc: 5.20 ng/ml

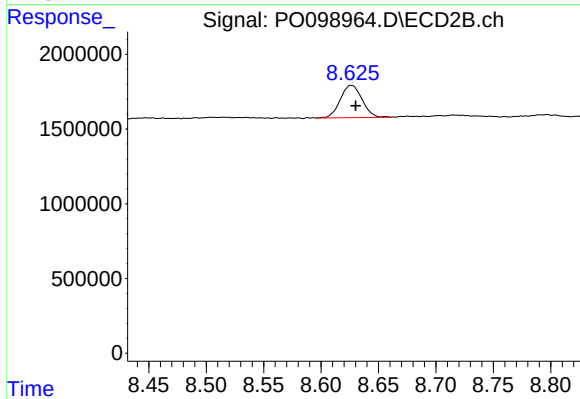

#2 Decachlorobiphenyl

R.T.: 8.626 min
Delta R.T.: -0.004 min
Response: 2862568
Conc: 5.34 ng/ml