

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0102623\
 Data File : P0099001.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Oct 2023 02:00
 Operator : YP/AJ
 Sample : 05075-01 10X
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SWC-1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/27/2023
 Supervised By :Ankita Jodhani 10/27/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 27 03:25:58 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0102523.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 25 06:04:36 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.476	3.630	3298495	1453016	1.669	2.019
2) SA Decachlor...	10.278	8.629	2102118	1245132	1.856	2.321 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102623\
Data File : PO099001.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Oct 2023 02:00
Operator : YP/AJ
Sample : 05075-01 10X
Misc :
ALS Vial : 33 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SWC-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/27/2023
Supervised By :Ankita Jodhani 10/27/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 27 03:25:58 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102523.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 25 06:04:36 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

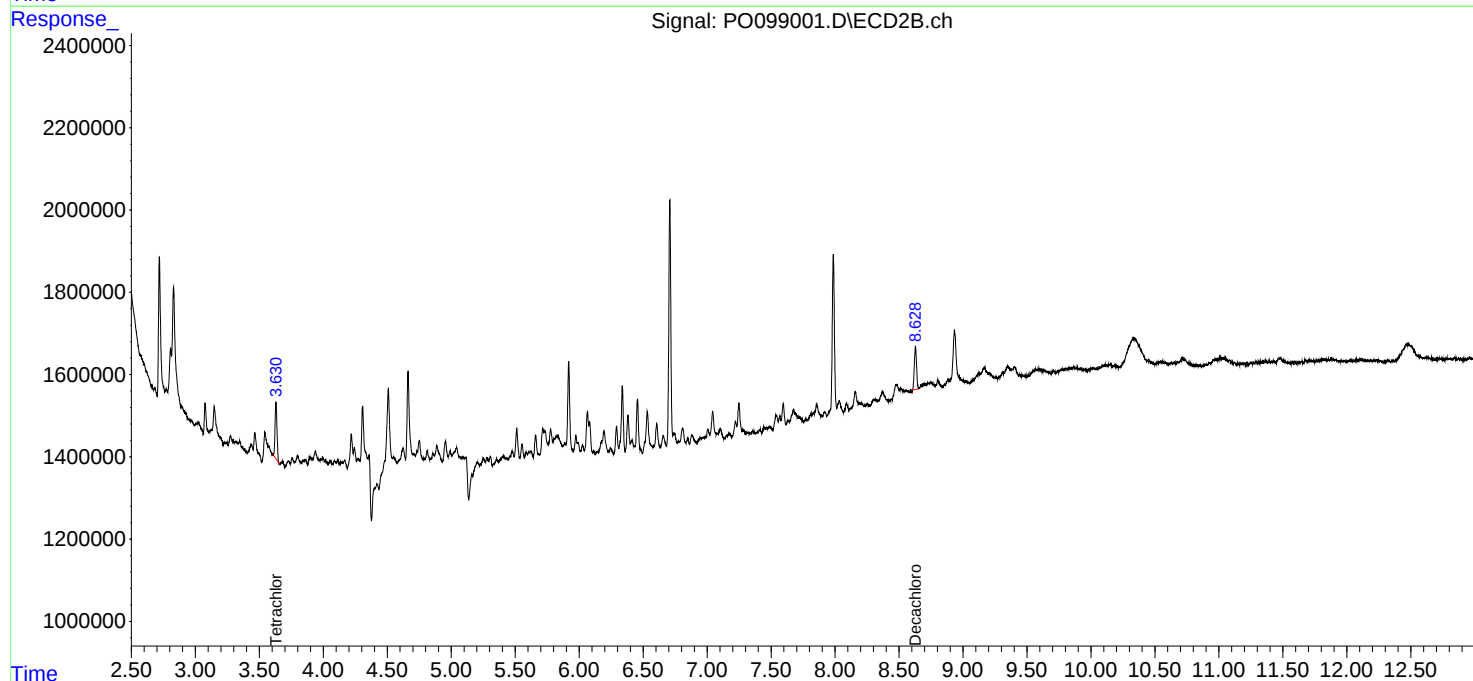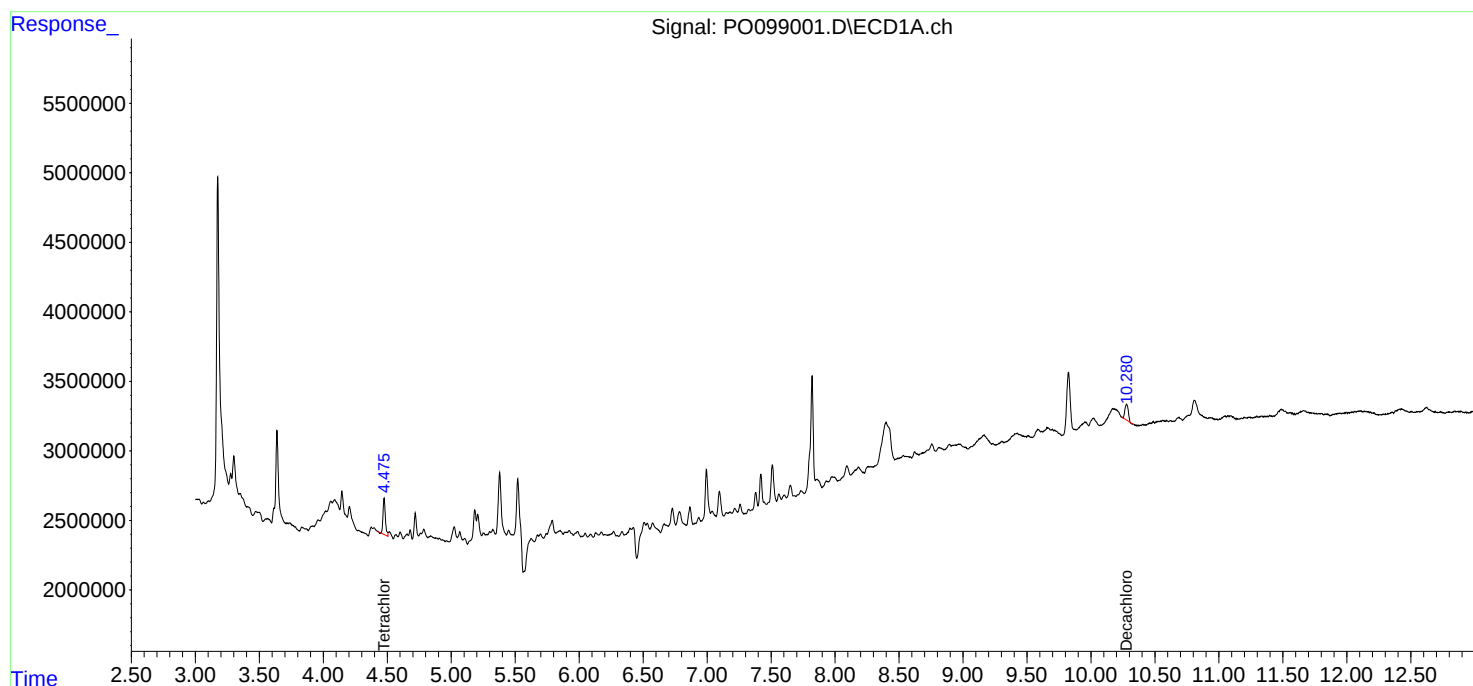

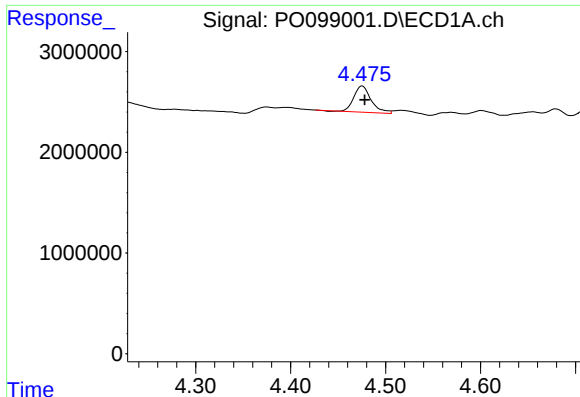


#1 Tetrachloro-m-xylene

R.T.: 4.476 min
Delta R.T.: -0.002 min
Response: 3298495
Conc: 1.67 ng/ml

Instrument :
ECD_O
ClientSampleId :
SWC-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/27/2023
Supervised By :Ankita Jodhani 10/27/2023

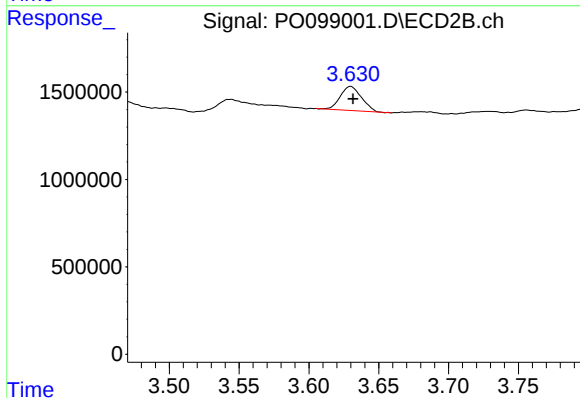


#1 Tetrachloro-m-xylene

R.T.: 3.630 min
Delta R.T.: -0.002 min
Response: 1453016
Conc: 2.02 ng/ml

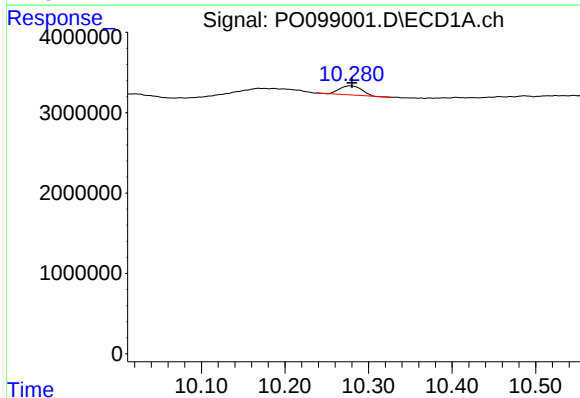

#2 Decachlorobiphenyl

R.T.: 10.278 min
Delta R.T.: -0.002 min
Response: 2102118
Conc: 1.86 ng/ml

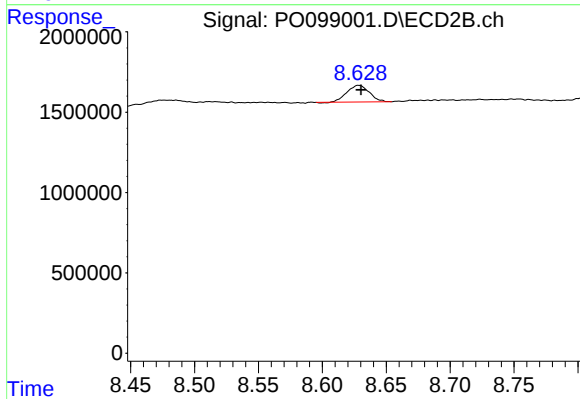

#2 Decachlorobiphenyl

R.T.: 8.629 min
Delta R.T.: -0.002 min
Response: 1245132
Conc: 2.32 ng/ml