

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0102623\
 Data File : P0099019.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Oct 2023 07:05
 Operator : YP/AJ
 Sample : 05075-12
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 WC-2

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/27/2023
 Supervised By :Ankita Jodhani 10/27/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 27 07:34:48 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0102523.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 25 06:04:36 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.474	3.629	31258933	11596225	15.820m	16.113m
2) SA Decachlor...	10.277	8.628	30545891	10322468	26.963	19.239 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102623\
Data File : PO099019.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Oct 2023 07:05
Operator : YP/AJ
Sample : 05075-12
Misc :
ALS Vial : 51 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
WC-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/27/2023
Supervised By :Ankita Jodhani 10/27/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 27 07:34:48 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102523.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 25 06:04:36 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

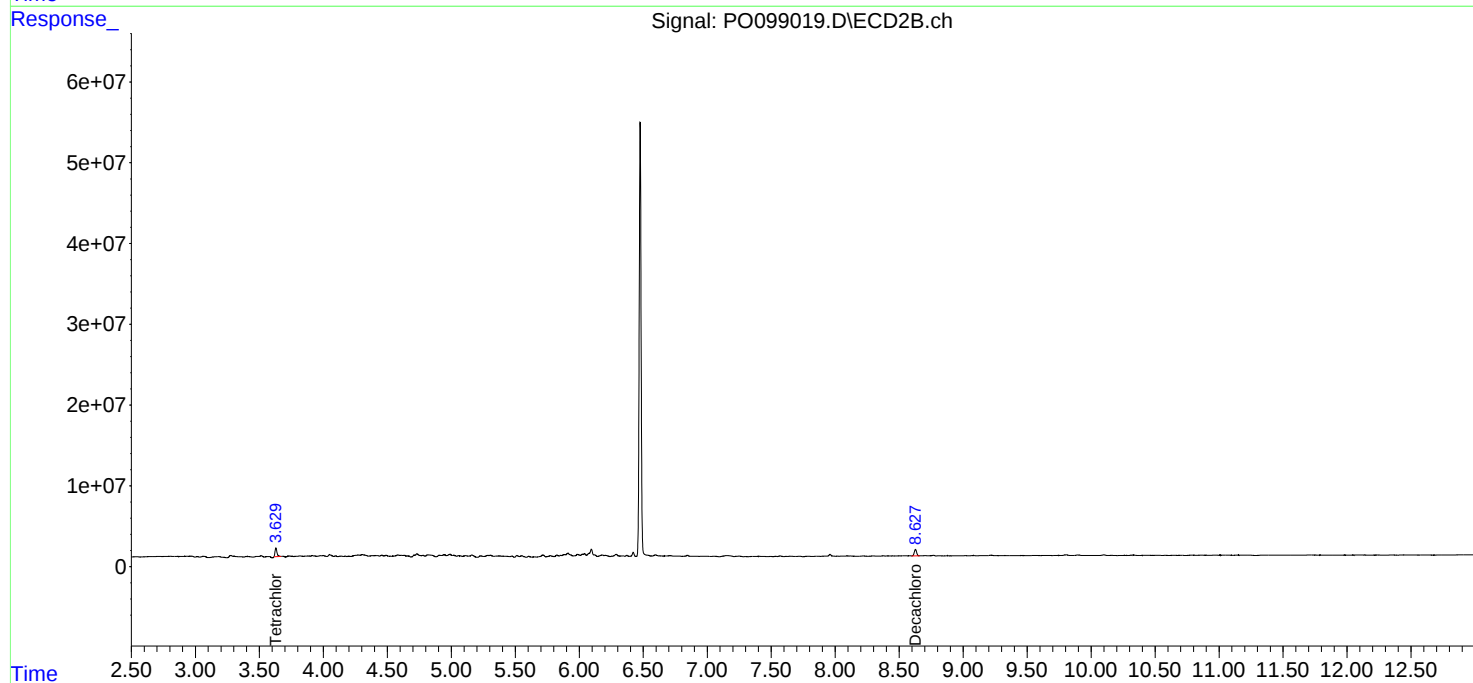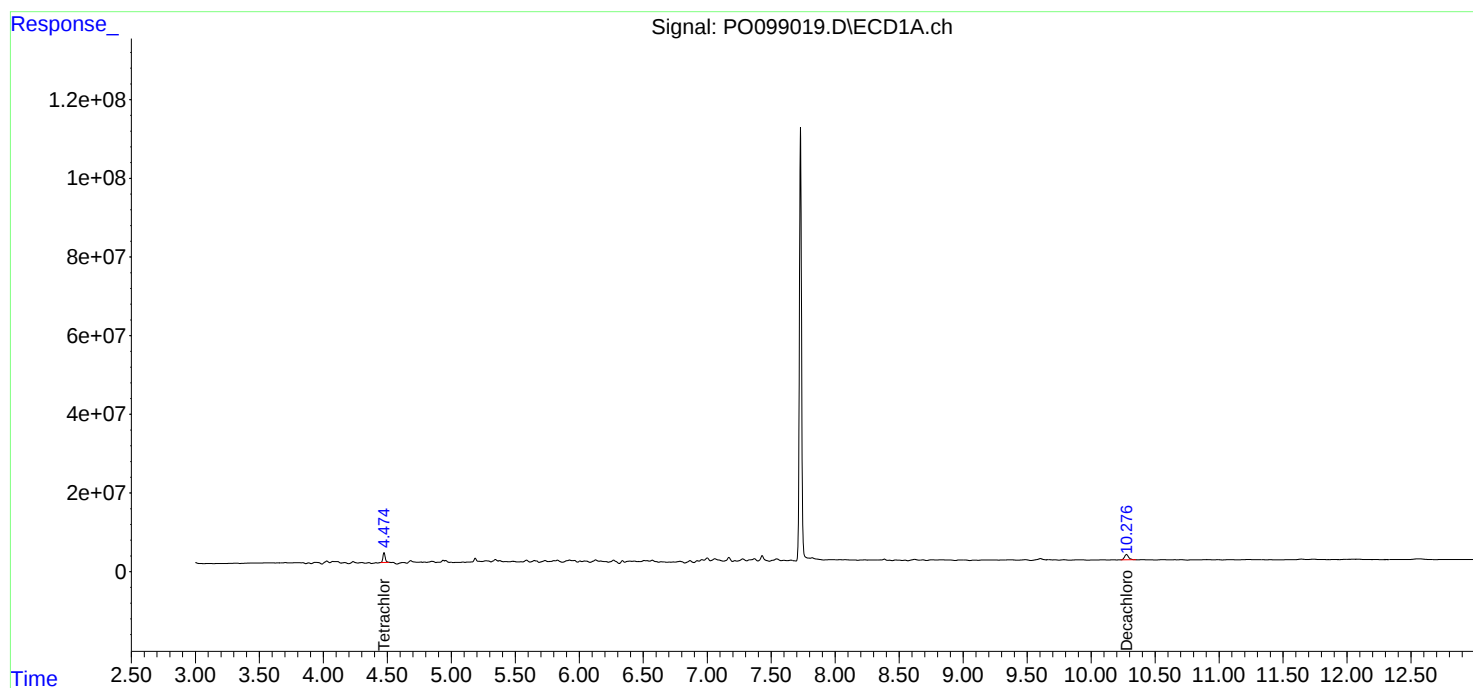

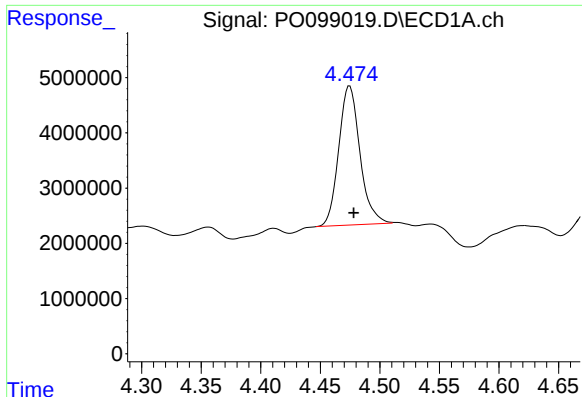


#1 Tetrachloro-m-xylene

R.T.: 4.474 min
Delta R.T.: -0.004 min
Response: 31258933
Conc: 15.82 ng/ml

Instrument :
ECD_O
ClientSampleId :
WC-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/27/2023
Supervised By :Ankita Jodhani 10/27/2023

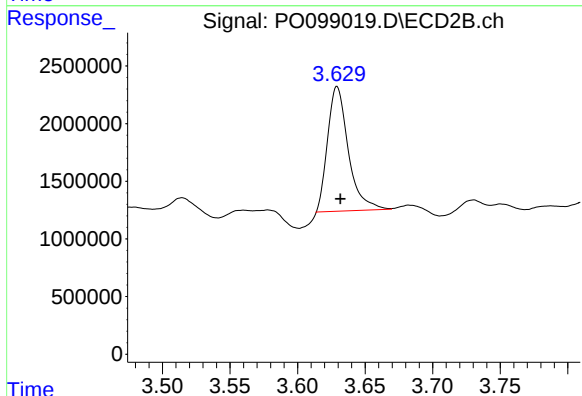


#1 Tetrachloro-m-xylene

R.T.: 3.629 min
Delta R.T.: -0.003 min
Response: 11596225
Conc: 16.11 ng/ml m

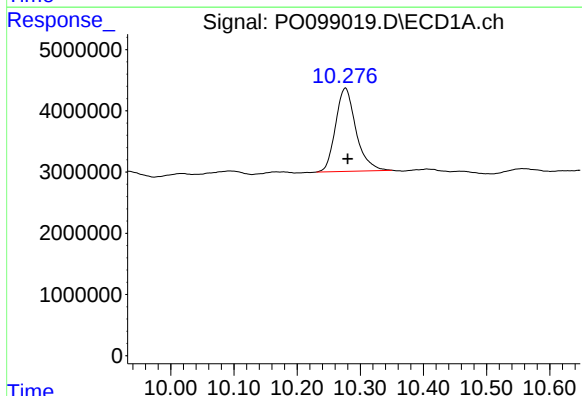

#2 Decachlorobiphenyl

R.T.: 10.277 min
Delta R.T.: -0.003 min
Response: 30545891
Conc: 26.96 ng/ml

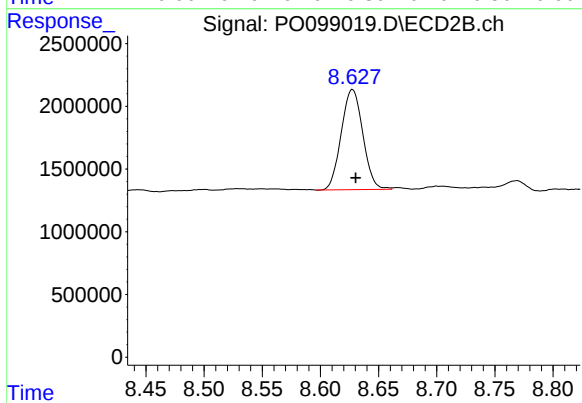

#2 Decachlorobiphenyl

R.T.: 8.628 min
Delta R.T.: -0.003 min
Response: 10322468
Conc: 19.24 ng/ml