

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0102720\
 Data File : P0072802.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 27 Oct 2020 11:20
 Operator : DD\AJ
 Sample : PB132443BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PB132443BL

Manual Integrations
 APPROVED

Ankita
 10/28/2020 4:41:42 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 28 07:29:05 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0102620.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Oct 27 16:48:42 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.948	4.023	746748	538232	16.196	15.357
2) SA Decachlor...	10.980	9.312	697309	690002	18.874m	20.690

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102720\
Data File : PO072802.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 27 Oct 2020 11:20
Operator : DD\AJ
Sample : PB132443BL
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
PB132443BL


Manual Integrations
APPROVED

Ankita
10/28/2020 4:41:42 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 28 07:29:05 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102620.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Oct 27 16:48:42 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

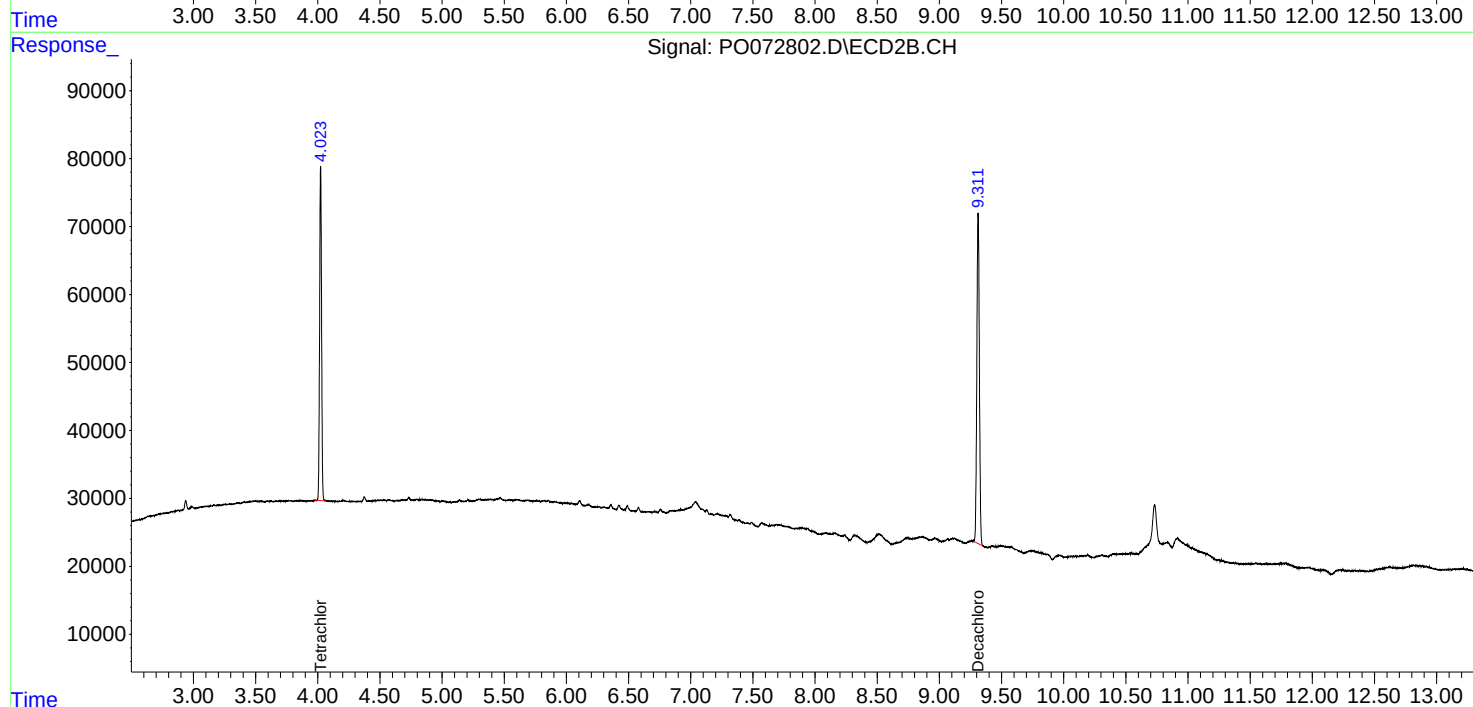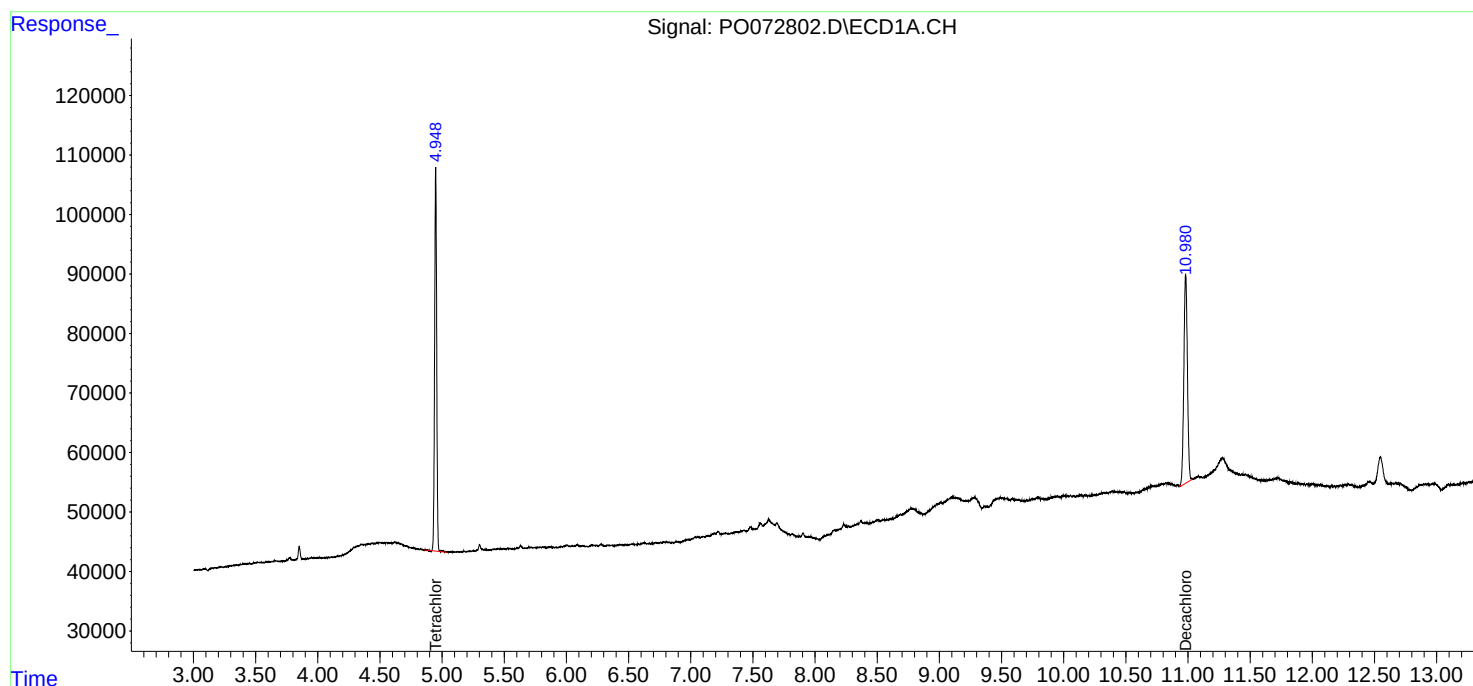

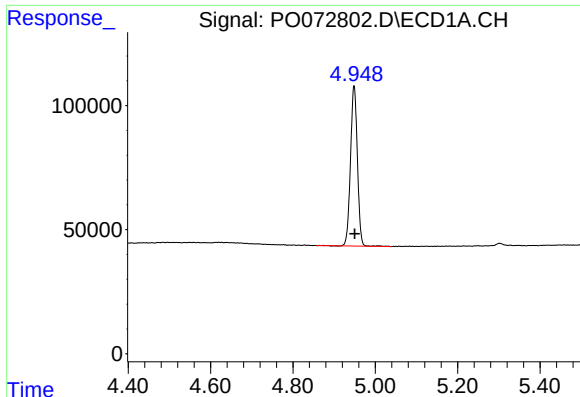


#1 Tetrachloro-m-xylene

R.T.: 4.948 min
Delta R.T.: -0.002 min
Response: 746748
Conc: 16.20 ng/ml

Instrument :
ECD_O
ClientSampleId :
PB132443BL


Manual Integrations
APPROVED

Ankita
10/28/2020 4:41:42 PM

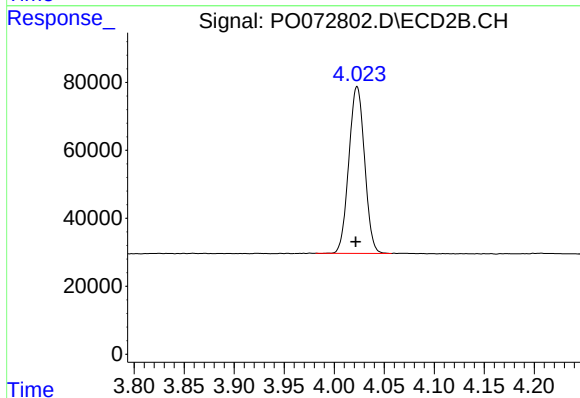


#1 Tetrachloro-m-xylene

R.T.: 4.023 min
Delta R.T.: 0.001 min
Response: 538232
Conc: 15.36 ng/ml

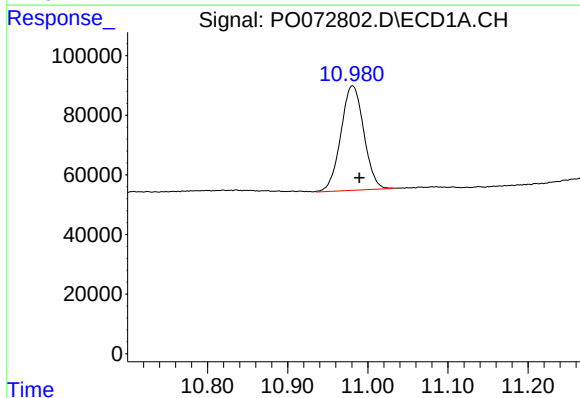

#2 Decachlorobiphenyl

R.T.: 10.980 min
Delta R.T.: -0.009 min
Response: 697309
Conc: 18.87 ng/ml m

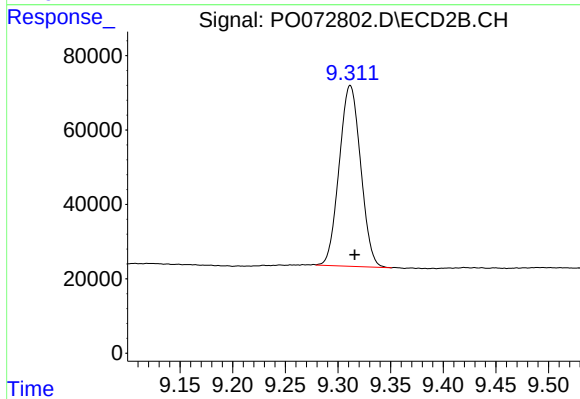

#2 Decachlorobiphenyl

R.T.: 9.312 min
Delta R.T.: -0.004 min
Response: 690002
Conc: 20.69 ng/ml