

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0102720\
 Data File : P0072819.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 27 Oct 2020 16:10
 Operator : DD\AJ
 Sample : L4214-07
 Misc : AR1254 LOD 25 PPB
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 LOD-MDL-WATER-01-QT4-2020

Manual Integrations
 APPROVED

Ankita
 10/28/2020 4:42:14 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 28 08:01:51 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0102620.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Oct 27 16:48:42 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.948	4.023	763362	567098	16.556	16.181
2) SA Decachlor...	10.983	9.311	742677	714679	20.102	21.430
Target Compounds						
26) L6 AR-1254-1	7.185	6.146	56200	56789	32.428	25.231
27) L6 AR-1254-2	7.415	6.305	68577	46149	25.665m	22.977
28) L6 AR-1254-3	7.797	6.723	77842	80618	28.803m	25.374
29) L6 AR-1254-4	8.095	6.961	65138	59987	29.724	27.581m
30) L6 AR-1254-5	8.525	7.389	58231	69766	26.449m	25.066

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102720\
Data File : PO072819.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 27 Oct 2020 16:10
Operator : DD\AJ
Sample : L4214-07
Misc : AR1254 LOD 25 PPB
ALS Vial : 23 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleID :
LOD-MDL-WATER-01-QT4-2020


Manual Integrations
APPROVED

Ankita
10/28/2020 4:42:14 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 28 08:01:51 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102620.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Oct 27 16:48:42 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

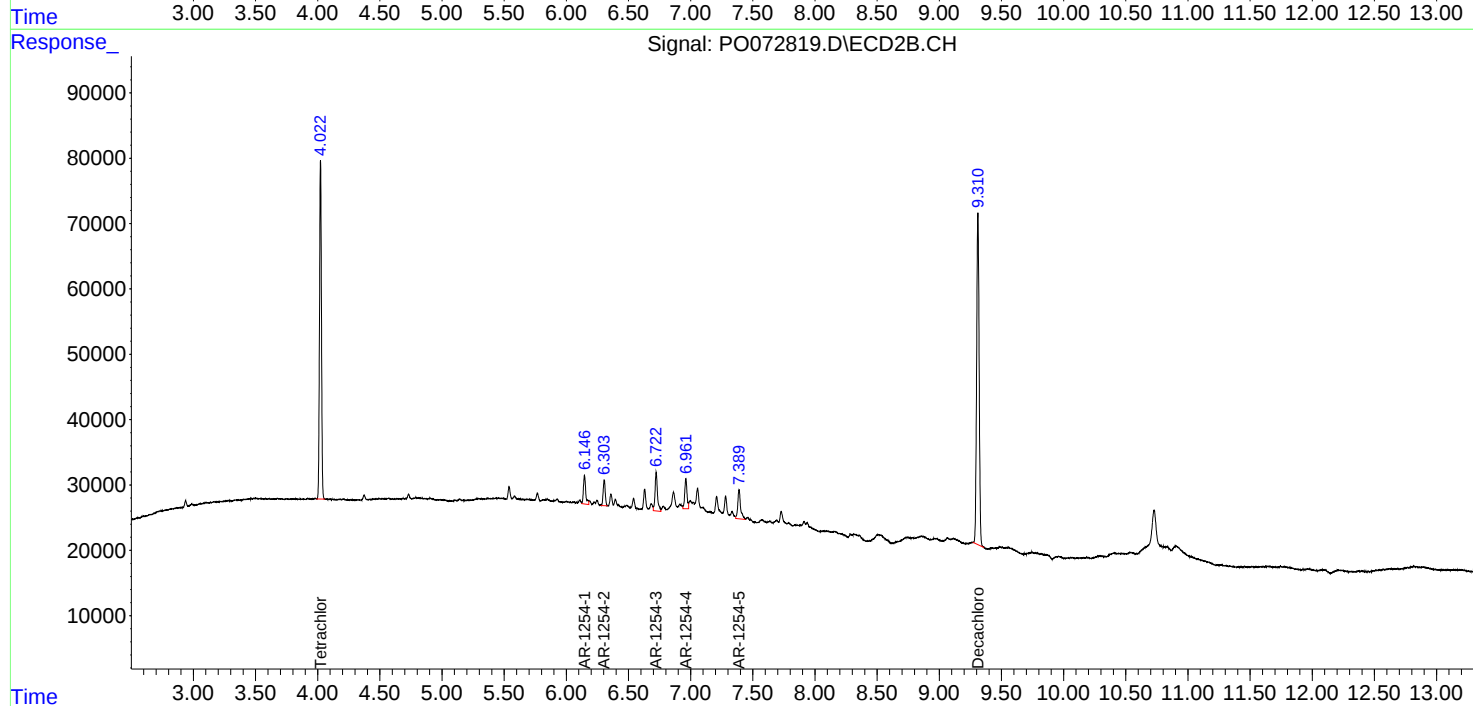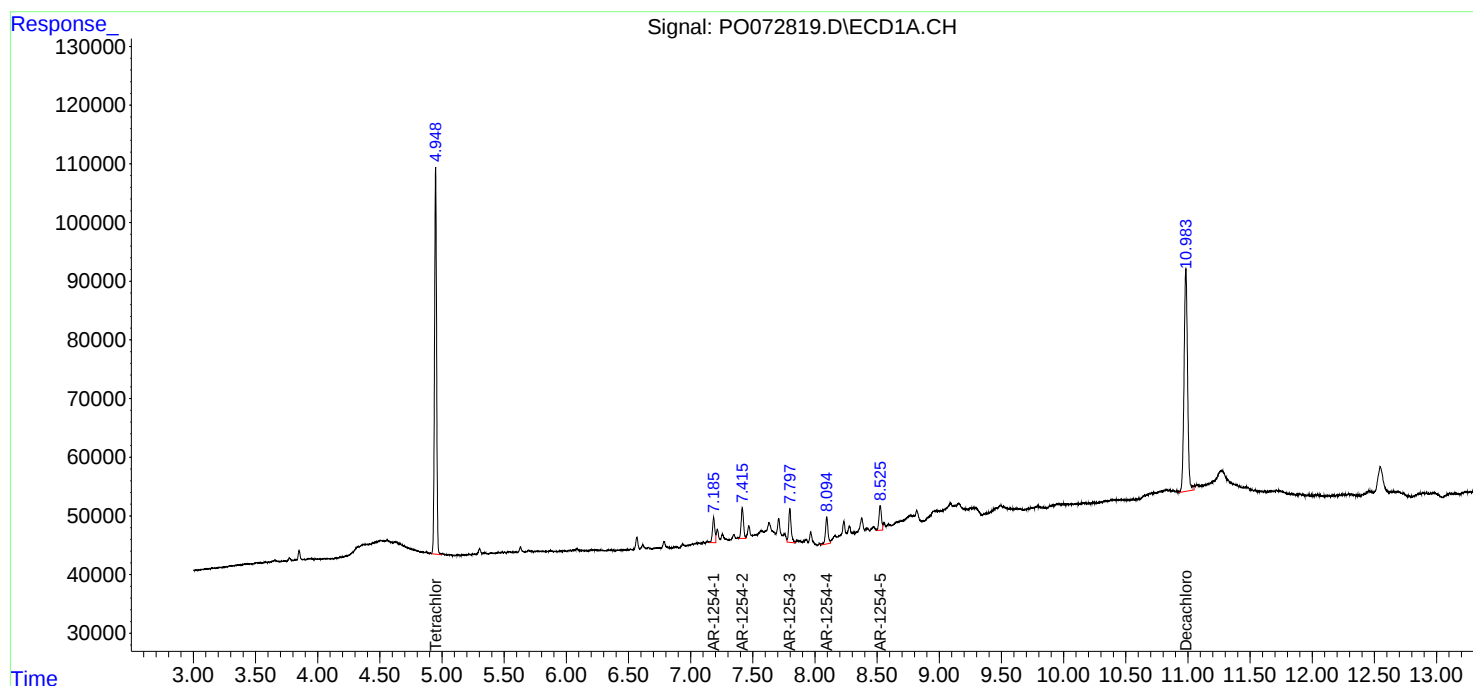

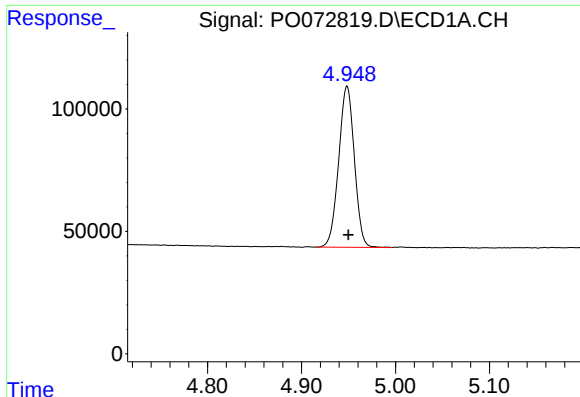


#1 Tetrachloro-m-xylene

R.T.: 4.948 min
Delta R.T.: -0.002 min
Response: 763362
Conc: 16.56 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2020


Manual Integrations
APPROVED

Ankita
10/28/2020 4:42:14 PM

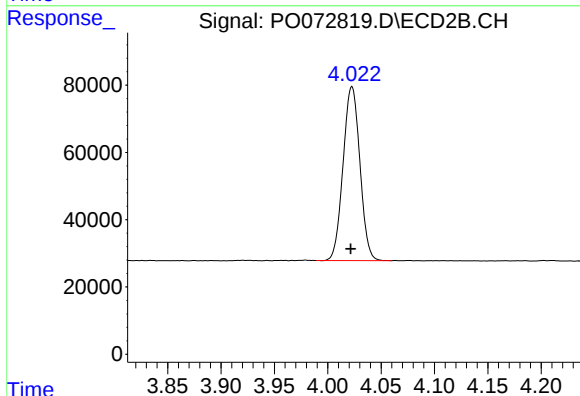


#1 Tetrachloro-m-xylene

R.T.: 4.023 min
Delta R.T.: 0.001 min
Response: 567098
Conc: 16.18 ng/ml

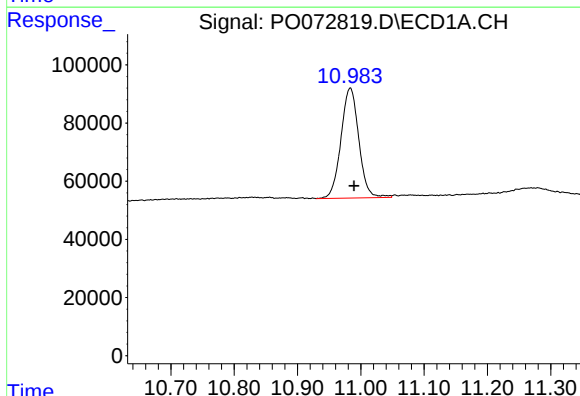


#2 Decachlorobiphenyl

R.T.: 10.983 min
Delta R.T.: -0.006 min
Response: 742677
Conc: 20.10 ng/ml

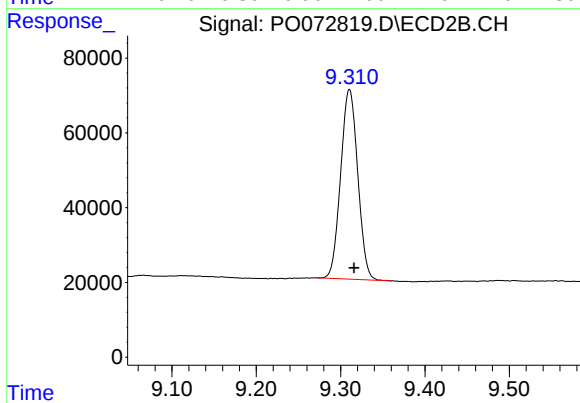

#2 Decachlorobiphenyl

R.T.: 9.311 min
Delta R.T.: -0.005 min
Response: 714679
Conc: 21.43 ng/ml

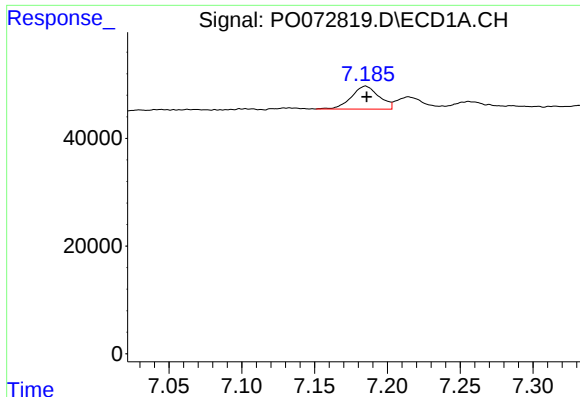


#26 AR-1254-1

R.T.: 7.185 min
Delta R.T.: 0.000 min
Response: 56200
Conc: 32.43 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2020


Manual Integrations
APPROVED

Ankita
10/28/2020 4:42:14 PM

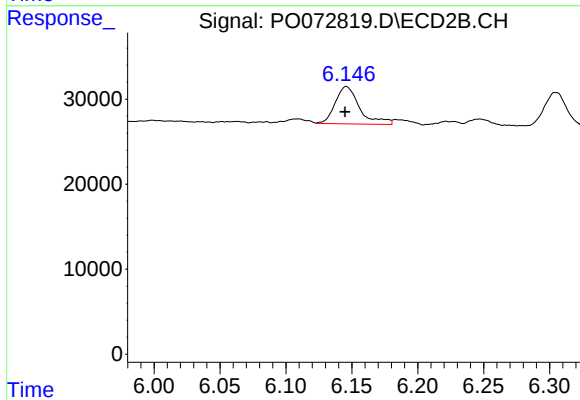


#26 AR-1254-1

R.T.: 6.146 min
Delta R.T.: 0.000 min
Response: 56789
Conc: 25.23 ng/ml

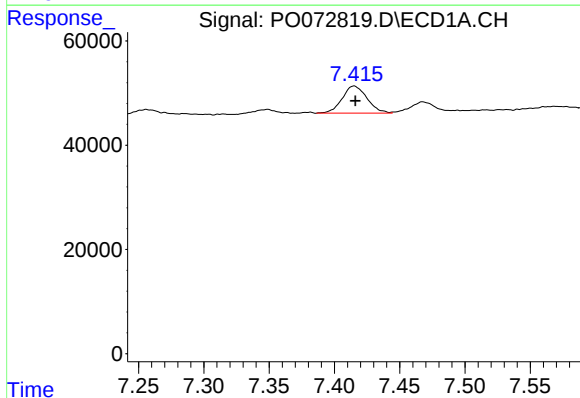


#27 AR-1254-2

R.T.: 7.415 min
Delta R.T.: -0.001 min
Response: 68577
Conc: 25.67 ng/ml m

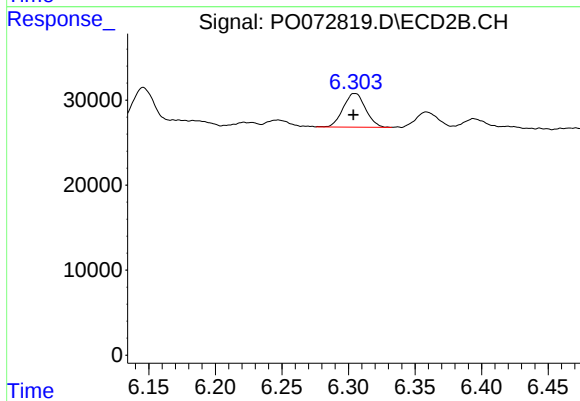

#27 AR-1254-2

R.T.: 6.305 min
Delta R.T.: 0.000 min
Response: 46149
Conc: 22.98 ng/ml

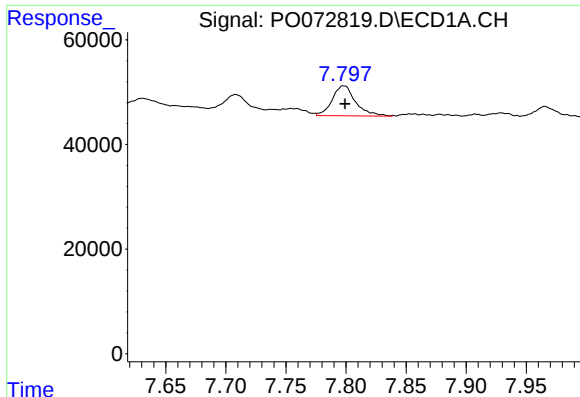


#28 AR-1254-3

R.T.: 7.797 min
Delta R.T.: -0.002 min
Response: 77842
Conc: 28.80 ng/ml m

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2020


Manual Integrations
APPROVED

Ankita
10/28/2020 4:42:14 PM

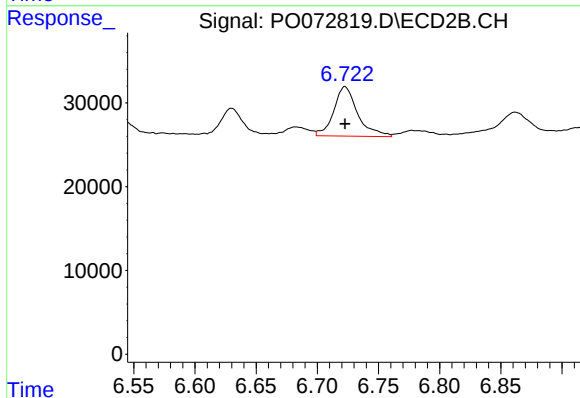


#28 AR-1254-3

R.T.: 6.723 min
Delta R.T.: 0.000 min
Response: 80618
Conc: 25.37 ng/ml

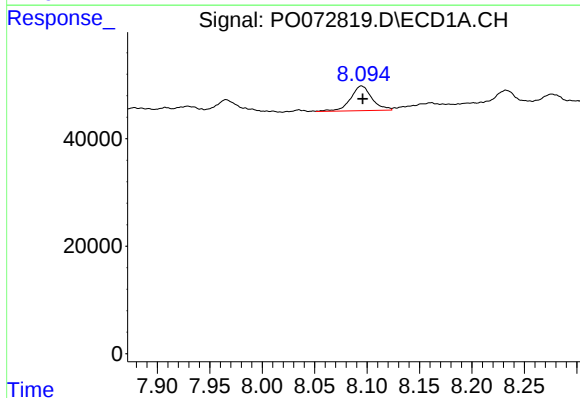


#29 AR-1254-4

R.T.: 8.095 min
Delta R.T.: -0.001 min
Response: 65138
Conc: 29.72 ng/ml

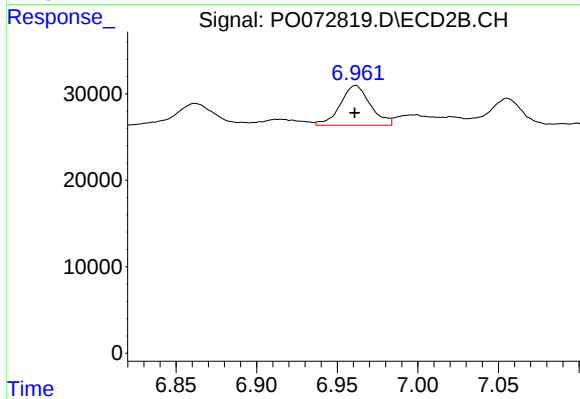

#29 AR-1254-4

R.T.: 6.961 min
Delta R.T.: 0.000 min
Response: 59987
Conc: 27.58 ng/ml m

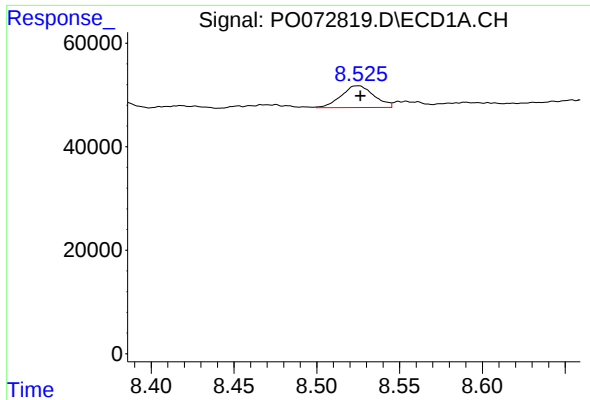


#30 AR-1254-5

R.T.: 8.525 min
Delta R.T.: -0.001 min
Response: 58231
Conc: 26.45 ng/ml m

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2020

Manual Integrations
APPROVED

Ankita
10/28/2020 4:42:14 PM

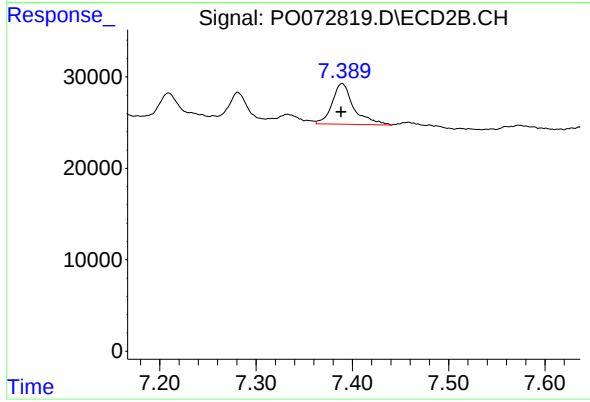

#30 AR-1254-5

R.T.: 7.389 min
Delta R.T.: 0.000 min
Response: 69766
Conc: 25.07 ng/ml