

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0102720\
 Data File : P0072820.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 27 Oct 2020 16:27
 Operator : DD\AJ
 Sample : L4214-07
 Misc : AR1262 LOD 25 PPB
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 LOD-MDL-WATER-01-QT4-2020

Manual Integrations
 APPROVED

Ankita
 10/28/2020 4:42:16 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 28 08:02:09 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0102620.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Oct 27 16:48:42 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.948	4.023	674721	497528	14.634	14.196
2) SA Decachlor...	10.980	9.311	638035	638287	17.270	19.140
Target Compounds						
36) L8 AR-1262-1	8.597	7.388	56119	35871	23.464m	25.871
37) L8 AR-1262-2	9.156	7.938	106567	102892	24.087m	22.554
38) L8 AR-1262-3	9.468	8.227	55760	265290	17.333m	144.979 #
39) L8 AR-1262-4	9.562	8.287	54181	182035	22.588m	54.680 #
40) L8 AR-1262-5	10.229	8.782	38208	34052	22.755	20.795

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102720\
Data File : PO072820.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 27 Oct 2020 16:27
Operator : DD\AJ
Sample : L4214-07
Misc : AR1262 LOD 25 PPB
ALS Vial : 24 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleID :
LOD-MDL-WATER-01-QT4-2020


Manual Integrations
APPROVED

Ankita
10/28/2020 4:42:16 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 28 08:02:09 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102620.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Oct 27 16:48:42 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

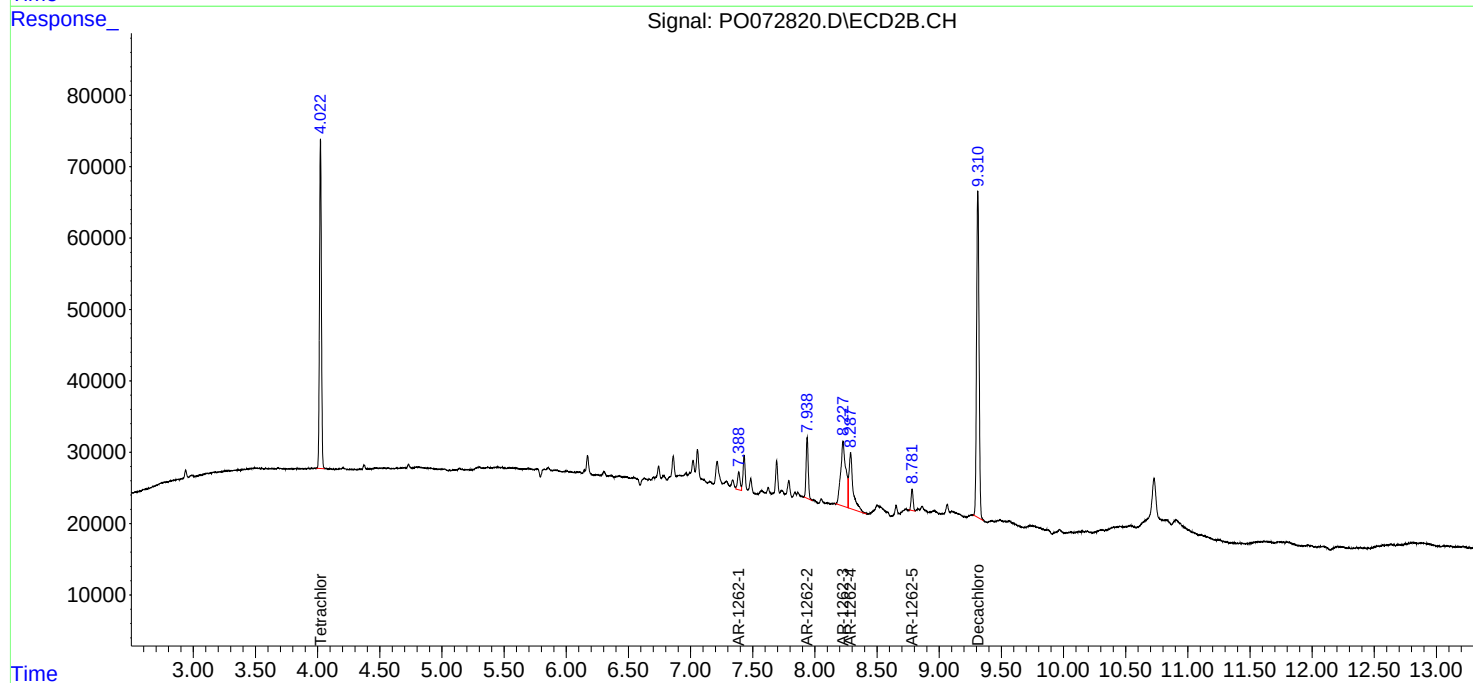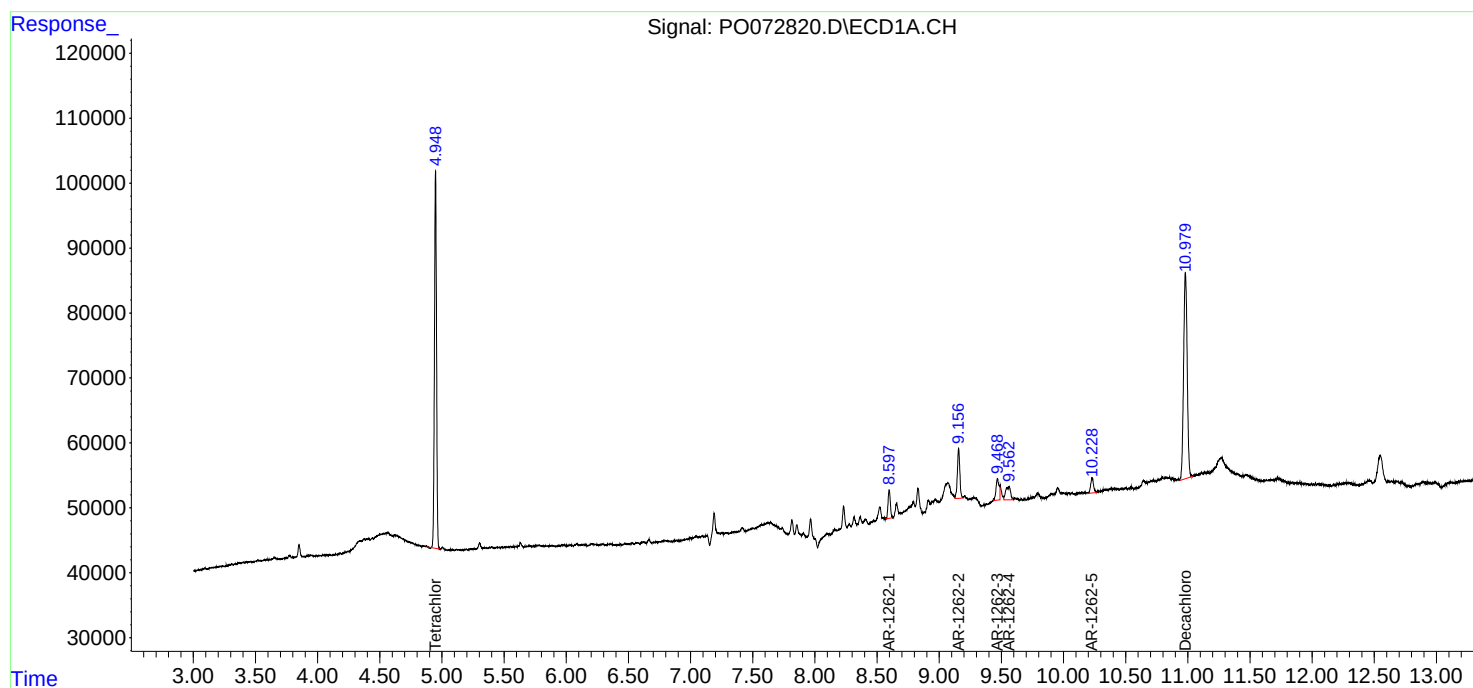

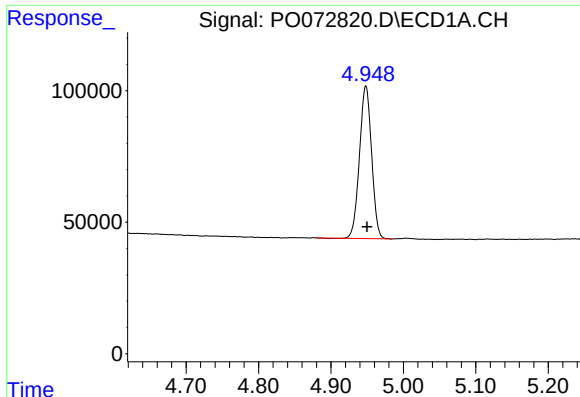


#1 Tetrachloro-m-xylene

R.T.: 4.948 min
Delta R.T.: -0.002 min
Response: 674721
Conc: 14.63 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2020


Manual Integrations
APPROVED

Ankita
10/28/2020 4:42:16 PM

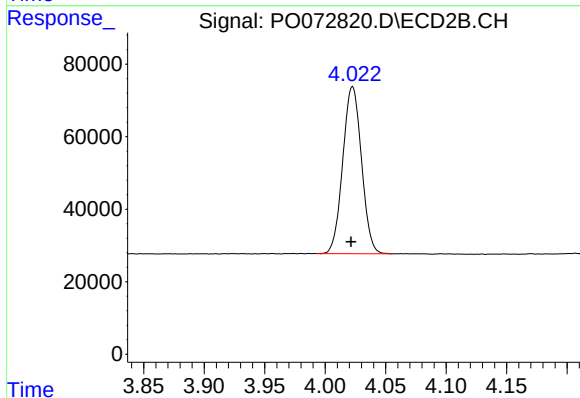


#1 Tetrachloro-m-xylene

R.T.: 4.023 min
Delta R.T.: 0.001 min
Response: 497528
Conc: 14.20 ng/ml

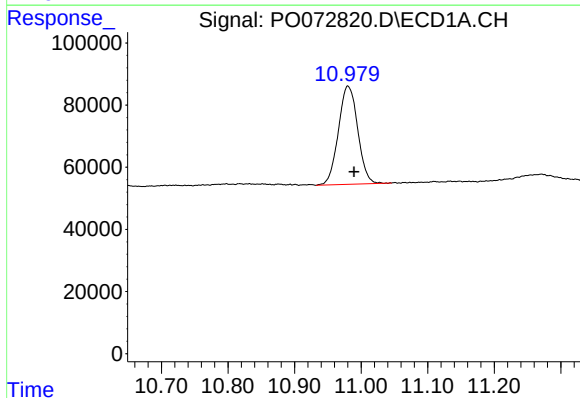


#2 Decachlorobiphenyl

R.T.: 10.980 min
Delta R.T.: -0.009 min
Response: 638035
Conc: 17.27 ng/ml

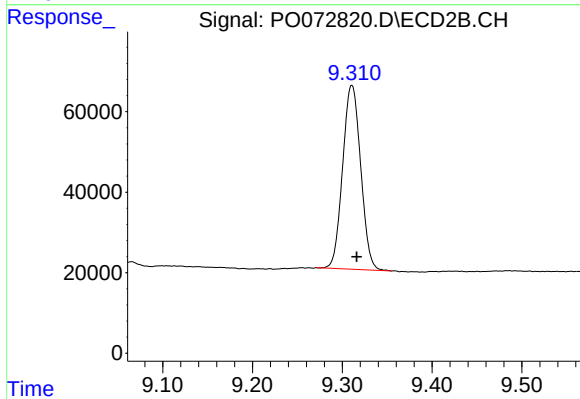

#2 Decachlorobiphenyl

R.T.: 9.311 min
Delta R.T.: -0.005 min
Response: 638287
Conc: 19.14 ng/ml

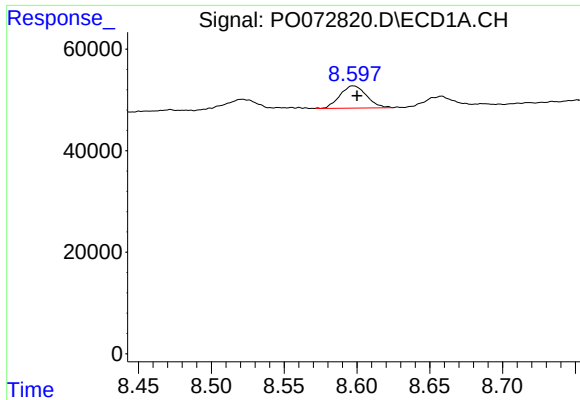


#36 AR-1262-1

R.T.: 8.597 min
Delta R.T.: -0.003 min
Response: 56119
Conc: 23.46 ng/ml m

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2020


Manual Integrations
APPROVED

Ankita
10/28/2020 4:42:16 PM

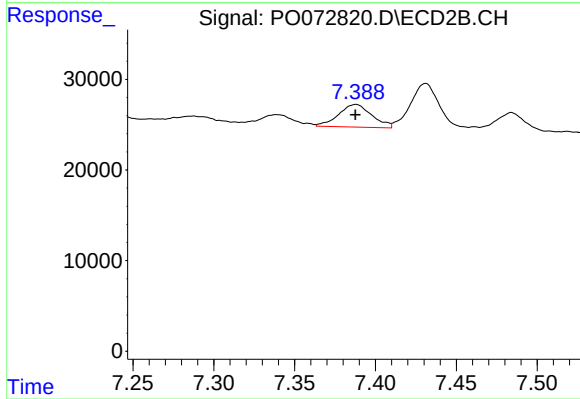


#36 AR-1262-1

R.T.: 7.388 min
Delta R.T.: 0.000 min
Response: 35871
Conc: 25.87 ng/ml

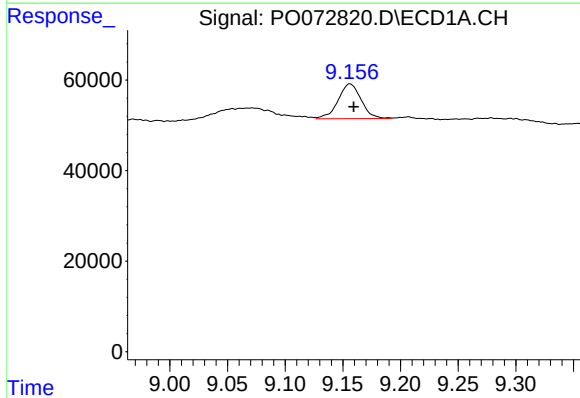


#37 AR-1262-2

R.T.: 9.156 min
Delta R.T.: -0.004 min
Response: 106567
Conc: 24.09 ng/ml m

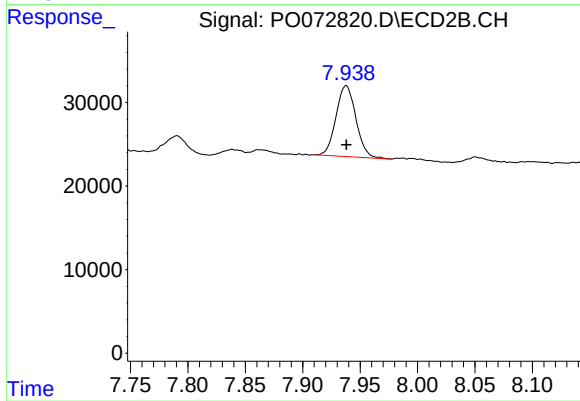

#37 AR-1262-2

R.T.: 7.938 min
Delta R.T.: 0.000 min
Response: 102892
Conc: 22.55 ng/ml

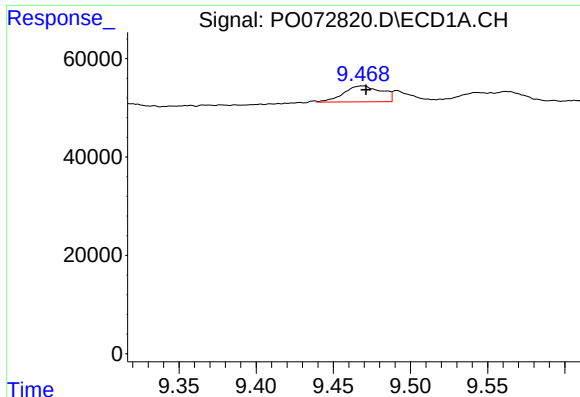


#38 AR-1262-3

R.T.: 9.468 min
Delta R.T.: -0.004 min
Response: 55760
Conc: 17.33 ng/ml m

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2020


Manual Integrations
APPROVED

Ankita
10/28/2020 4:42:16 PM

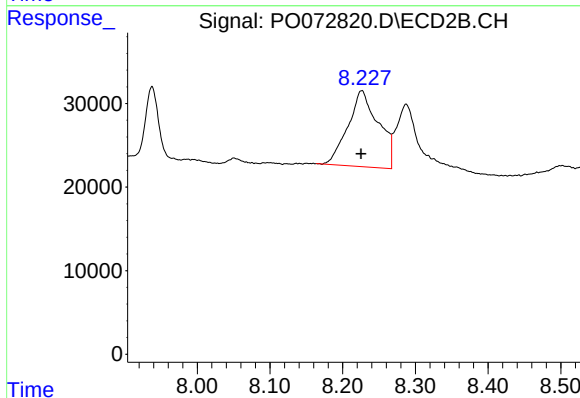


#38 AR-1262-3

R.T.: 8.227 min
Delta R.T.: 0.001 min
Response: 265290
Conc: 144.98 ng/ml

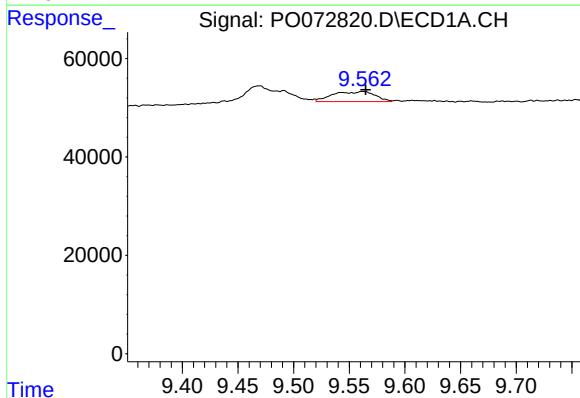


#39 AR-1262-4

R.T.: 9.562 min
Delta R.T.: -0.003 min
Response: 54181
Conc: 22.59 ng/ml m

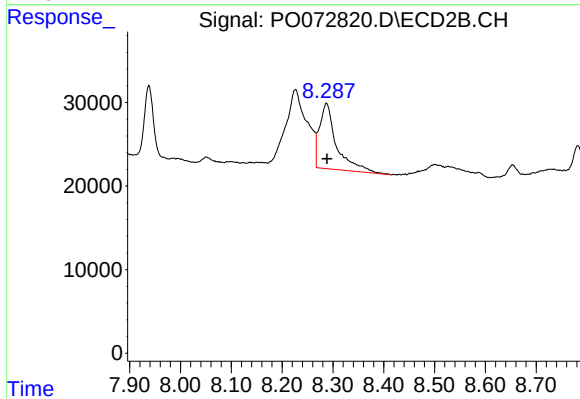

#39 AR-1262-4

R.T.: 8.287 min
Delta R.T.: -0.001 min
Response: 182035
Conc: 54.68 ng/ml

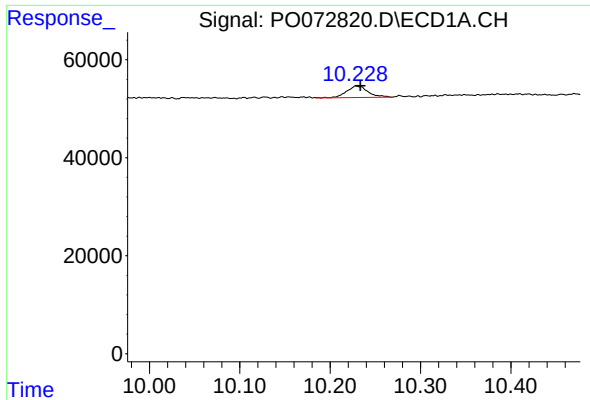


#40 AR-1262-5

R.T.: 10.229 min
Delta R.T.: -0.004 min
Response: 38208
Conc: 22.75 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT4-2020

Manual Integrations
APPROVED

Ankita
10/28/2020 4:42:16 PM

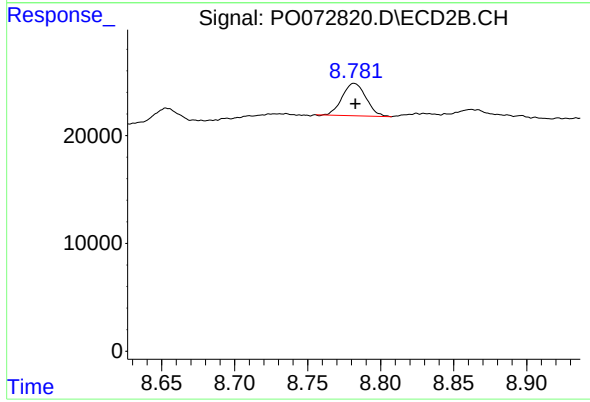

#40 AR-1262-5

R.T.: 8.782 min
Delta R.T.: 0.000 min
Response: 34052
Conc: 20.79 ng/ml