

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102720\
 Data File : PO072879.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 28 Oct 2020 10:26
 Operator : DD\AJ
 Sample : L4214-09
 Misc : AR1221 MDL 25 PPB
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MDL-WATER-03-QT4-2020

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 28 11:45:40 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102620.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Oct 27 16:48:42 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.948	4.021	761531	524137	16.517	14.955
2) SA Decachlor...	10.982	9.305	745133	729186	20.169	21.865

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102720\
Data File : PO072879.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 28 Oct 2020 10:26
Operator : DD\AJ
Sample : L4214-09
Misc : AR1221 MDL 25 PPB
ALS Vial : 53 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2020

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 28 11:45:40 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102620.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Oct 27 16:48:42 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

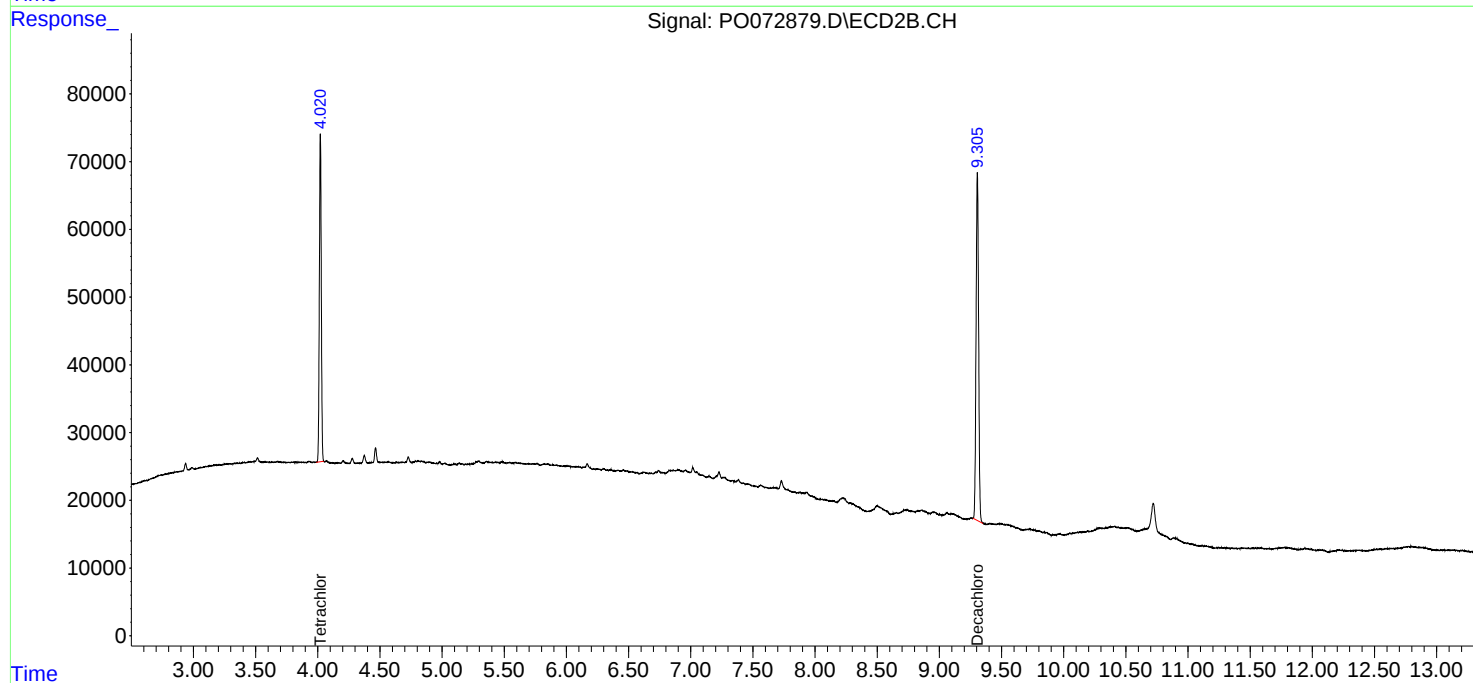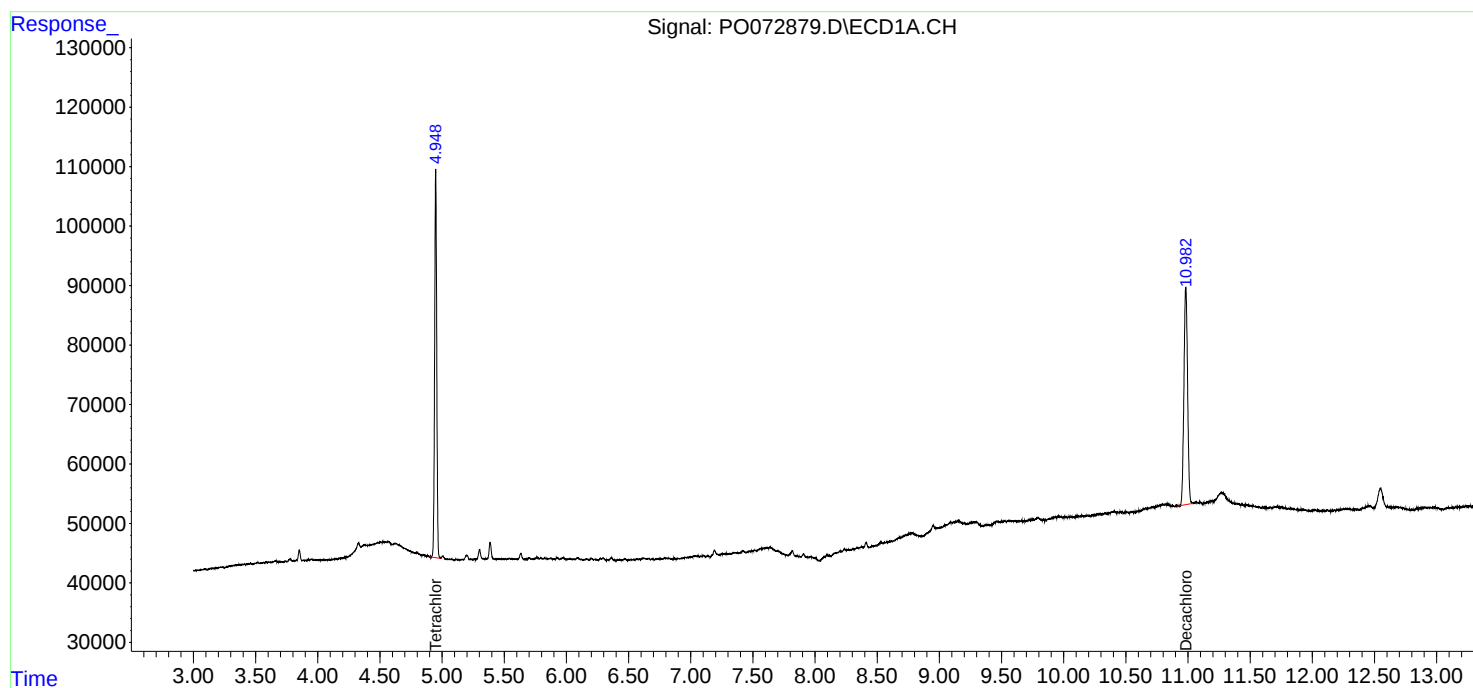


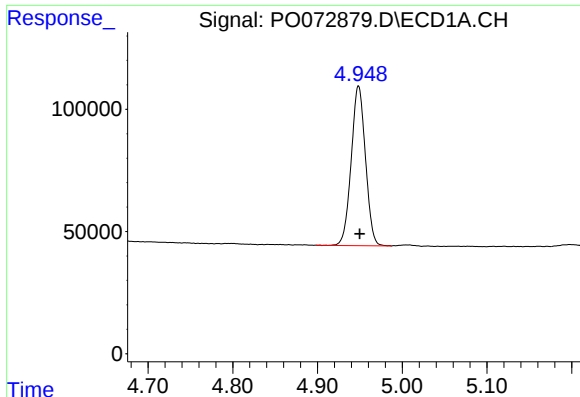

#1 Tetrachloro-m-xylene


R.T.: 4.948 min
Delta R.T.: -0.002 min
Response: 761531
Conc: 16.52 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2020

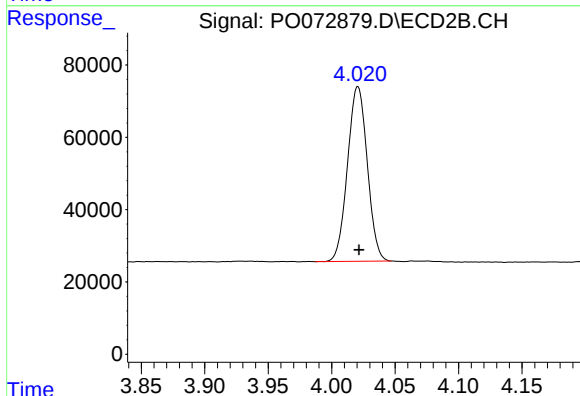


#1 Tetrachloro-m-xylene

R.T.: 4.021 min
Delta R.T.: 0.000 min
Response: 524137
Conc: 14.96 ng/ml

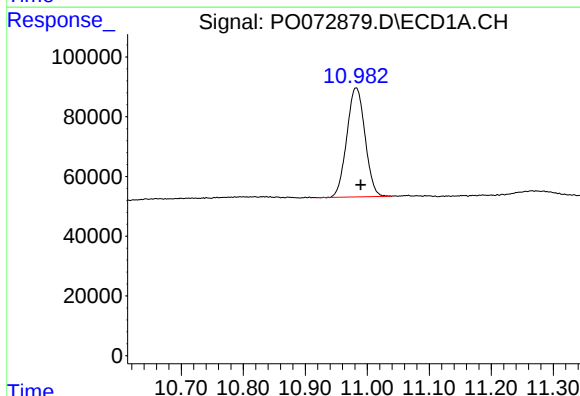

#2 Decachlorobiphenyl

R.T.: 10.982 min
Delta R.T.: -0.008 min
Response: 745133
Conc: 20.17 ng/ml

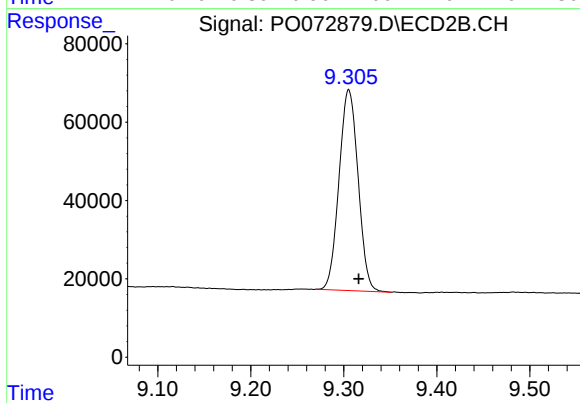

#2 Decachlorobiphenyl

R.T.: 9.305 min
Delta R.T.: -0.011 min
Response: 729186
Conc: 21.87 ng/ml