

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0102721\
 Data File : P0082232.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 27 Oct 2021 13:17
 Operator : AJ\MA
 Sample : M4346-07 10X
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SEC-2021-1A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 28 02:22:42 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Oct 19 04:37:47 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.979	3.973	169157	66872	2.093	2.266
2) SA Decachlor...	11.099	9.300	131110	54310	2.359	2.132
Target Compounds						
26) L6 AR-1254-1	7.231	6.110	662465	436340	276.616	262.010
27) L6 AR-1254-2	7.462	6.270	929596	382163	254.847	255.972
28) L6 AR-1254-3	7.846	6.691	801183	478190	221.393	213.545
29) L6 AR-1254-4	8.145	6.932	507220	281770	188.223	191.849
30) L6 AR-1254-5	8.577	7.364	567310	358289	194.786	173.986



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102721\
Data File : P0082232.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 27 Oct 2021 13:17
Operator : AJ\MA
Sample : M4346-07 10X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampled :
SEC-2021-1A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 28 02:22:42 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101821.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Oct 19 04:37:47 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

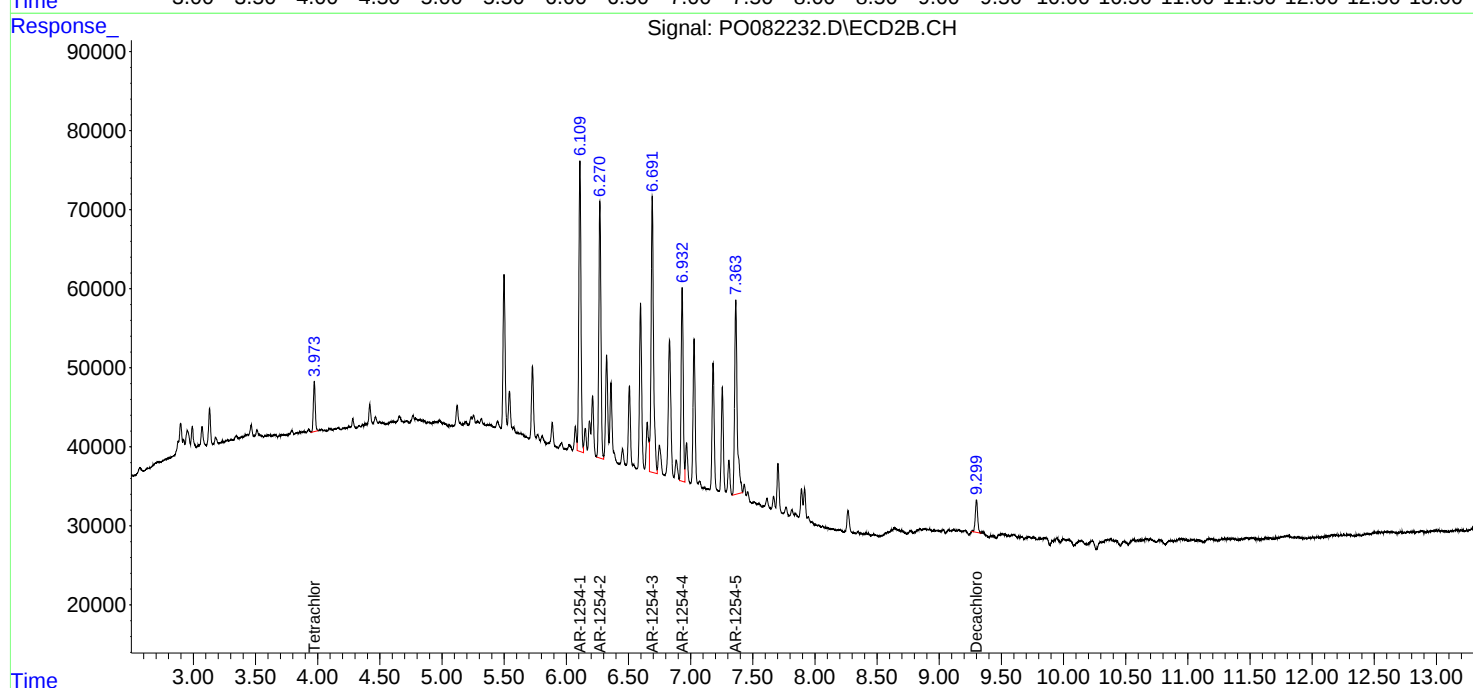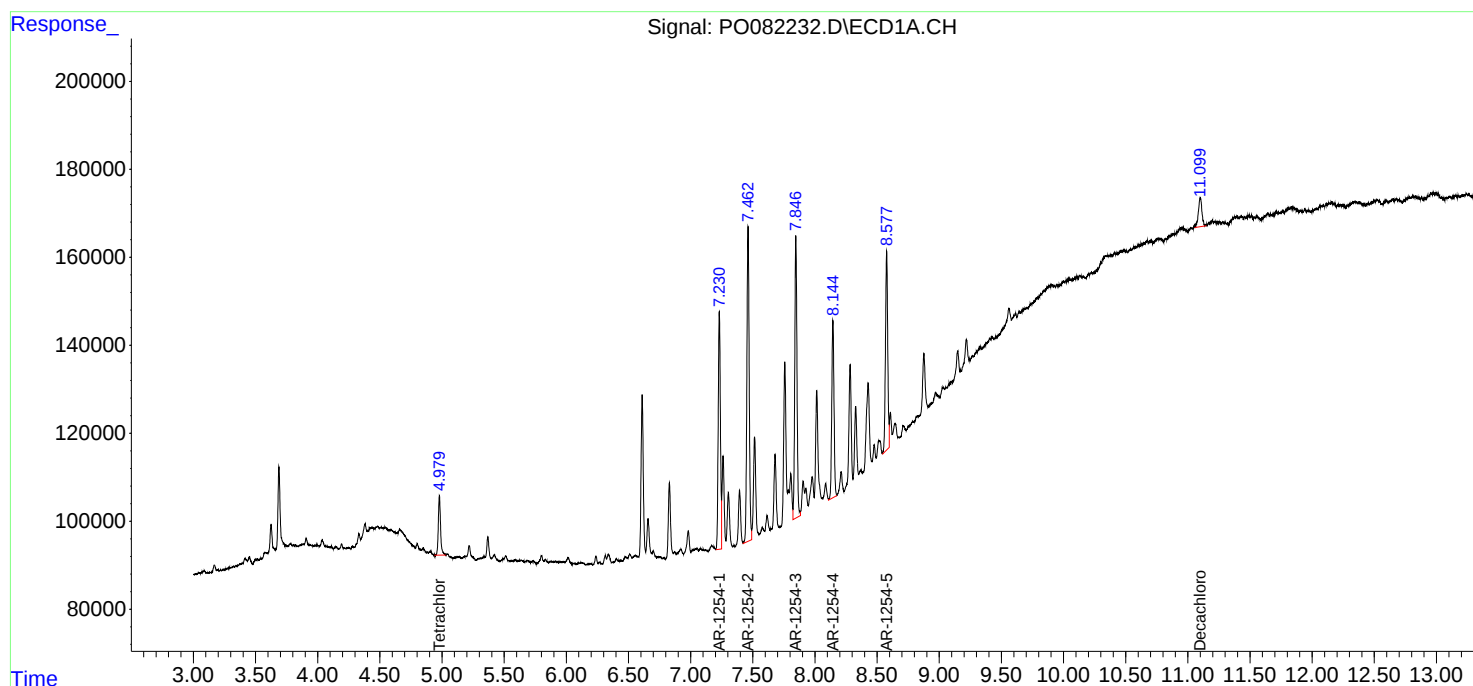


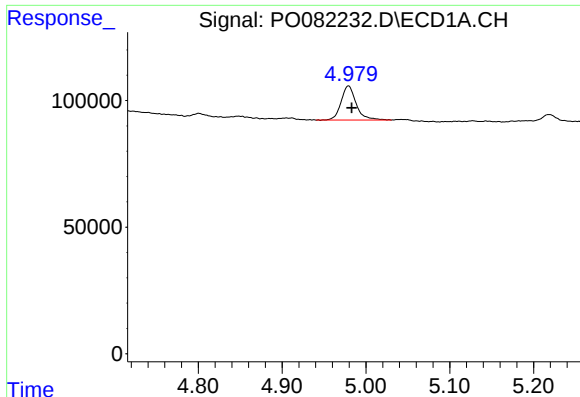

#1 Tetrachloro-m-xylene


R.T.: 4.979 min
Delta R.T.: -0.004 min
Response: 169157
Conc: 2.09 ng/ml

Instrument :
ECD_O
ClientSampleId :
SEC-2021-1A

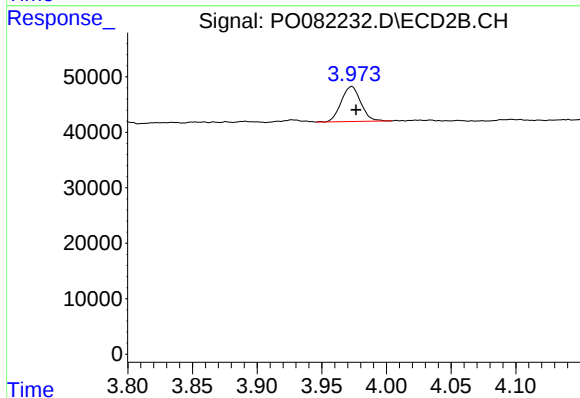


#1 Tetrachloro-m-xylene

R.T.: 3.973 min
Delta R.T.: -0.003 min
Response: 66872
Conc: 2.27 ng/ml

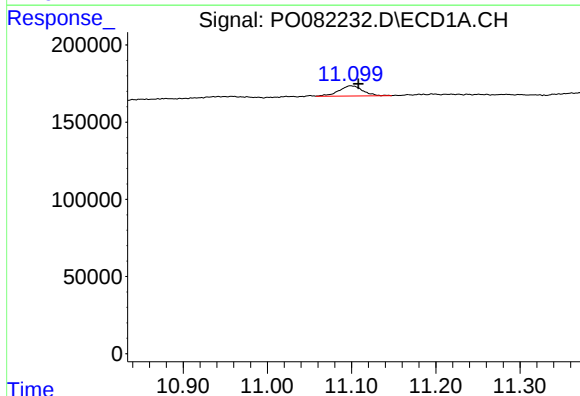


#2 Decachlorobiphenyl

R.T.: 11.099 min
Delta R.T.: -0.009 min
Response: 131110
Conc: 2.36 ng/ml

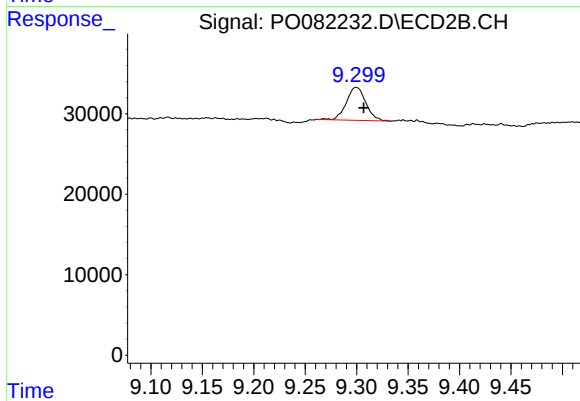

#2 Decachlorobiphenyl


R.T.: 9.300 min
Delta R.T.: -0.007 min
Response: 54310
Conc: 2.13 ng/ml

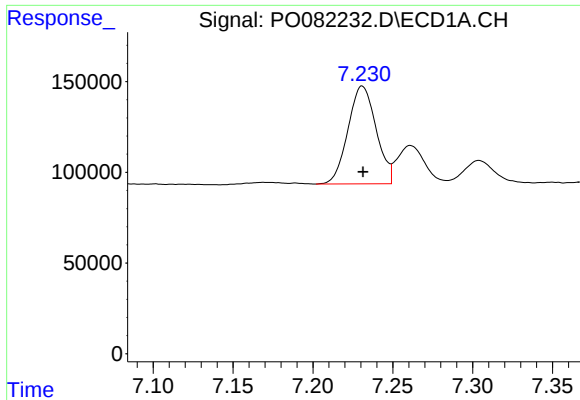

#26 AR-1254-1


R.T.: 7.231 min
Delta R.T.: 0.000 min
Response: 662465
Conc: 276.62 ng/ml

Instrument :
ECD_O
ClientSampleId :
SEC-2021-1A

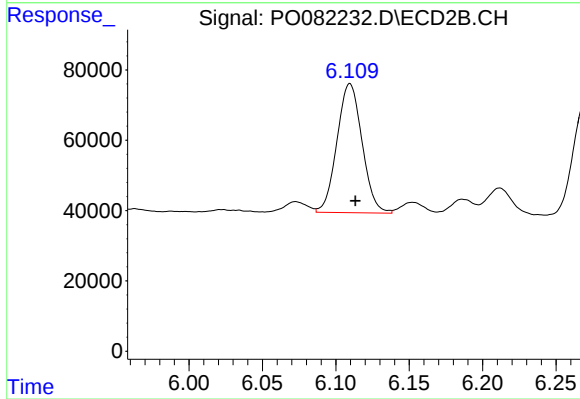


#26 AR-1254-1

R.T.: 6.110 min
Delta R.T.: -0.004 min
Response: 436340
Conc: 262.01 ng/ml

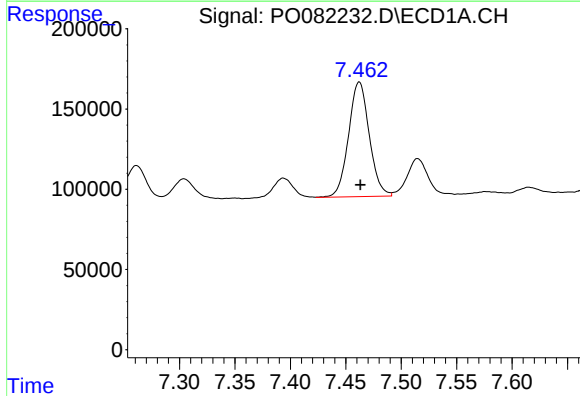


#27 AR-1254-2

R.T.: 7.462 min
Delta R.T.: 0.000 min
Response: 929596
Conc: 254.85 ng/ml

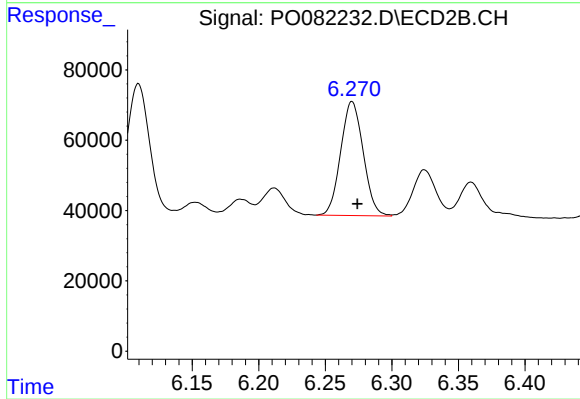

#27 AR-1254-2


R.T.: 6.270 min
Delta R.T.: -0.004 min
Response: 382163
Conc: 255.97 ng/ml

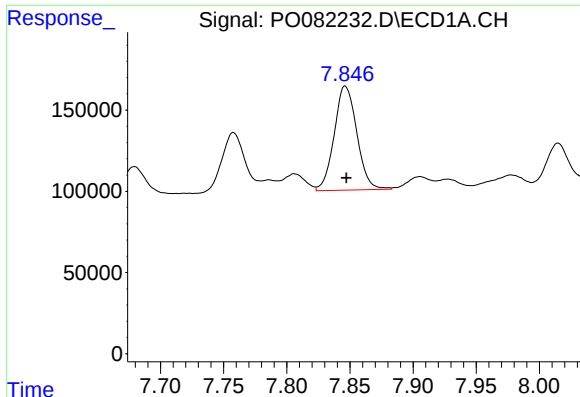

#28 AR-1254-3


R.T.: 7.846 min
Delta R.T.: -0.001 min
Response: 801183
Conc: 221.39 ng/ml

Instrument :
ECD_O
ClientSampleId :
SEC-2021-1A

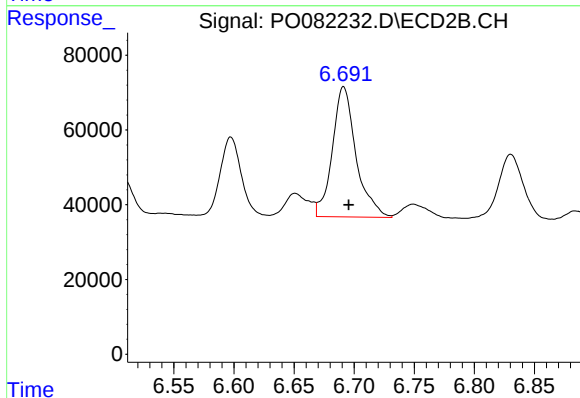


#28 AR-1254-3

R.T.: 6.691 min
Delta R.T.: -0.004 min
Response: 478190
Conc: 213.54 ng/ml

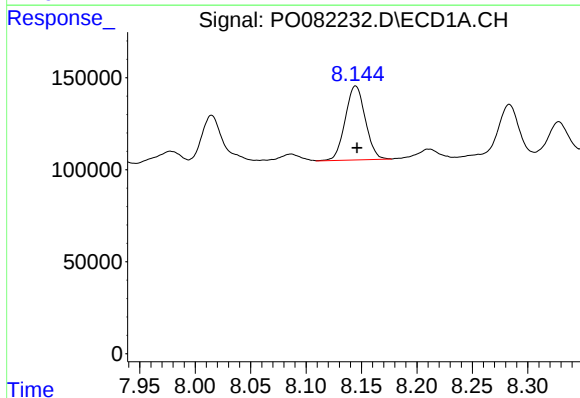


#29 AR-1254-4

R.T.: 8.145 min
Delta R.T.: -0.001 min
Response: 507220
Conc: 188.22 ng/ml

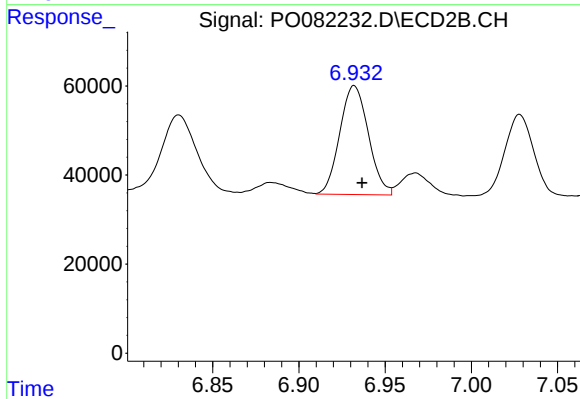

#29 AR-1254-4


R.T.: 6.932 min
Delta R.T.: -0.005 min
Response: 281770
Conc: 191.85 ng/ml

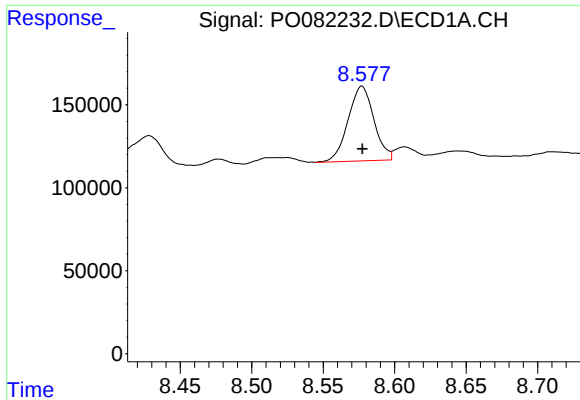

#30 AR-1254-5

R.T.: 8.577 min
Delta R.T.: 0.000 min
Response: 567310
Conc: 194.79 ng/ml

Instrument :
ECD_O
ClientSampleId :
SEC-2021-1A

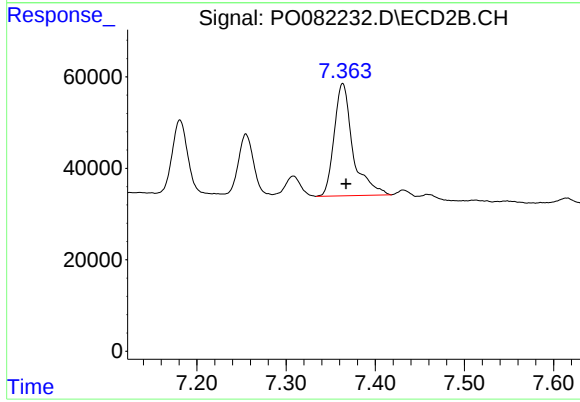

#30 AR-1254-5

R.T.: 7.364 min
Delta R.T.: -0.004 min
Response: 358289
Conc: 173.99 ng/ml