

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0102721\
 Data File : P0082240.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 27 Oct 2021 15:35
 Operator : AJ\MA
 Sample : M4346-10 10X
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SEC-2021-2B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 28 02:28:09 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Oct 19 04:37:47 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.978	3.973	135363	51238	1.675	1.737
2)	SA Decachlor...	11.099	9.299	108379	39444	1.950	1.549
Target Compounds							
26)	L6 AR-1254-1	7.230	6.109	1193946	766332	498.539	460.161
27)	L6 AR-1254-2	7.461	6.270	1691484	665300	463.717	445.616
28)	L6 AR-1254-3	7.846	6.692	1448216	826973	400.190	369.300
29)	L6 AR-1254-4	8.144	6.932	956126	495113	354.807	337.108
30)	L6 AR-1254-5	8.575	7.363	1024844	619585	351.881	300.871



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102721\
Data File : P0082240.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 27 Oct 2021 15:35
Operator : AJ\MA
Sample : M4346-10 10X
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampled :
SEC-2021-2B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 28 02:28:09 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101821.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Oct 19 04:37:47 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

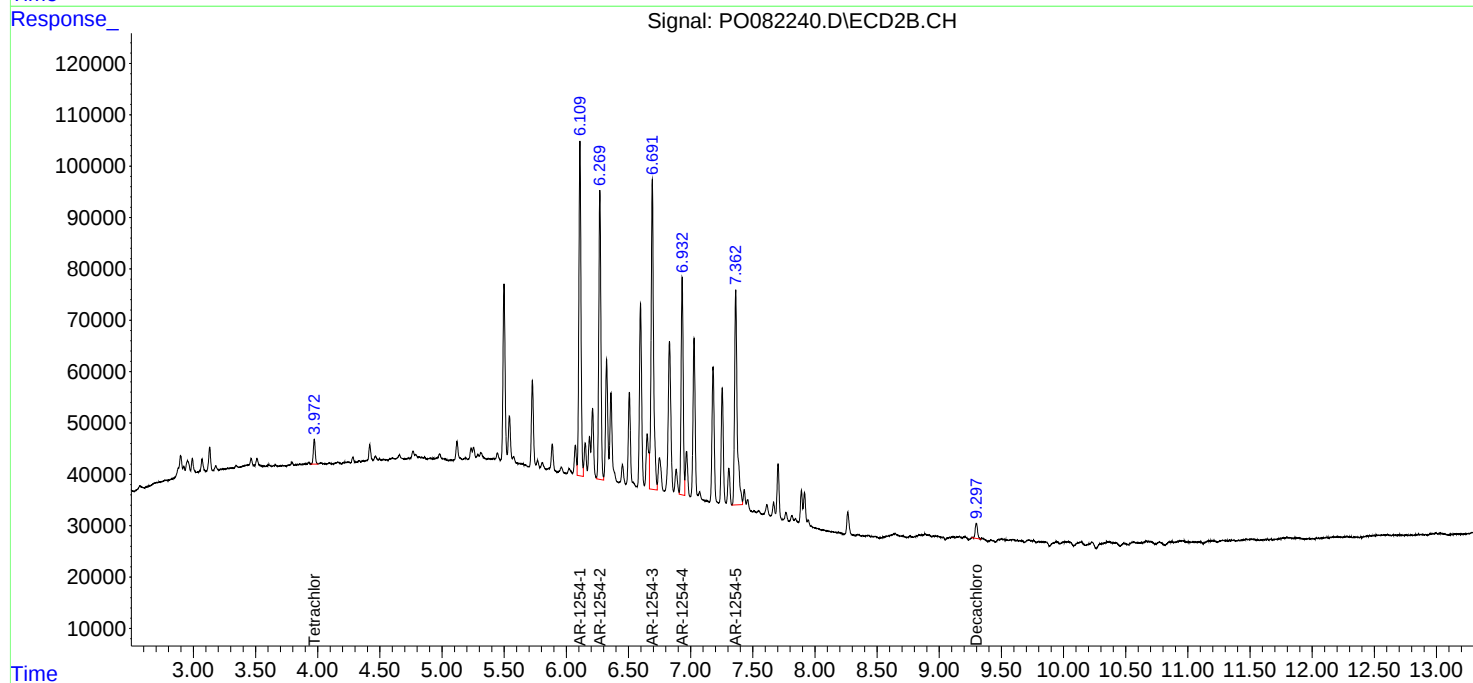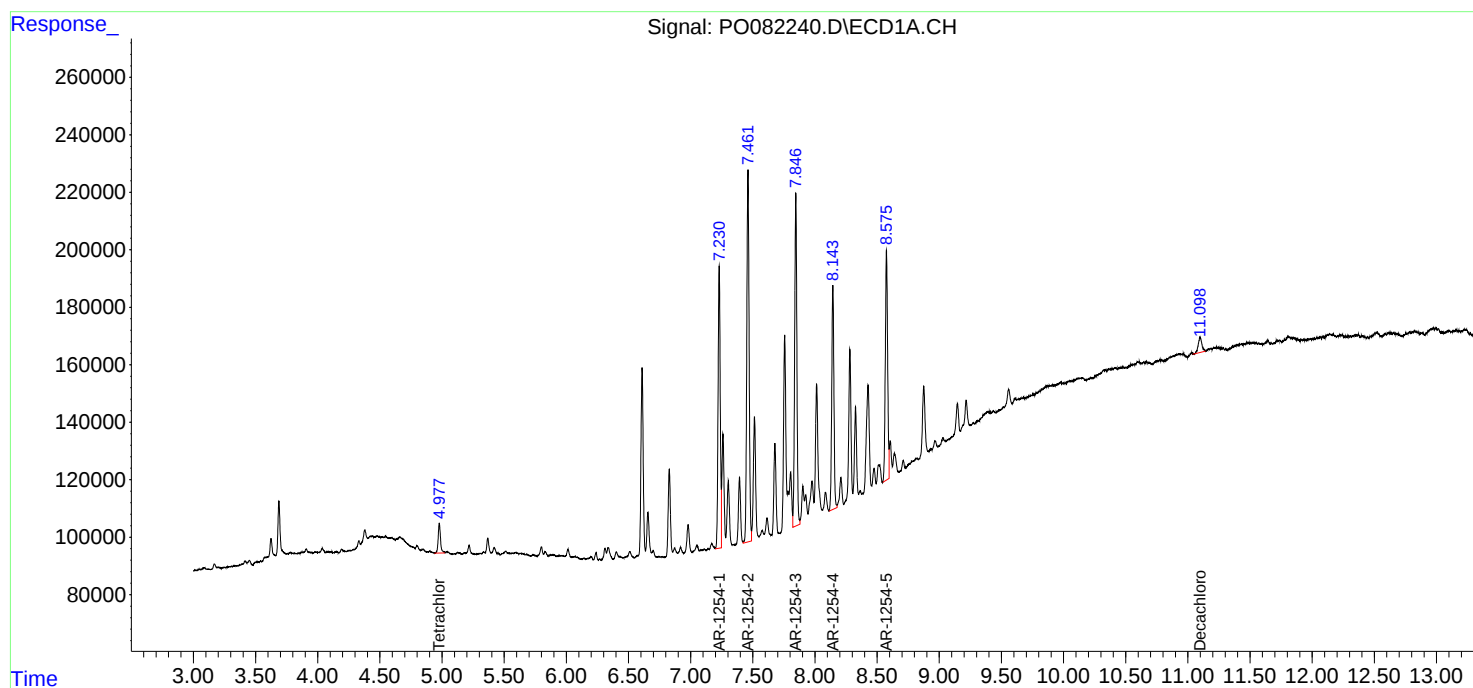


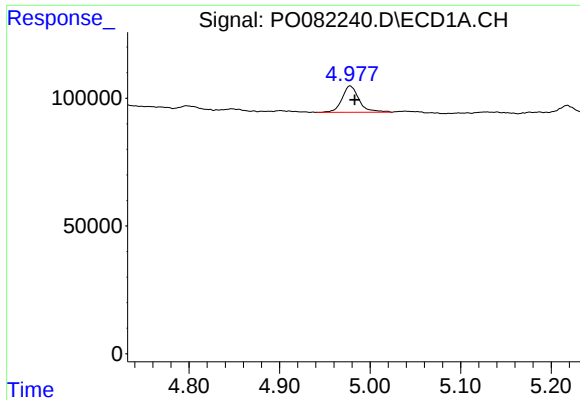

#1 Tetrachloro-m-xylene


R.T.: 4.978 min
Delta R.T.: -0.005 min
Response: 135363
Conc: 1.68 ng/ml

Instrument :
ECD_O
ClientSampleId :
SEC-2021-2B

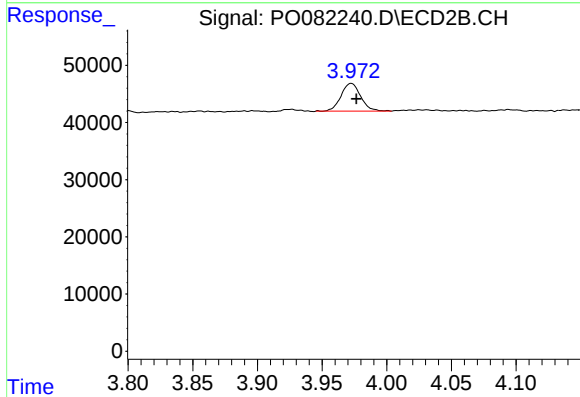


#1 Tetrachloro-m-xylene

R.T.: 3.973 min
Delta R.T.: -0.004 min
Response: 51238
Conc: 1.74 ng/ml

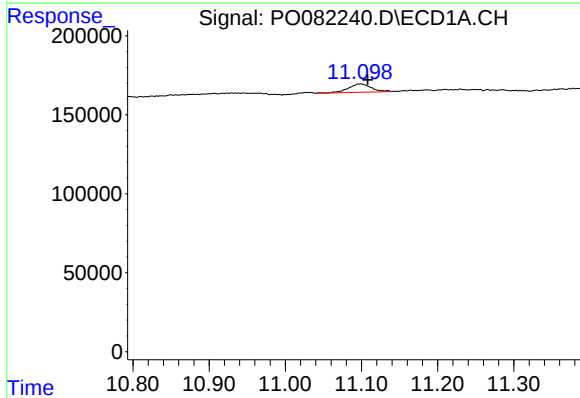


#2 Decachlorobiphenyl

R.T.: 11.099 min
Delta R.T.: -0.009 min
Response: 108379
Conc: 1.95 ng/ml

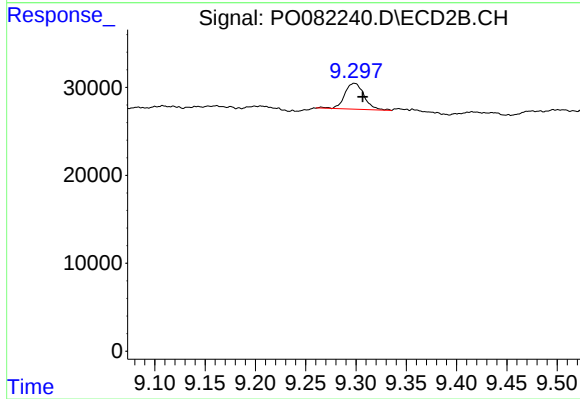

#2 Decachlorobiphenyl


R.T.: 9.299 min
Delta R.T.: -0.008 min
Response: 39444
Conc: 1.55 ng/ml

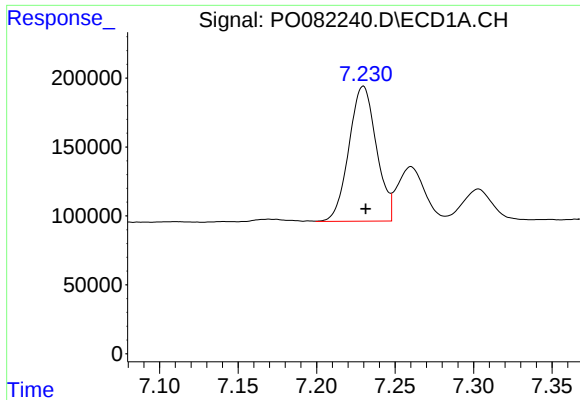

#26 AR-1254-1


R.T.: 7.230 min
Delta R.T.: -0.002 min
Response: 1193946
Conc: 498.54 ng/ml

Instrument :
ECD_O
ClientSampleId :
SEC-2021-2B

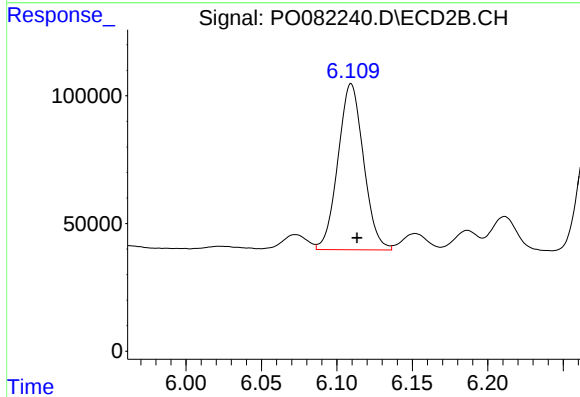


#26 AR-1254-1

R.T.: 6.109 min
Delta R.T.: -0.004 min
Response: 766332
Conc: 460.16 ng/ml

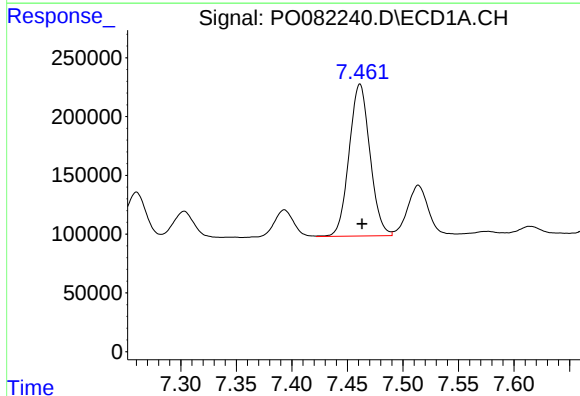


#27 AR-1254-2

R.T.: 7.461 min
Delta R.T.: -0.002 min
Response: 1691484
Conc: 463.72 ng/ml

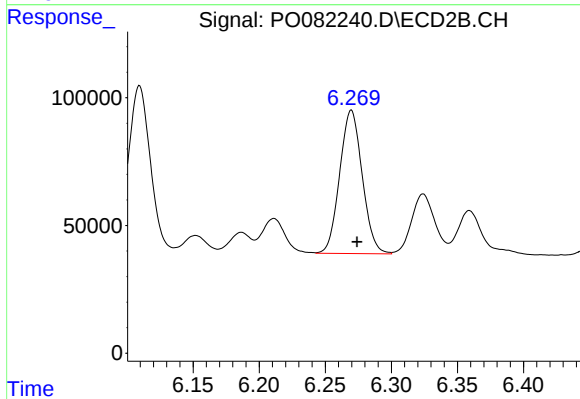

#27 AR-1254-2


R.T.: 6.270 min
Delta R.T.: -0.004 min
Response: 665300
Conc: 445.62 ng/ml

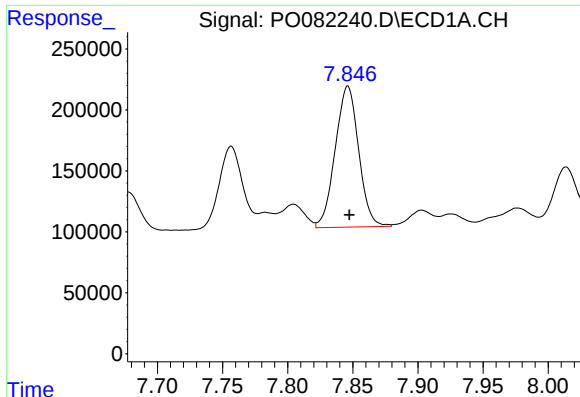

#28 AR-1254-3


R.T.: 7.846 min
Delta R.T.: -0.001 min
Response: 1448216
Conc: 400.19 ng/ml

Instrument :
ECD_O
ClientSampleId :
SEC-2021-2B

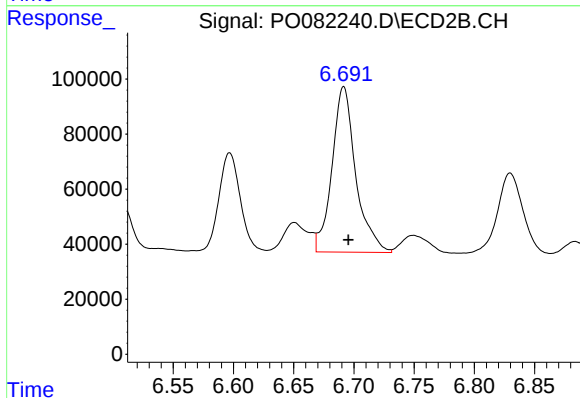


#28 AR-1254-3

R.T.: 6.692 min
Delta R.T.: -0.004 min
Response: 826973
Conc: 369.30 ng/ml

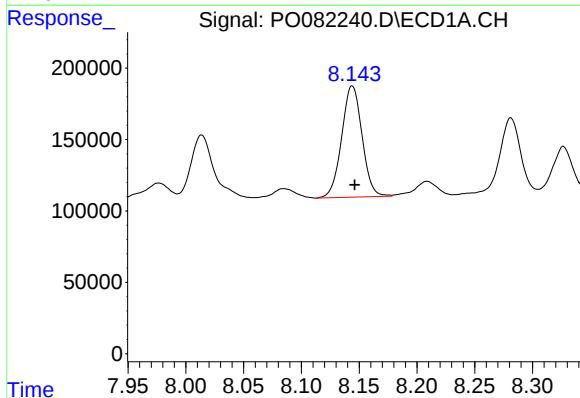


#29 AR-1254-4

R.T.: 8.144 min
Delta R.T.: -0.002 min
Response: 956126
Conc: 354.81 ng/ml

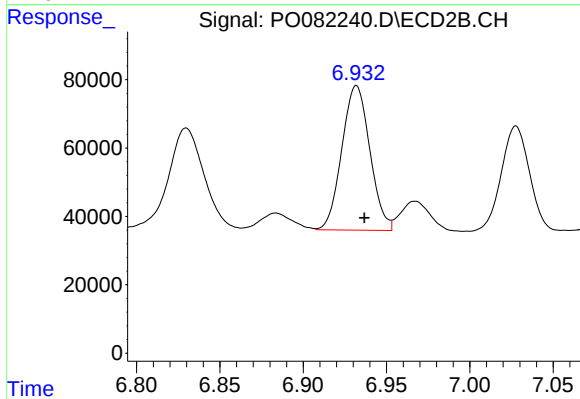

#29 AR-1254-4


R.T.: 6.932 min
Delta R.T.: -0.005 min
Response: 495113
Conc: 337.11 ng/ml

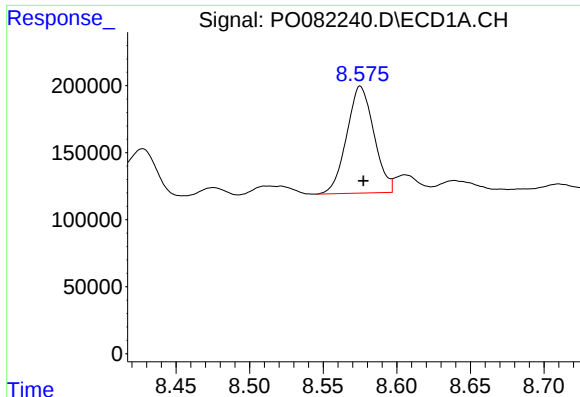

#30 AR-1254-5

R.T.: 8.575 min
Delta R.T.: -0.002 min
Response: 1024844
Conc: 351.88 ng/ml

Instrument :
ECD_O
ClientSampleId :
SEC-2021-2B

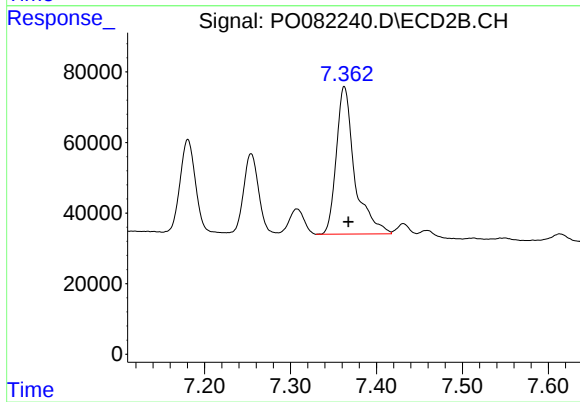

#30 AR-1254-5

R.T.: 7.363 min
Delta R.T.: -0.005 min
Response: 619585
Conc: 300.87 ng/ml