

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102721\
 Data File : PO082247.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 27 Oct 2021 17:35
 Operator : AJ\MA
 Sample : M4346-17 10X
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SEC-2021-6A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 28 02:32:00 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Oct 19 04:37:47 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.978	3.971	109209	44103	1.352	1.495
2) SA Decachlor...	11.100	9.297	72811	37410	1.310	1.469
Target Compounds						
26) L6 AR-1254-1	7.229	6.108	792465	531720	330.898	319.283
27) L6 AR-1254-2	7.461	6.269	1113478	452784	305.258	303.274
28) L6 AR-1254-3	7.845	6.690	947572	564944	261.845	252.286
29) L6 AR-1254-4	8.144	6.931	604817	332381	224.440	226.308
30) L6 AR-1254-5	8.576	7.362	656666	404348	225.467	196.352



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102721\
Data File : P0082247.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 27 Oct 2021 17:35
Operator : AJ\MA
Sample : M4346-17 10X
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampled :
SEC-2021-6A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 28 02:32:00 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101821.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Oct 19 04:37:47 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

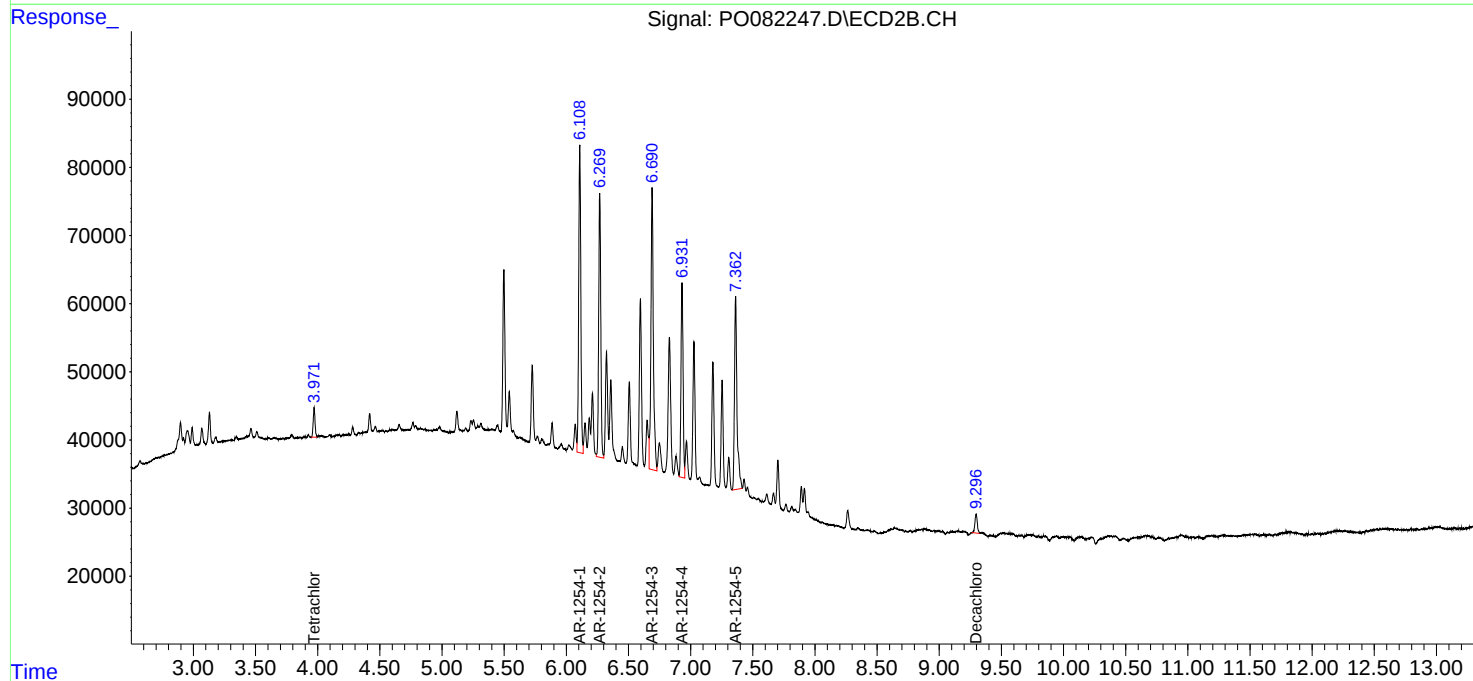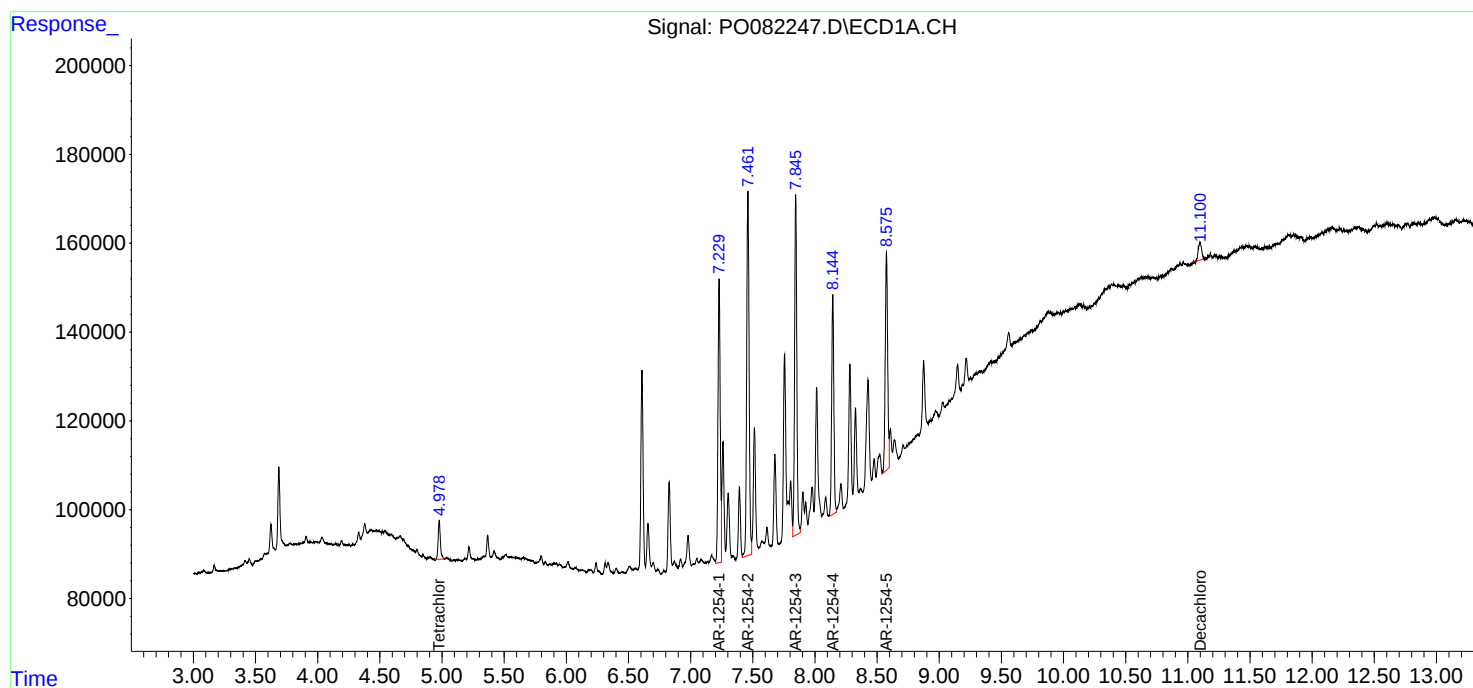


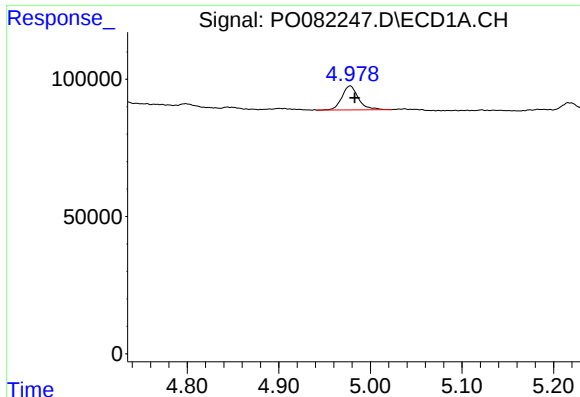

#1 Tetrachloro-m-xylene


R.T.: 4.978 min
Delta R.T.: -0.005 min
Response: 109209
Conc: 1.35 ng/ml

Instrument :
ECD_O
ClientSampleId :
SEC-2021-6A

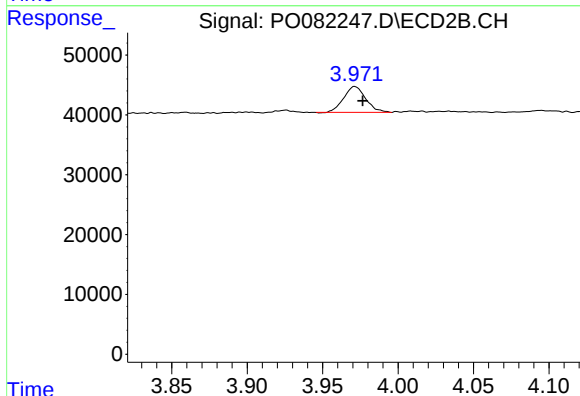


#1 Tetrachloro-m-xylene

R.T.: 3.971 min
Delta R.T.: -0.005 min
Response: 44103
Conc: 1.49 ng/ml

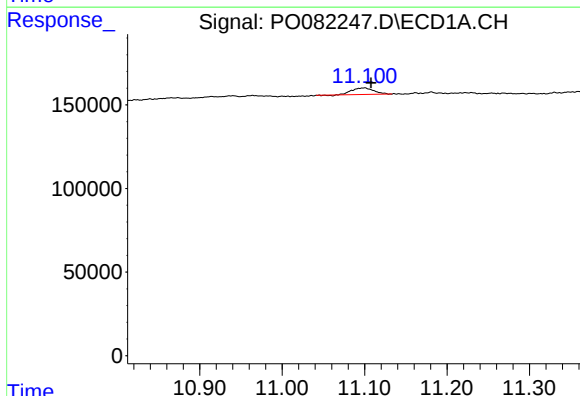


#2 Decachlorobiphenyl

R.T.: 11.100 min
Delta R.T.: -0.008 min
Response: 72811
Conc: 1.31 ng/ml

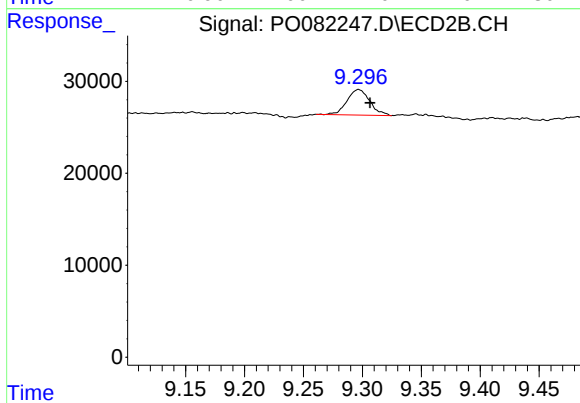

#2 Decachlorobiphenyl


R.T.: 9.297 min
Delta R.T.: -0.010 min
Response: 37410
Conc: 1.47 ng/ml

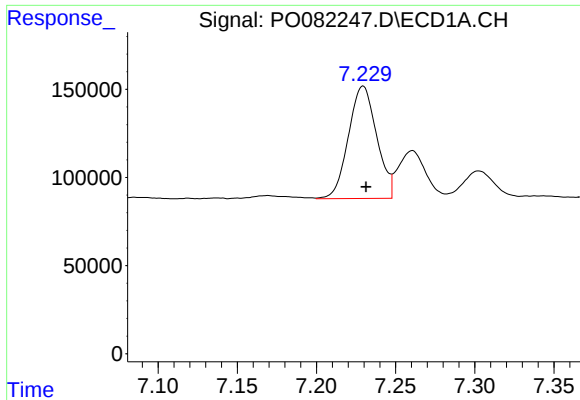

#26 AR-1254-1


R.T.: 7.229 min
Delta R.T.: -0.002 min
Response: 792465
Conc: 330.90 ng/ml

Instrument :
ECD_O
ClientSampleId :
SEC-2021-6A

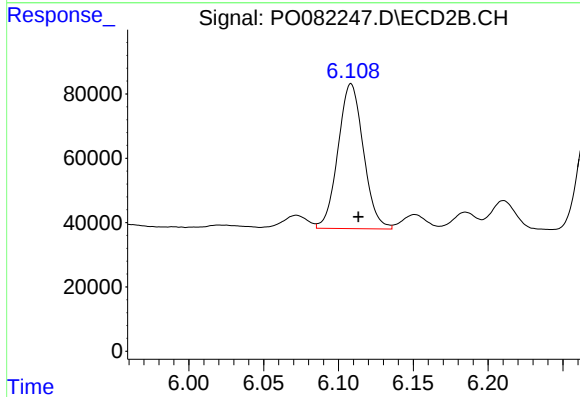


#26 AR-1254-1

R.T.: 6.108 min
Delta R.T.: -0.005 min
Response: 531720
Conc: 319.28 ng/ml

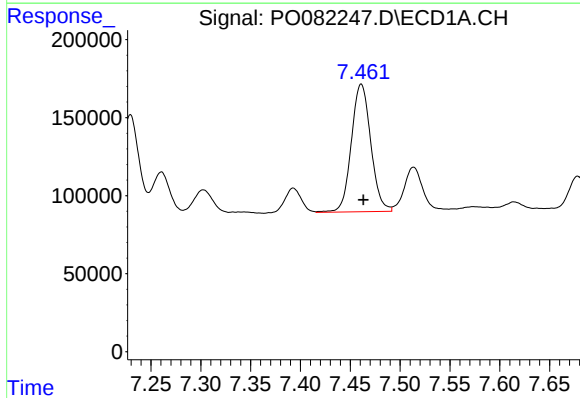


#27 AR-1254-2

R.T.: 7.461 min
Delta R.T.: -0.002 min
Response: 1113478
Conc: 305.26 ng/ml

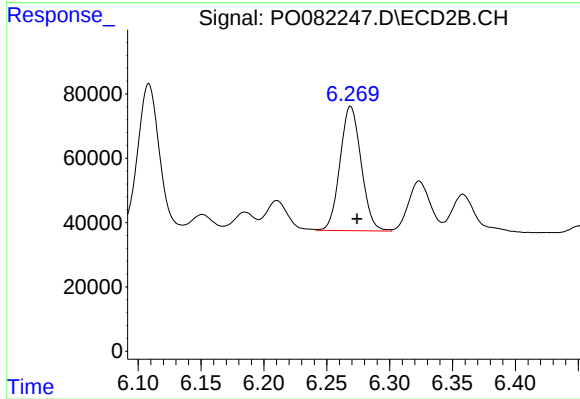

#27 AR-1254-2


R.T.: 6.269 min
Delta R.T.: -0.005 min
Response: 452784
Conc: 303.27 ng/ml

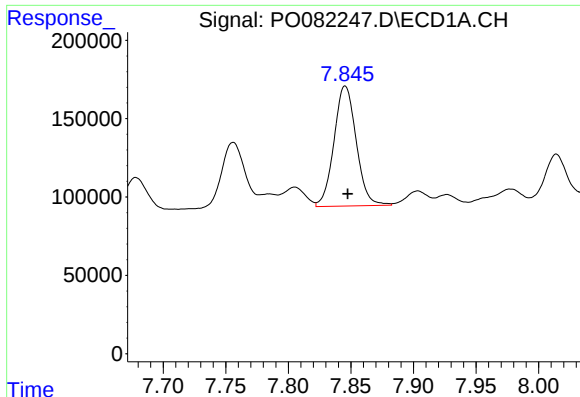

#28 AR-1254-3


R.T.: 7.845 min
Delta R.T.: -0.002 min
Response: 947572
Conc: 261.85 ng/ml

Instrument :
ECD_O
ClientSampleId :
SEC-2021-6A

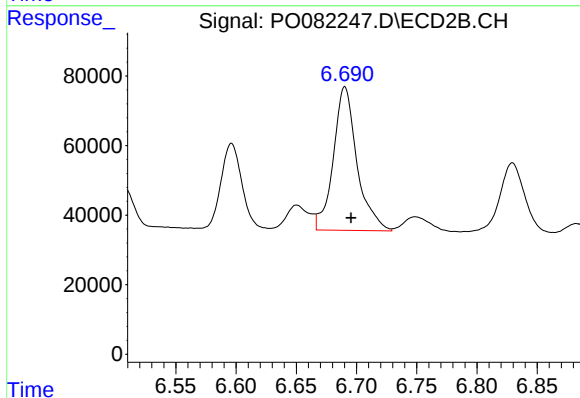


#28 AR-1254-3

R.T.: 6.690 min
Delta R.T.: -0.005 min
Response: 564944
Conc: 252.29 ng/ml

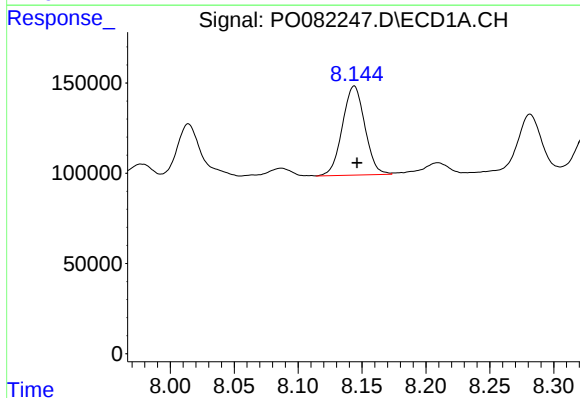


#29 AR-1254-4

R.T.: 8.144 min
Delta R.T.: -0.002 min
Response: 604817
Conc: 224.44 ng/ml

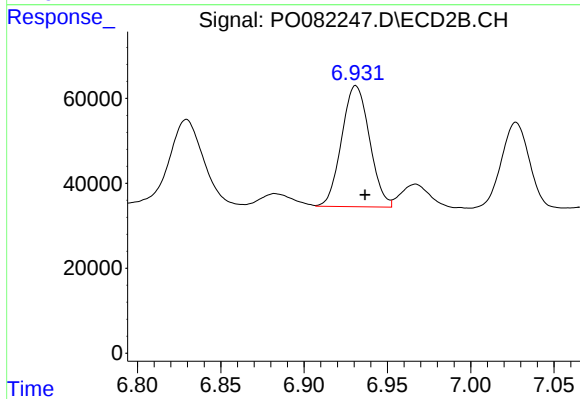

#29 AR-1254-4


R.T.: 6.931 min
Delta R.T.: -0.006 min
Response: 332381
Conc: 226.31 ng/ml

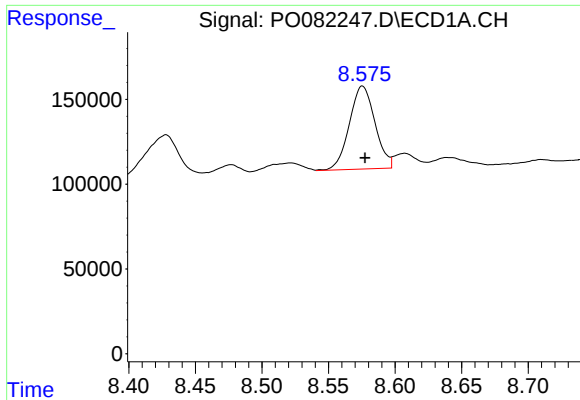

#30 AR-1254-5

R.T.: 8.576 min
Delta R.T.: -0.002 min
Response: 656666
Conc: 225.47 ng/ml

Instrument :
ECD_O
ClientSampleId :
SEC-2021-6A

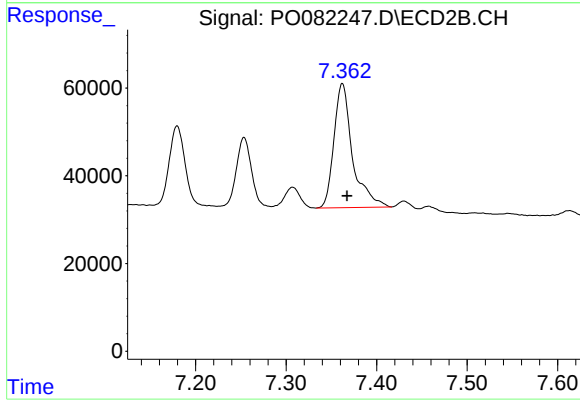

#30 AR-1254-5

R.T.: 7.362 min
Delta R.T.: -0.005 min
Response: 404348
Conc: 196.35 ng/ml