

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0102721\
 Data File : P0082253.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 27 Oct 2021 19:54
 Operator : AJ\MA
 Sample : M4346-18 10X
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SEC-2021-6B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 28 02:36:08 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Oct 19 04:37:47 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.980	3.973	125532	48632	1.554	1.648
2) SA Decachlor...	11.100	9.299	98306	33995	1.769	1.335
Target Compounds						
26) L6 AR-1254-1	7.230	6.110	1937420	1204823	808.980	723.462
27) L6 AR-1254-2	7.463	6.271	2709720	1002370	742.865	671.385
28) L6 AR-1254-3	7.847	6.692	2335451	1281938	645.362	572.474
29) L6 AR-1254-4	8.145	6.932	1519635	762824	563.918	519.384
30) L6 AR-1254-5	8.577	7.364	1597500	955487	548.504	463.986


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102721\
Data File : P0082253.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 27 Oct 2021 19:54
Operator : AJ\MA
Sample : M4346-18 10X
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampled :
SEC-2021-6B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 28 02:36:08 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101821.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Oct 19 04:37:47 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

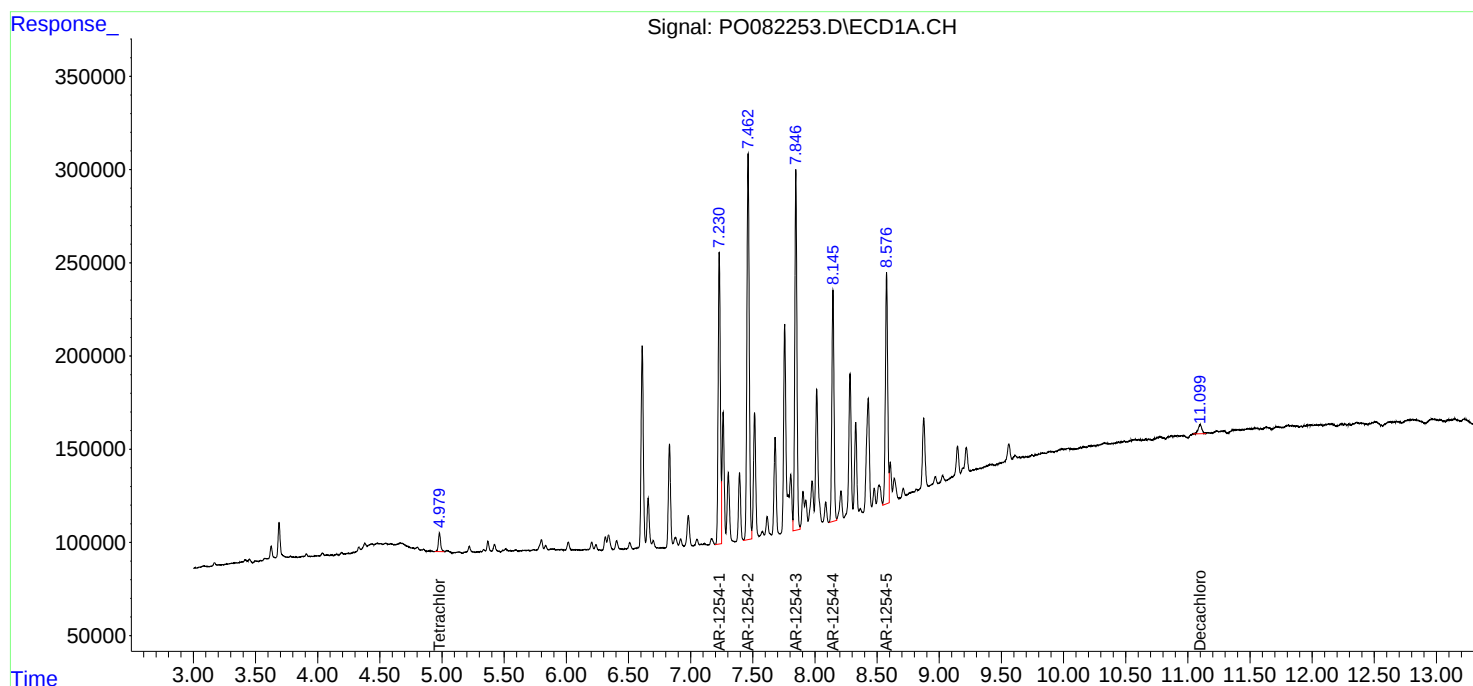


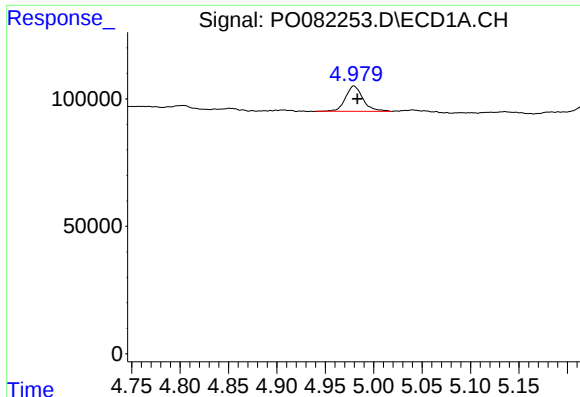

#1 Tetrachloro-m-xylene


R.T.: 4.980 min
Delta R.T.: -0.003 min
Response: 125532
Conc: 1.55 ng/ml

Instrument :
ECD_O
ClientSampleId :
SEC-2021-6B

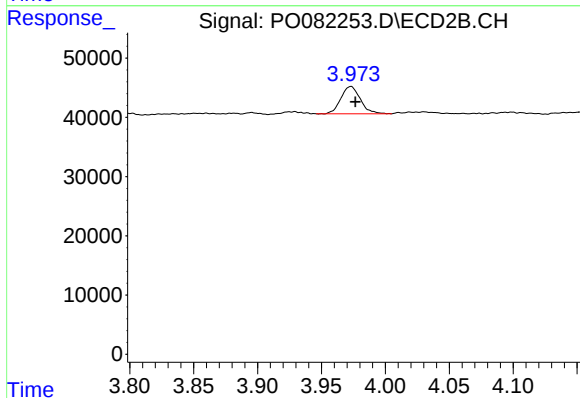


#1 Tetrachloro-m-xylene

R.T.: 3.973 min
Delta R.T.: -0.003 min
Response: 48632
Conc: 1.65 ng/ml

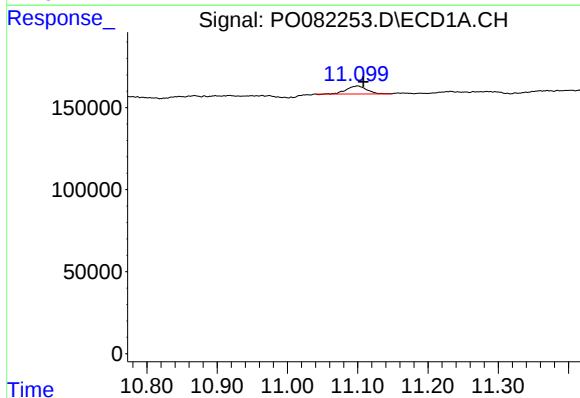


#2 Decachlorobiphenyl

R.T.: 11.100 min
Delta R.T.: -0.008 min
Response: 98306
Conc: 1.77 ng/ml

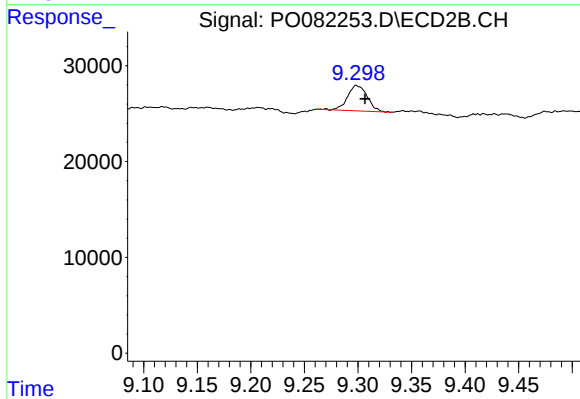

#2 Decachlorobiphenyl


R.T.: 9.299 min
Delta R.T.: -0.008 min
Response: 33995
Conc: 1.33 ng/ml

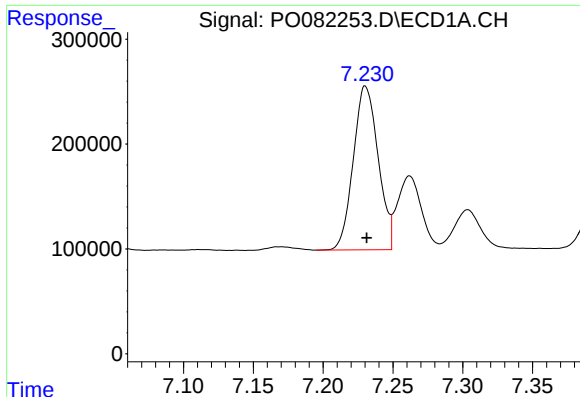

#26 AR-1254-1


R.T.: 7.230 min
Delta R.T.: -0.001 min
Response: 1937420
Conc: 808.98 ng/ml

Instrument :
ECD_O
ClientSampleId :
SEC-2021-6B

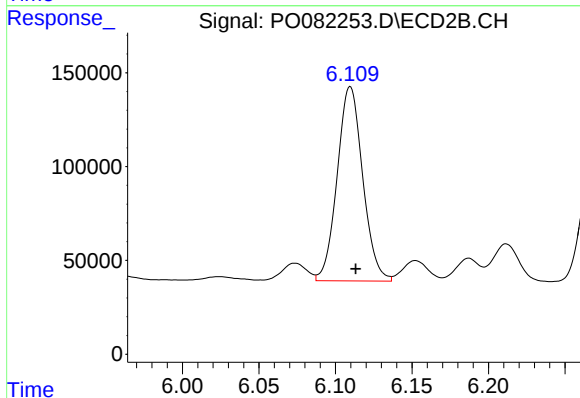


#26 AR-1254-1

R.T.: 6.110 min
Delta R.T.: -0.004 min
Response: 1204823
Conc: 723.46 ng/ml

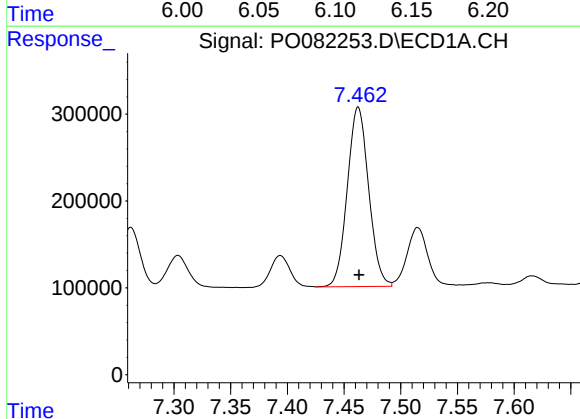


#27 AR-1254-2

R.T.: 7.463 min
Delta R.T.: 0.000 min
Response: 2709720
Conc: 742.86 ng/ml

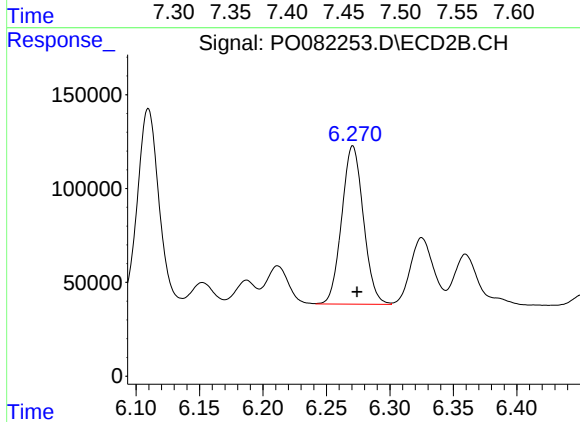

#27 AR-1254-2


R.T.: 6.271 min
Delta R.T.: -0.003 min
Response: 1002370
Conc: 671.39 ng/ml

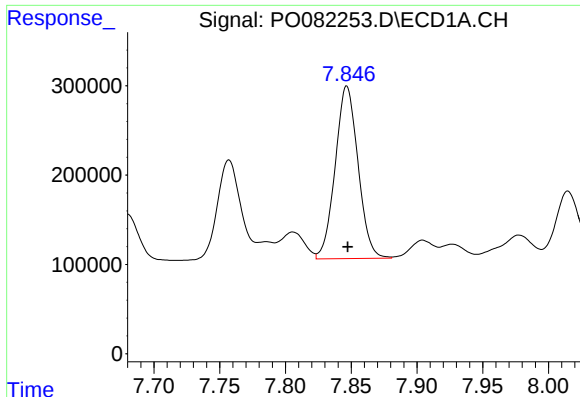

#28 AR-1254-3


R.T.: 7.847 min
Delta R.T.: 0.000 min
Response: 2335451
Conc: 645.36 ng/ml

Instrument :
ECD_O
ClientSampleId :
SEC-2021-6B

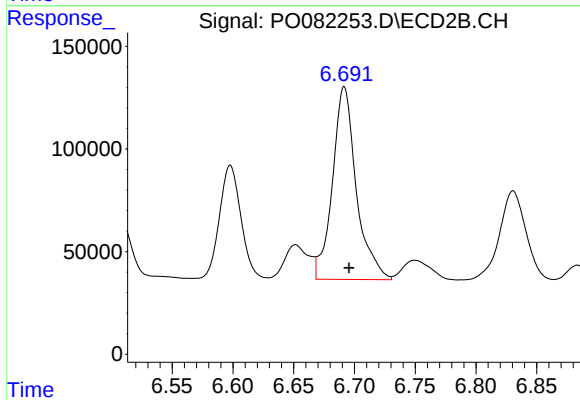


#28 AR-1254-3

R.T.: 6.692 min
Delta R.T.: -0.004 min
Response: 1281938
Conc: 572.47 ng/ml

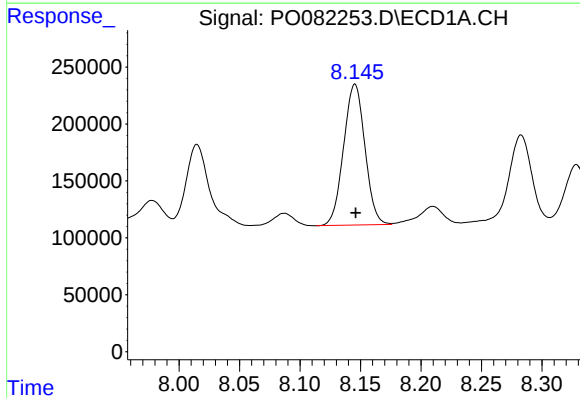


#29 AR-1254-4

R.T.: 8.145 min
Delta R.T.: 0.000 min
Response: 1519635
Conc: 563.92 ng/ml

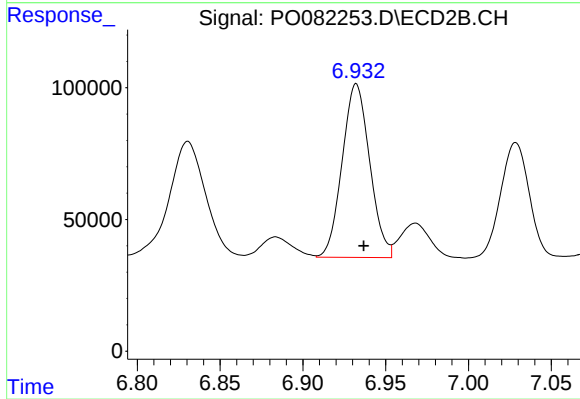

#29 AR-1254-4


R.T.: 6.932 min
Delta R.T.: -0.004 min
Response: 762824
Conc: 519.38 ng/ml

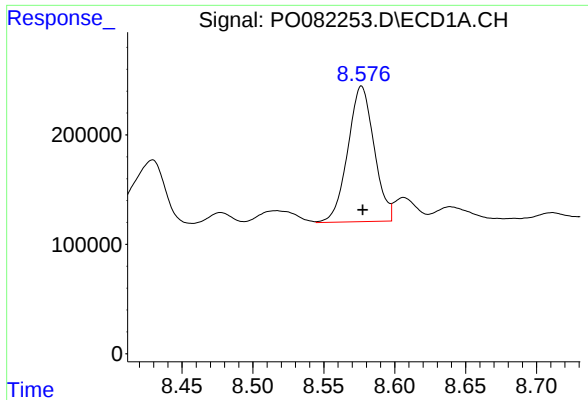

#30 AR-1254-5

R.T.: 8.577 min
Delta R.T.: 0.000 min
Response: 1597500
Conc: 548.50 ng/ml

Instrument :
ECD_O
ClientSampleId :
SEC-2021-6B

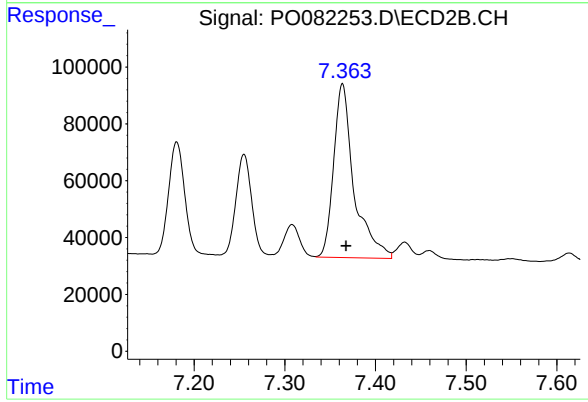

#30 AR-1254-5

R.T.: 7.364 min
Delta R.T.: -0.004 min
Response: 955487
Conc: 463.99 ng/ml