

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102723\
 Data File : PO099077.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Oct 2023 05:50
 Operator : YP/AJ
 Sample : 05111-06 10X
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 BC-259215-2-2

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 28 06:44:24 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102523.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 25 06:04:36 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.474	3.628	3547332	1188381	1.795	1.651
2)	SA Decachlor...	10.277	8.624	2647687	1237238	2.337	2.306

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102723\
Data File : PO099077.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Oct 2023 05:50
Operator : YP/AJ
Sample : 05111-06 10X
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
BC-259215-2-2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 28 06:44:24 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102523.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 25 06:04:36 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

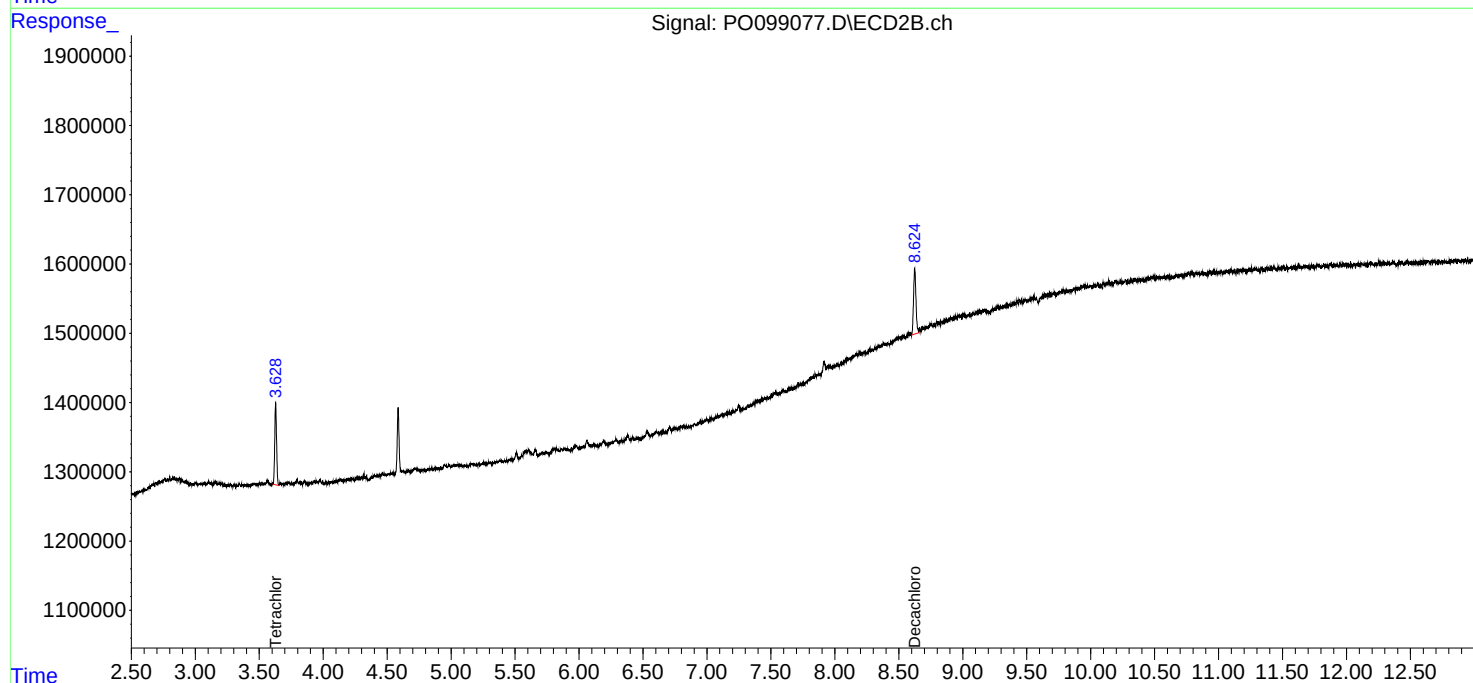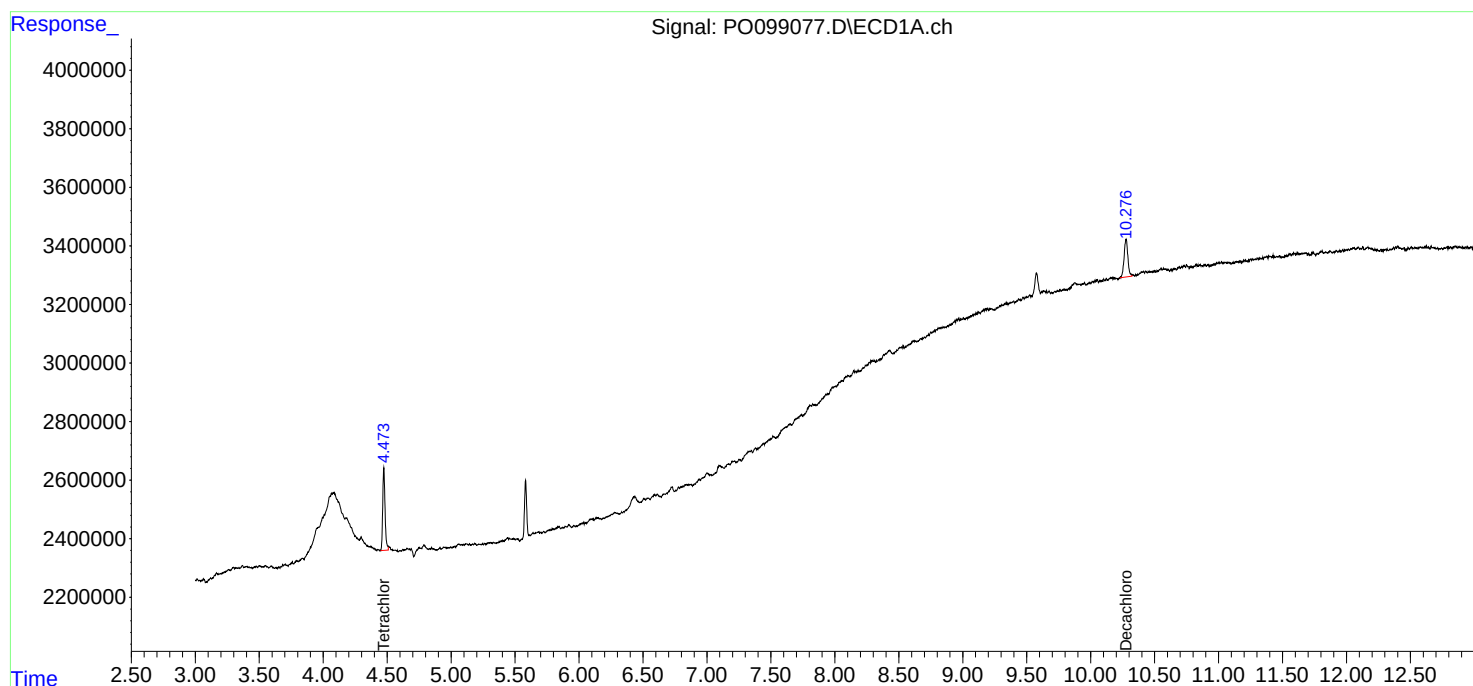


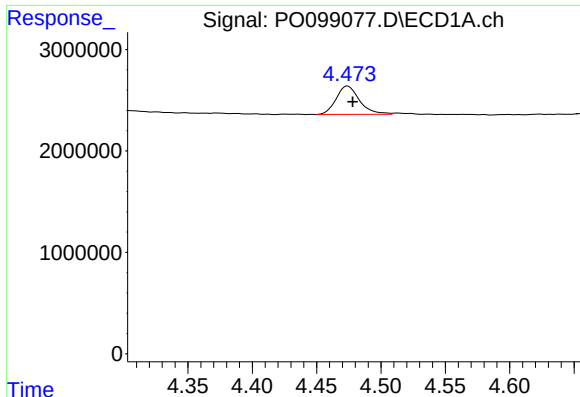

#1 Tetrachloro-m-xylene


R.T.: 4.474 min
Delta R.T.: -0.004 min
Response: 3547332
Conc: 1.80 ng/ml

Instrument :
ECD_O
ClientSampleId :
BC-259215-2-2

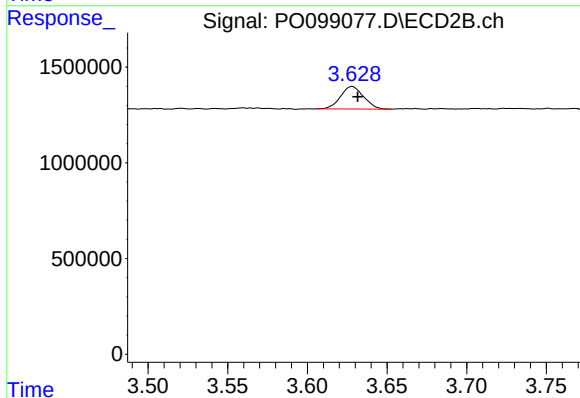


#1 Tetrachloro-m-xylene

R.T.: 3.628 min
Delta R.T.: -0.004 min
Response: 1188381
Conc: 1.65 ng/ml

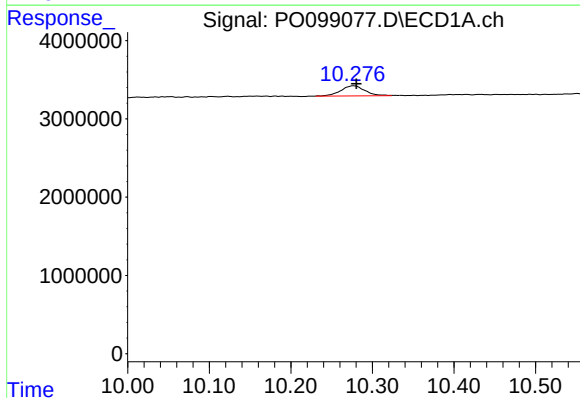

#2 Decachlorobiphenyl

R.T.: 10.277 min
Delta R.T.: -0.003 min
Response: 2647687
Conc: 2.34 ng/ml

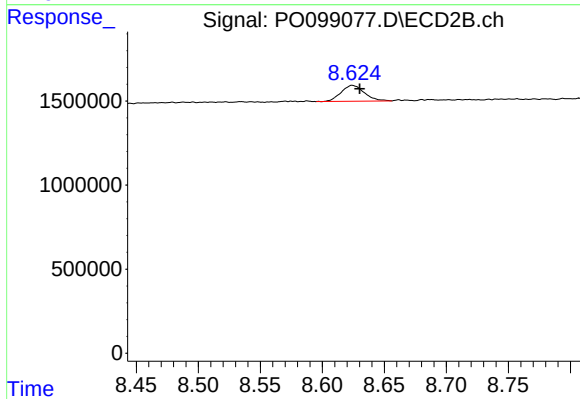

#2 Decachlorobiphenyl

R.T.: 8.624 min
Delta R.T.: -0.006 min
Response: 1237238
Conc: 2.31 ng/ml