

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0102725\
 Data File : P0114685.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Oct 2025 17:51
 Operator : YP/AJ
 Sample : Q3459-16 10X
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 BC283118LOK-END-3-2

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/28/2025
 Supervised By :mohammad ahmed 10/29/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 28 01:16:32 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0100925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Oct 21 02:40:25 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.348	3.653	7144102	6113722	1.316m	1.528
2) SA Decachlor...	9.929	8.647	6306003	6556799	1.732	1.967

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102725\
Data File : PO114685.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Oct 2025 17:51
Operator : YP/AJ
Sample : Q3459-16 10X
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
BC283118LOK-END-3-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/28/2025
Supervised By :mohammad ahmed 10/29/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 28 01:16:32 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100925.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Oct 21 02:40:25 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

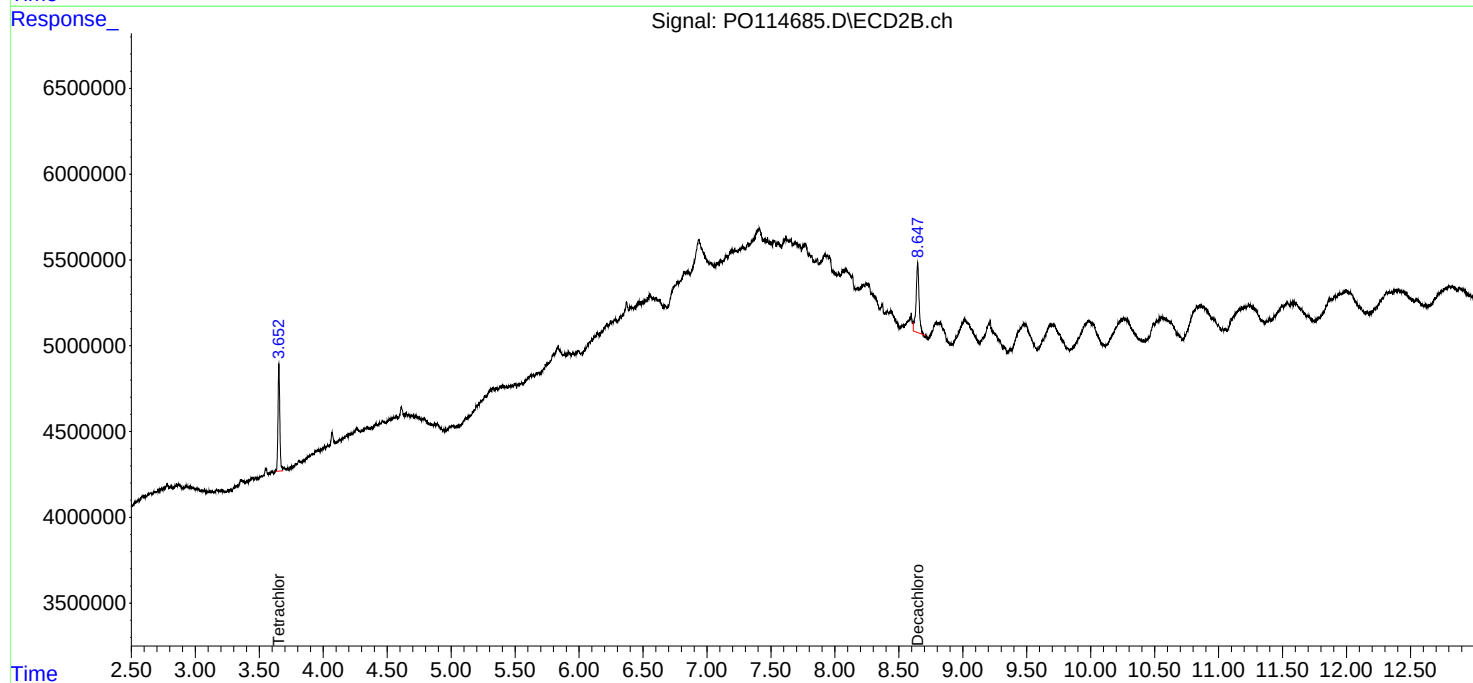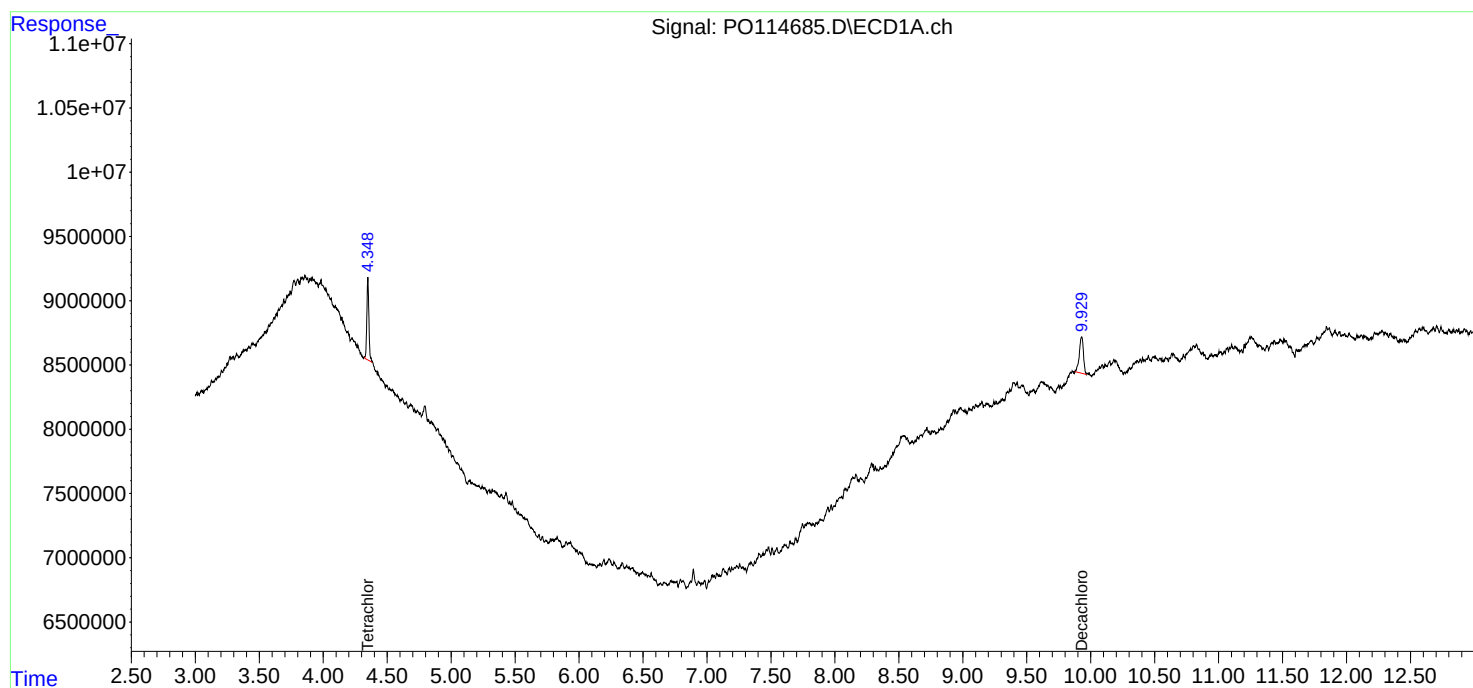

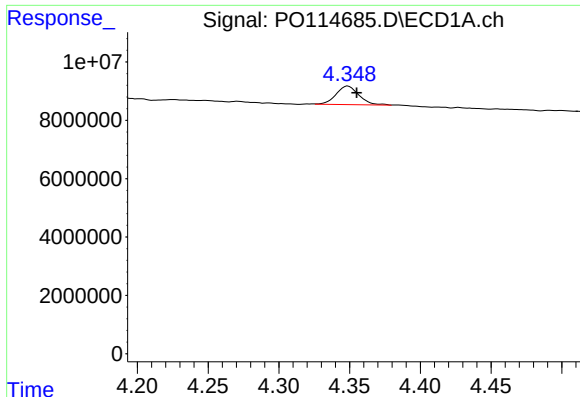


#1 Tetrachloro-m-xylene

R.T.: 4.348 min
Delta R.T.: -0.007 min
Response: 7144102
Conc: 1.32 ng/ml

Instrument :
ECD_O
ClientSampleId :
BC283118LOK-END-3-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/28/2025
Supervised By :mohammad ahmed 10/29/2025

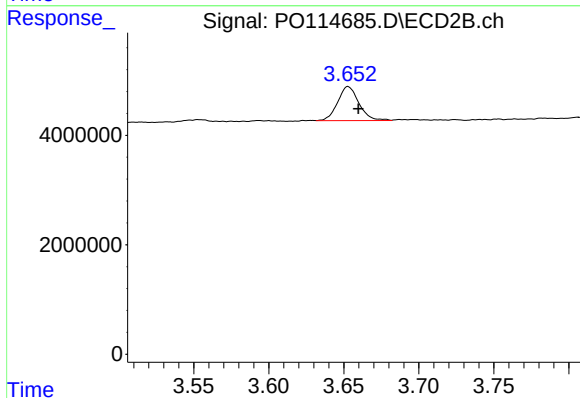


#1 Tetrachloro-m-xylene

R.T.: 3.653 min
Delta R.T.: -0.007 min
Response: 6113722
Conc: 1.53 ng/ml

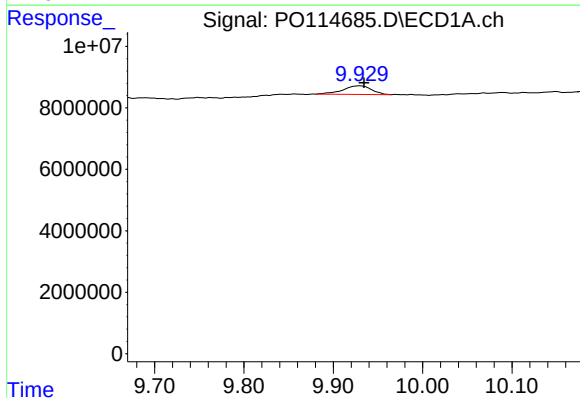

#2 Decachlorobiphenyl

R.T.: 9.929 min
Delta R.T.: -0.005 min
Response: 6306003
Conc: 1.73 ng/ml

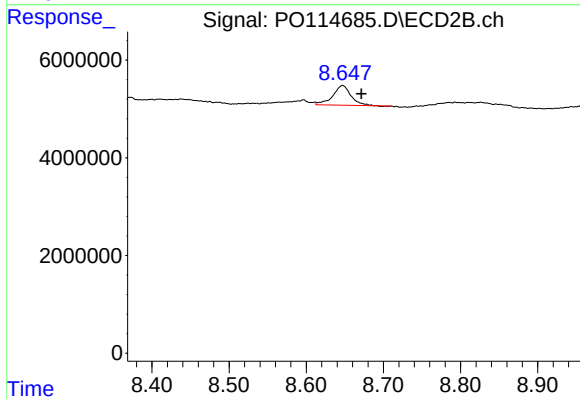

#2 Decachlorobiphenyl

R.T.: 8.647 min
Delta R.T.: -0.024 min
Response: 6556799
Conc: 1.97 ng/ml