

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102818\
 Data File : P0050685.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 27 Oct 2018 18:22
 Operator : SM/SJ
 Sample : J5696-10
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 EB-2018.10.25-SED

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 29 02:12:09 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101818.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Oct 19 02:02:26 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.361	3.353	8394853	4559509	28.134	23.192
2) SA Decachlor...	10.025	8.103	4447936	3881860	20.499	20.309

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102818\
Data File : P0050685.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 27 Oct 2018 18:22
Operator : SM/SJ
Sample : J5696-10
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
EB-2018.10.25-SED

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 29 02:12:09 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101818.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Oct 19 02:02:26 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

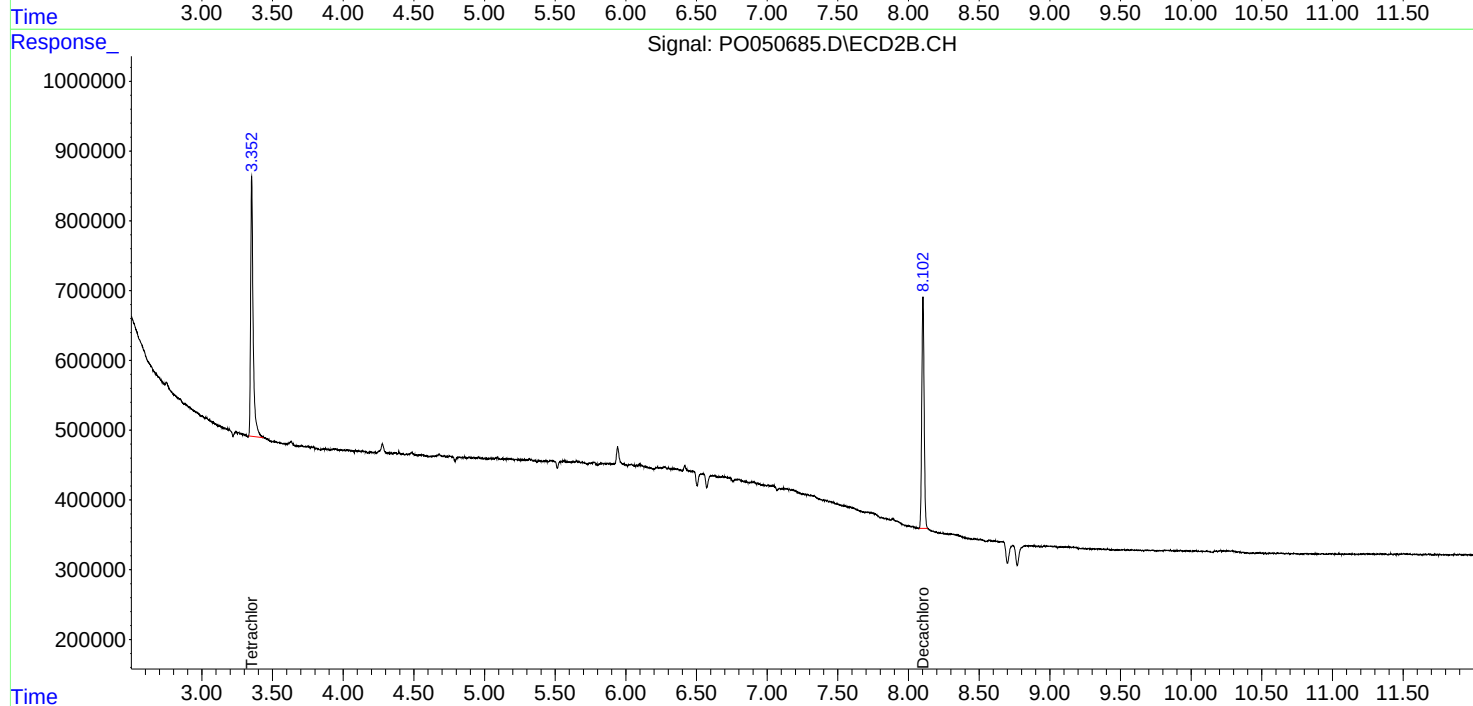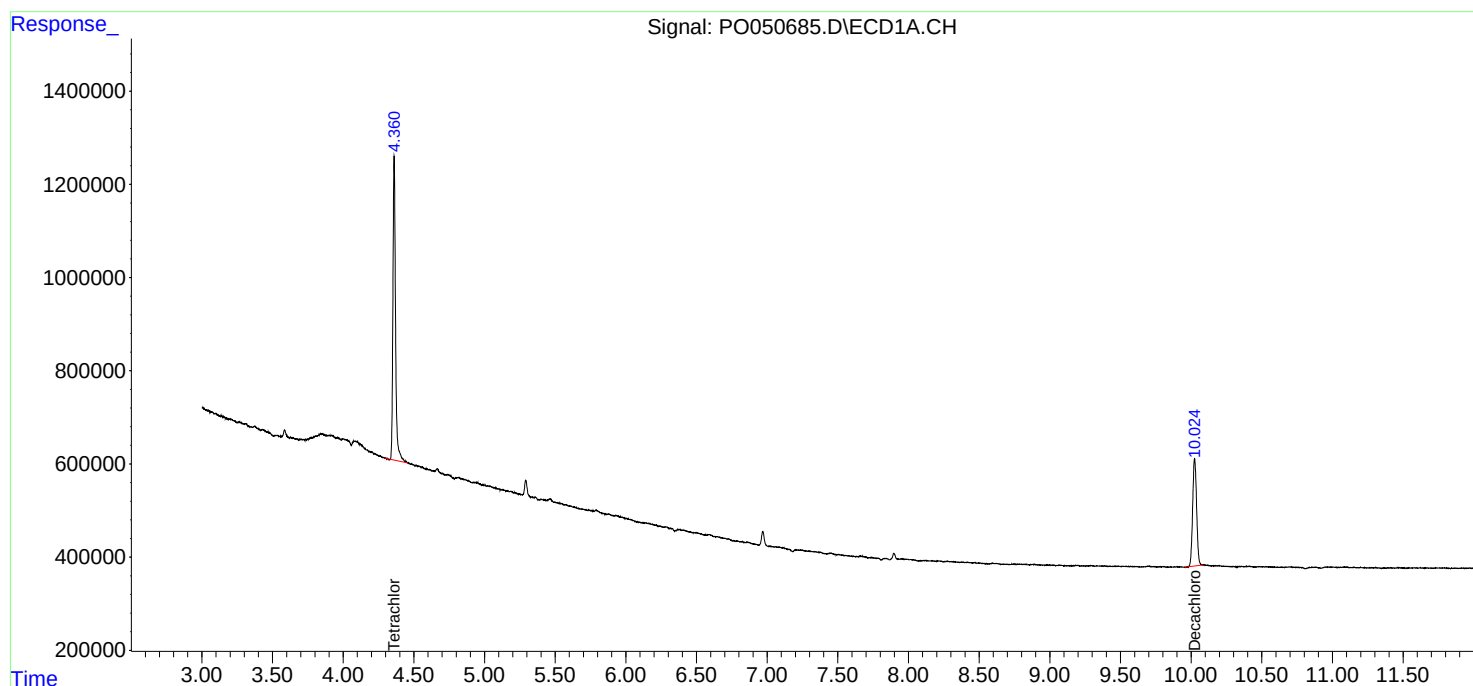


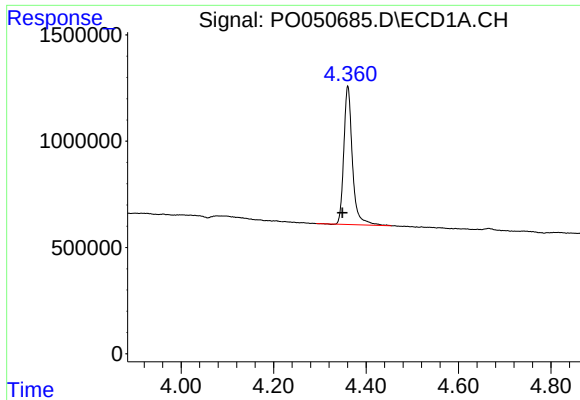

#1 Tetrachloro-m-xylene


R.T.: 4.361 min
Delta R.T.: 0.012 min
Response: 8394853
Conc: 28.13 ng/ml

Instrument :
ECD_O
ClientSampleId :
EB-2018.10.25-SED

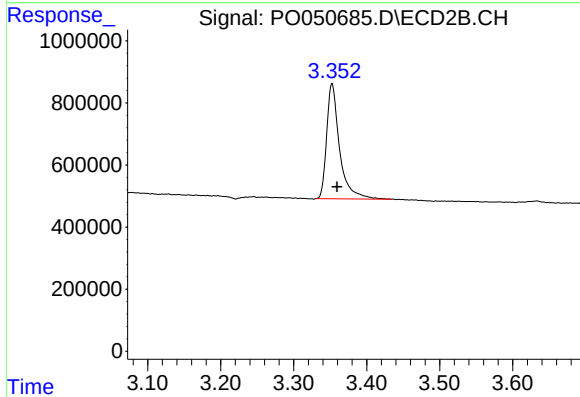


#1 Tetrachloro-m-xylene

R.T.: 3.353 min
Delta R.T.: -0.007 min
Response: 4559509
Conc: 23.19 ng/ml

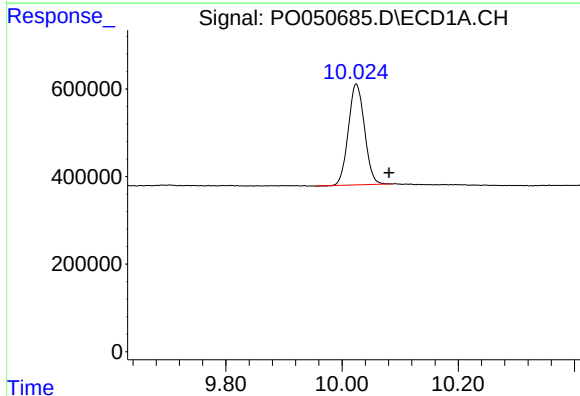

#2 Decachlorobiphenyl

R.T.: 10.025 min
Delta R.T.: -0.056 min
Response: 4447936
Conc: 20.50 ng/ml

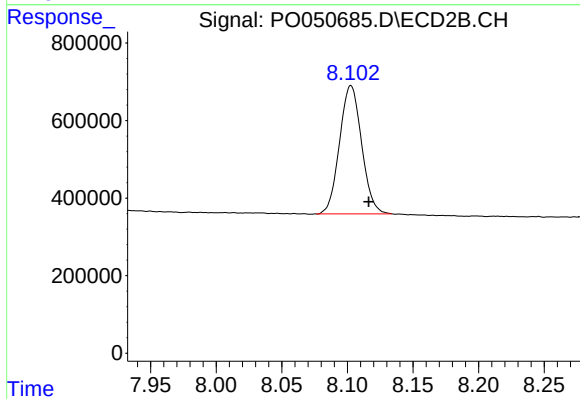

#2 Decachlorobiphenyl

R.T.: 8.103 min
Delta R.T.: -0.013 min
Response: 3881860
Conc: 20.31 ng/ml