

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102818\
 Data File : PO050712.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 28 Oct 2018 2:15
 Operator : SM/SJ
 Sample : J5688-01
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 DPC-91567-OD-01

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 29 02:31:46 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101818.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Oct 19 02:02:26 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.357	3.350	9291167	5377025	31.137	27.350
2)	SA Decachlor...	10.022	8.100	6362509	5624448	29.322	29.425

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102818\
Data File : PO050712.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 28 Oct 2018 2:15
Operator : SM/SJ
Sample : J5688-01
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
DPC-91567-OD-01

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 29 02:31:46 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101818.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Oct 19 02:02:26 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

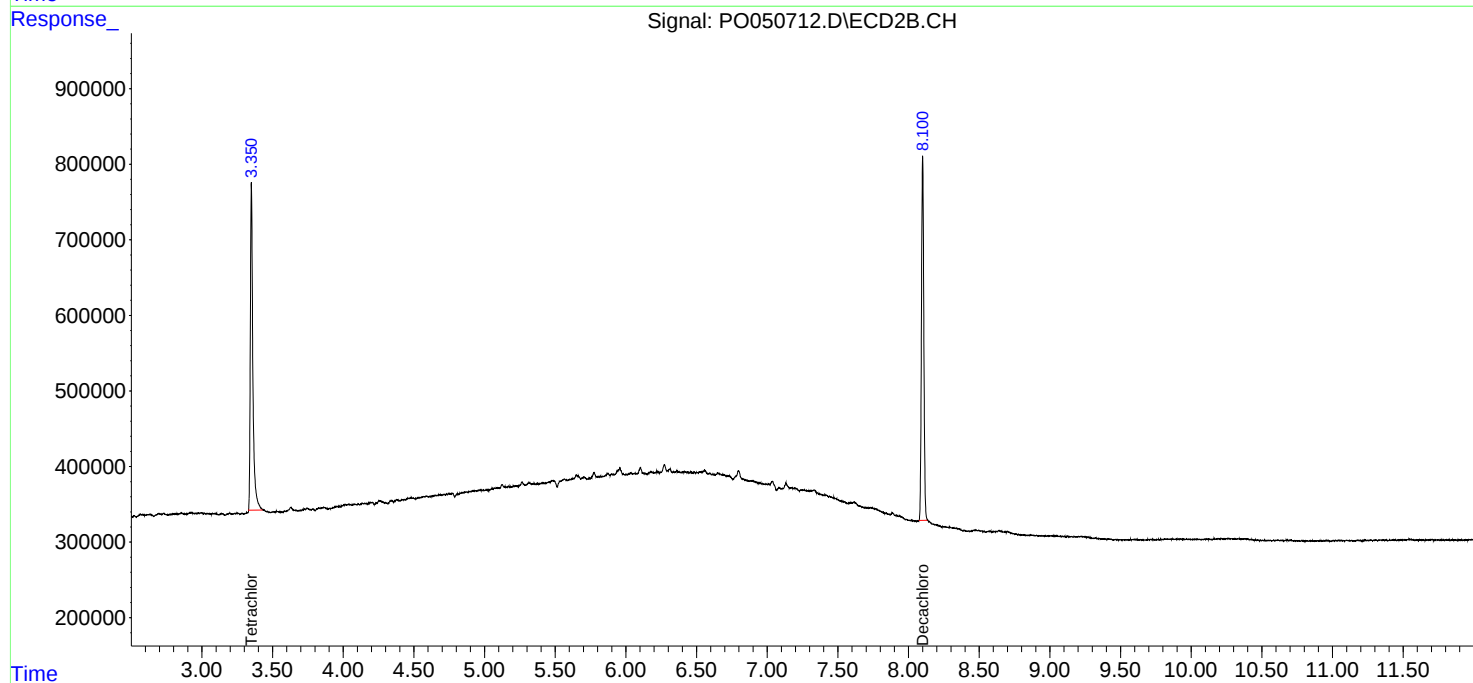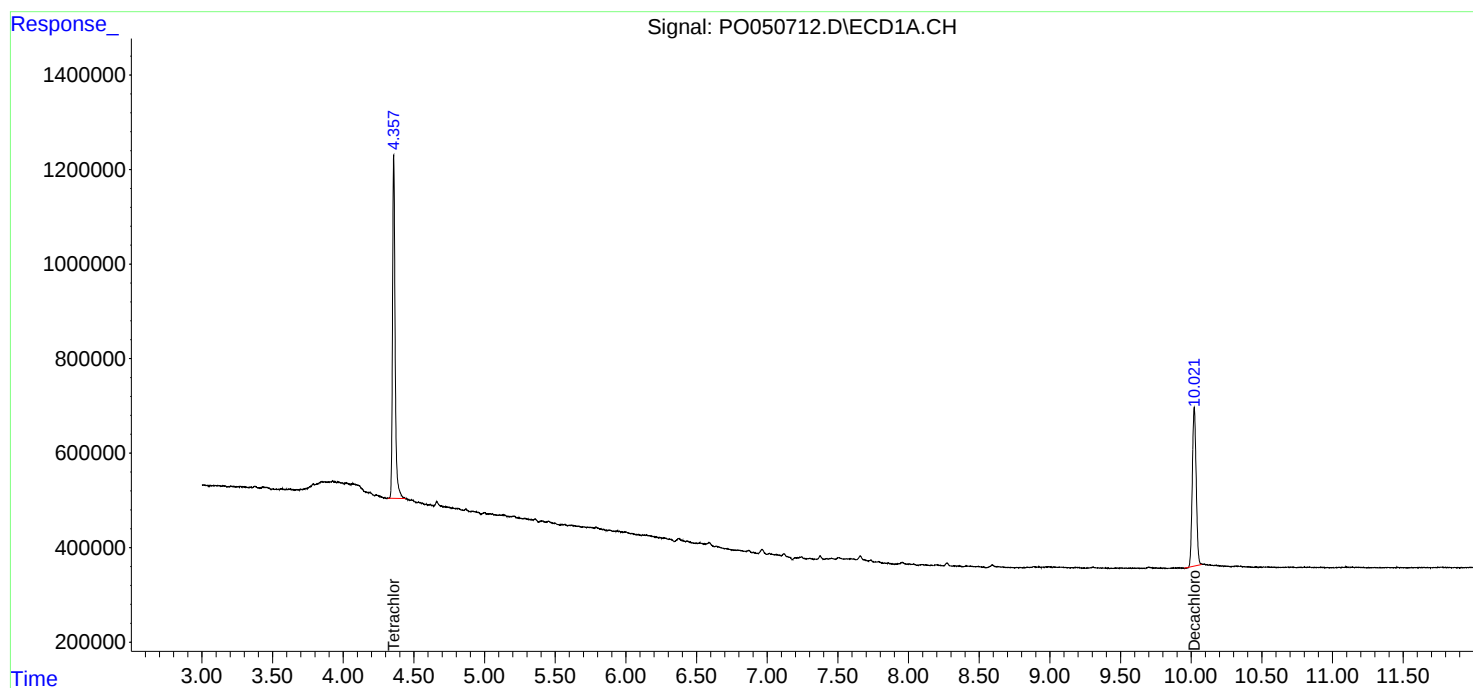


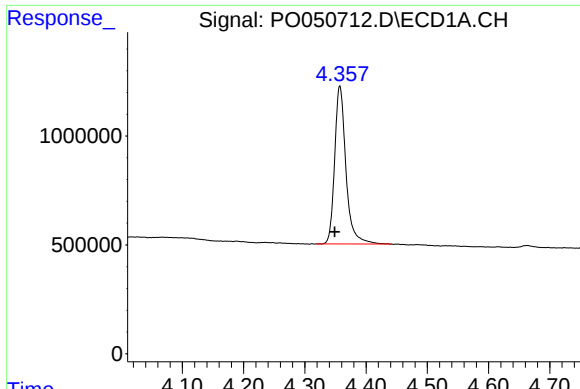

#1 Tetrachloro-m-xylene


R.T.: 4.357 min
Delta R.T.: 0.008 min
Response: 9291167
Conc: 31.14 ng/ml

Instrument :
ECD_O
ClientSampleId :
DPC-91567-OD-01

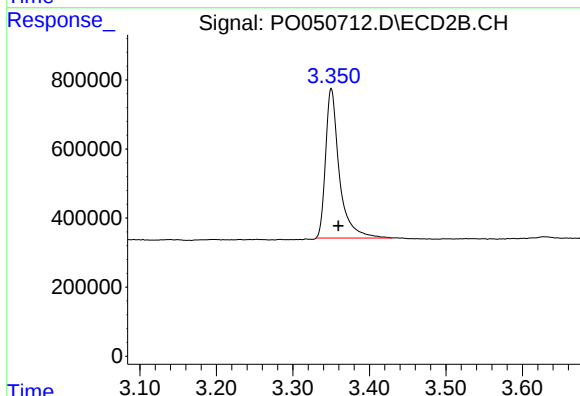


#1 Tetrachloro-m-xylene

R.T.: 3.350 min
Delta R.T.: -0.009 min
Response: 5377025
Conc: 27.35 ng/ml

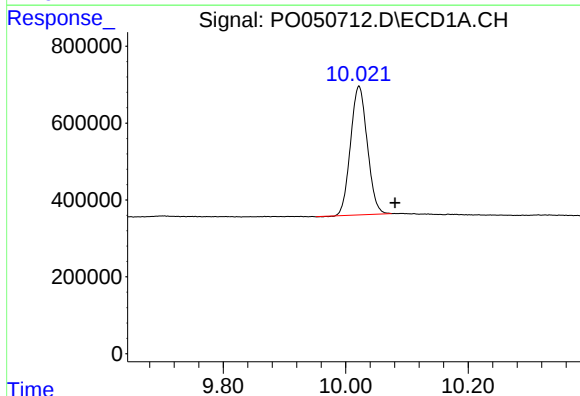

#2 Decachlorobiphenyl

R.T.: 10.022 min
Delta R.T.: -0.059 min
Response: 6362509
Conc: 29.32 ng/ml

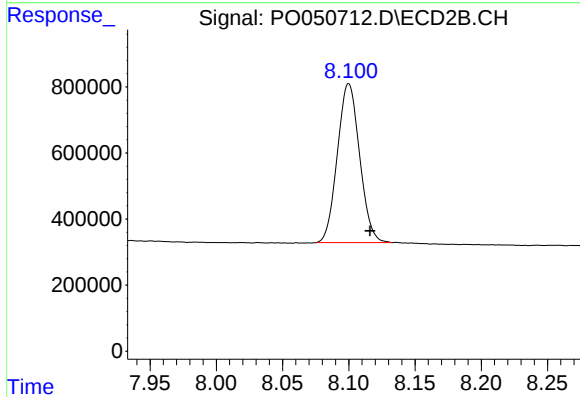

#2 Decachlorobiphenyl

R.T.: 8.100 min
Delta R.T.: -0.016 min
Response: 5624448
Conc: 29.43 ng/ml