

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102821\
 Data File : PO082284.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 28 Oct 2021 10:40
 Operator : AJ\MA
 Sample : PB140276BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PB140276BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 29 01:18:26 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Oct 19 04:37:47 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.976	3.971	1728526	654542	21.392	22.185
2)	SA Decachlor...	11.092	9.293	1346463	659953	24.226	25.911

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102821\
Data File : PO082284.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 28 Oct 2021 10:40
Operator : AJ\MA
Sample : PB140276BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
PB140276BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 29 01:18:26 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101821.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Oct 19 04:37:47 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

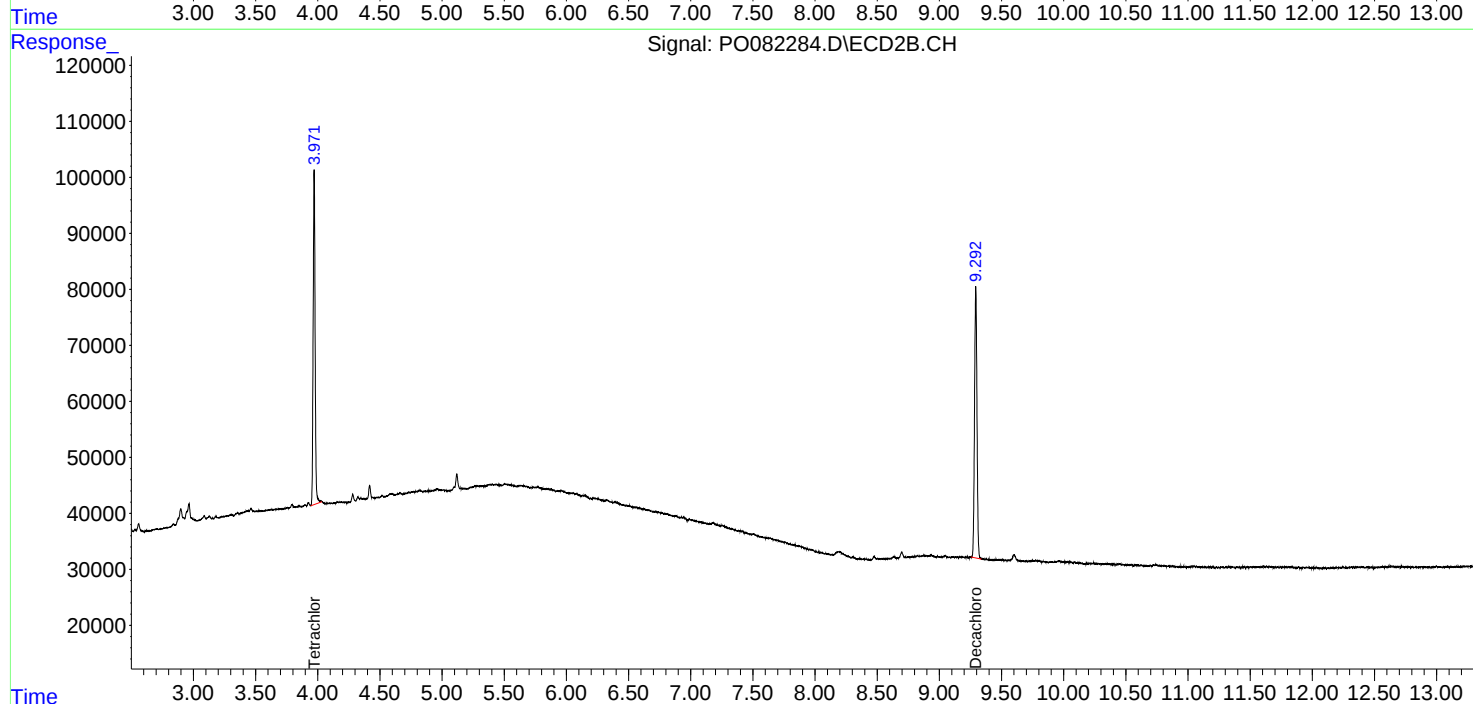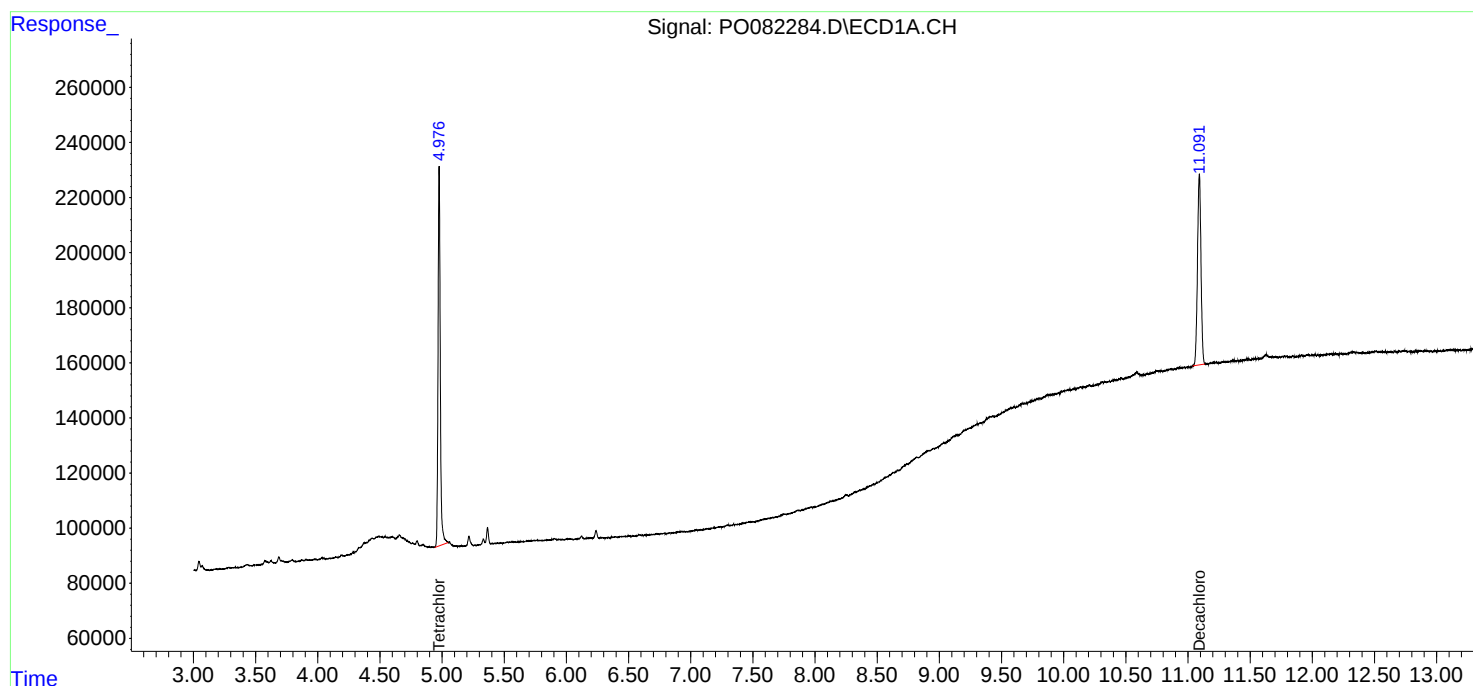


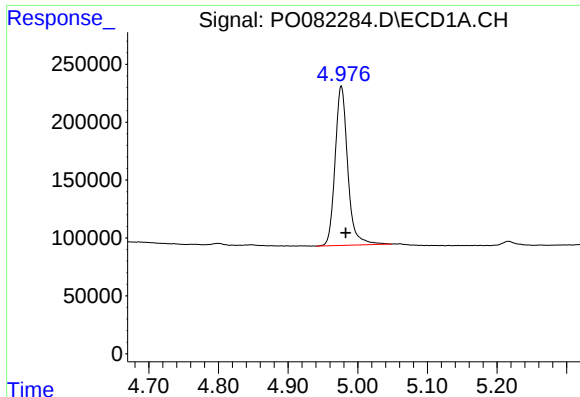

#1 Tetrachloro-m-xylene


R.T.: 4.976 min
Delta R.T.: -0.007 min
Response: 1728526
Conc: 21.39 ng/ml

Instrument :
ECD_O
ClientSampleId :
PB140276BL

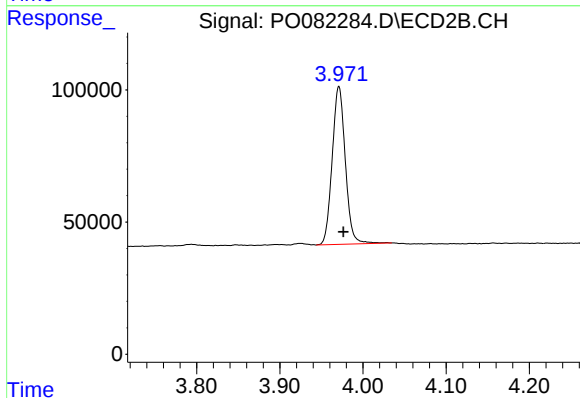


#1 Tetrachloro-m-xylene

R.T.: 3.971 min
Delta R.T.: -0.005 min
Response: 654542
Conc: 22.18 ng/ml

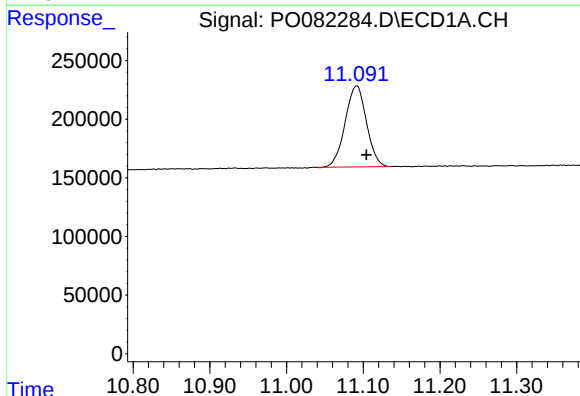

#2 Decachlorobiphenyl

R.T.: 11.092 min
Delta R.T.: -0.012 min
Response: 1346463
Conc: 24.23 ng/ml

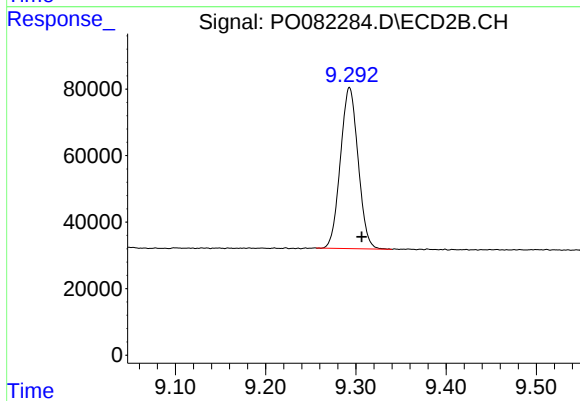

#2 Decachlorobiphenyl

R.T.: 9.293 min
Delta R.T.: -0.014 min
Response: 659953
Conc: 25.91 ng/ml