

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102821\
 Data File : PO082290.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 28 Oct 2021 12:23
 Operator : AJ\MA
 Sample : M4342-05 10X
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CLI-2021-3-B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 29 01:22:00 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Oct 19 04:37:47 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.978	3.972	108088	41861	1.338	1.419m
2) SA Decachlor...	11.101	9.295	98199	47349	1.767m	1.859m

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102821\
Data File : PO082290.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 28 Oct 2021 12:23
Operator : AJ\MA
Sample : M4342-05 10X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
CLI-2021-3-B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 29 01:22:00 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101821.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Oct 19 04:37:47 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

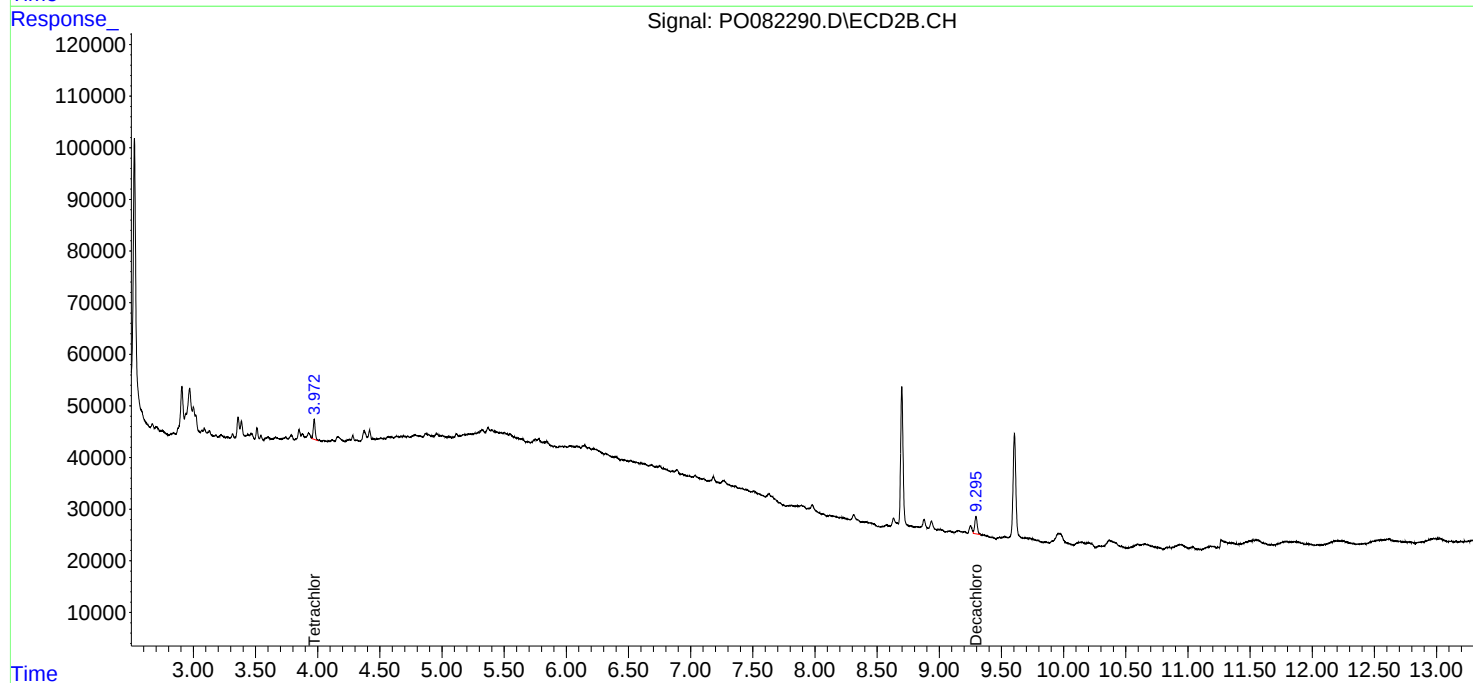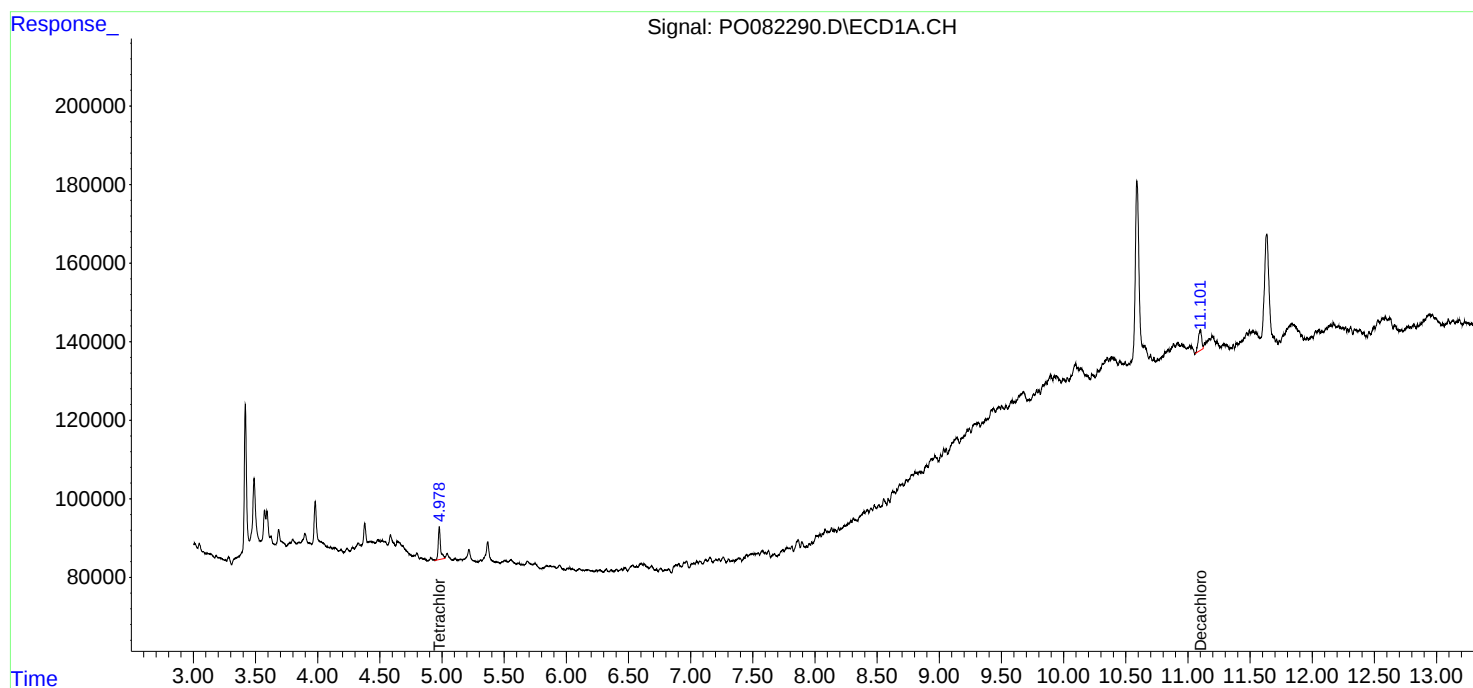


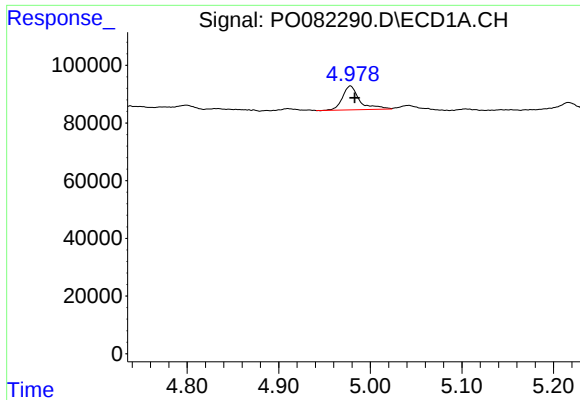

#1 Tetrachloro-m-xylene


R.T.: 4.978 min
Delta R.T.: -0.005 min
Response: 108088
Conc: 1.34 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2021-3-B

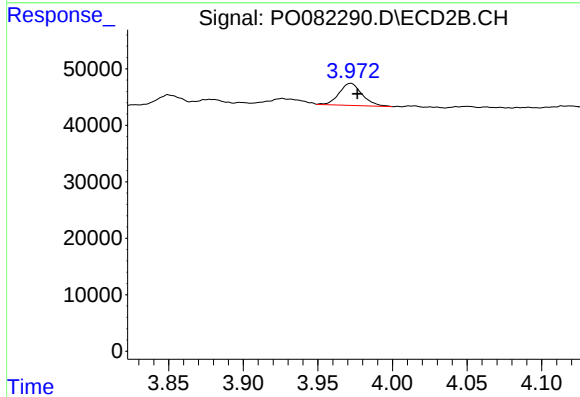


#1 Tetrachloro-m-xylene

R.T.: 3.972 min
Delta R.T.: -0.005 min
Response: 41861
Conc: 1.42 ng/ml m

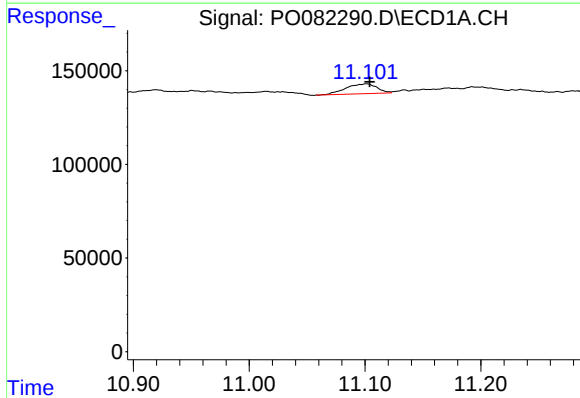

#2 Decachlorobiphenyl

R.T.: 11.101 min
Delta R.T.: -0.003 min
Response: 98199
Conc: 1.77 ng/ml m

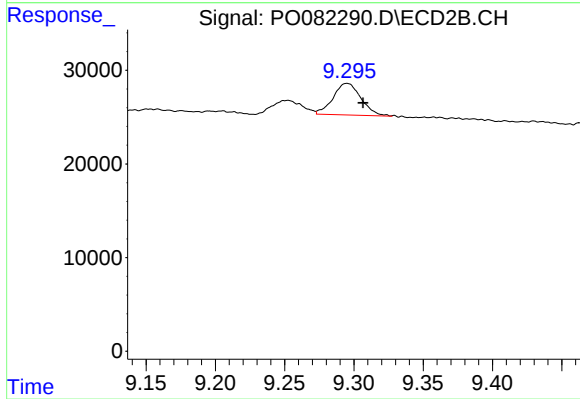

#2 Decachlorobiphenyl

R.T.: 9.295 min
Delta R.T.: -0.012 min
Response: 47349
Conc: 1.86 ng/ml m